

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031163.D
 Acq On : 22 May 2023 14:08
 Operator : SY/MD
 Sample : 02866-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	93	rVB	113923	130494	13.77%	1.684%
2	1.539	148	155	171	rVB	119194	146794	15.49%	1.894%
3	2.066	310	319	332	rBV	240831	349879	36.91%	4.514%
4	2.375	413	415	417	rBV3	1415	713	0.08%	0.009%
5	2.410	423	426	428	rBV4	1174	789	0.08%	0.010%
6	2.426	428	431	433	rBV4	2006	1316	0.14%	0.017%
7	2.561	472	473	476	rBV3	1197	733	0.08%	0.009%
8	2.838	557	559	560	rBV	1962	706	0.07%	0.009%
9	2.886	570	574	577	rBV4	2398	1665	0.18%	0.021%
10	2.909	577	581	587	rBV9	1632	2078	0.22%	0.027%
11	3.249	685	687	688	rBV2	1285	466	0.05%	0.006%
12	3.304	701	704	705	rBV2	1376	784	0.08%	0.010%
13	3.712	828	831	832	rBV4	1611	1035	0.11%	0.013%
14	3.806	850	860	883	rBV	61535	175922	18.56%	2.270%
15	4.259	986	1001	1019	rBV	164402	415173	43.80%	5.356%
16	4.597	1104	1106	1110	rVB5	1534	900	0.09%	0.012%
17	4.648	1120	1122	1124	rVB3	2091	834	0.09%	0.011%
18	4.857	1186	1187	1189	rBV2	1260	569	0.06%	0.007%
19	4.876	1191	1193	1197	rVV5	1415	896	0.09%	0.012%
20	4.966	1205	1221	1246	rBV2	360564	947884	100.00%	12.229%
21	5.375	1345	1348	1351	rBV5	1627	1143	0.12%	0.015%
22	5.542	1388	1400	1423	rBV	297741	616509	65.04%	7.954%
23	5.841	1483	1493	1514	rVB2	204224	403958	42.62%	5.212%
24	5.998	1531	1542	1560	rVB2	214362	431362	45.51%	5.565%
25	6.275	1626	1628	1630	rBV4	2007	842	0.09%	0.011%
26	6.368	1655	1657	1659	rVB3	2093	800	0.08%	0.010%
27	6.693	1756	1758	1761	rBV3	1615	1206	0.13%	0.016%
28	6.809	1792	1794	1798	rBV5	1384	906	0.10%	0.012%
29	6.854	1805	1808	1812	rBV4	2383	1955	0.21%	0.025%
30	6.921	1818	1829	1849	rBV	107539	210833	22.24%	2.720%
31	7.249	1921	1931	1948	rBV	389951	684275	72.19%	8.828%
32	7.561	2020	2028	2047	rVB	76919	134692	14.21%	1.738%
33	8.034	2166	2175	2191	rBV	194441	389764	41.12%	5.029%
34	8.680	2374	2376	2378	rVB3	1485	579	0.06%	0.007%
35	8.793	2397	2411	2436	rBV	456174	781042	82.40%	10.077%
36	8.950	2458	2460	2462	rBV3	1825	914	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031163.D
 Acq On : 22 May 2023 14:08
 Operator : SY/MD
 Sample : 02866-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.301	2567	2569	2572	rBV4	1675	892	0.09%	0.012%
38	9.317	2572	2574	2575	rBV2	1409	675	0.07%	0.009%
39	9.516	2634	2636	2637	rBV2	1285	485	0.05%	0.006%
40	9.545	2642	2645	2649	rBV5	2414	1915	0.20%	0.025%
41	9.719	2696	2699	2701	rBV4	1926	1417	0.15%	0.018%
42	9.911	2757	2759	2762	rBV4	1149	699	0.07%	0.009%
43	10.059	2802	2805	2806	rBV3	1597	754	0.08%	0.010%
44	10.159	2826	2836	2851	rBV	306660	489504	51.64%	6.315%
45	10.593	2969	2971	2974	rBV3	1430	872	0.09%	0.011%
46	10.674	2994	2996	3002	rVB6	2467	2019	0.21%	0.026%
47	11.040	3106	3110	3115	rBV7	2843	3067	0.32%	0.040%
48	11.191	3147	3157	3179	rVB	428229	686094	72.38%	8.852%
49	11.448	3233	3237	3238	rBV4	2051	1427	0.15%	0.018%
50	11.567	3263	3274	3293	rBV	421215	669090	70.59%	8.632%
51	11.712	3317	3319	3324	rBV5	1845	1484	0.16%	0.019%
52	12.043	3418	3422	3423	rBV4	1169	748	0.08%	0.010%
53	12.095	3434	3438	3439	rBV4	1838	1185	0.13%	0.015%
54	12.223	3474	3478	3480	rBV5	1064	883	0.09%	0.011%
55	12.255	3485	3488	3489	rBV3	2580	1504	0.16%	0.019%
56	12.278	3493	3495	3499	rVV5	1008	784	0.08%	0.010%
57	12.304	3501	3503	3507	rVB4	1790	1147	0.12%	0.015%
58	12.355	3516	3519	3522	rBV4	1437	1348	0.14%	0.017%
59	12.490	3558	3561	3562	rBV3	1870	1034	0.11%	0.013%
60	12.532	3571	3574	3577	rBV4	1282	794	0.08%	0.010%
61	12.548	3577	3579	3583	rVV4	1685	1120	0.12%	0.014%
62	12.596	3592	3594	3595	rBV2	1300	474	0.05%	0.006%
63	12.628	3601	3604	3605	rBV3	1070	542	0.06%	0.007%
64	12.661	3612	3614	3617	rBV3	1174	652	0.07%	0.008%
65	12.728	3633	3635	3638	rBV5	824	552	0.06%	0.007%
66	12.808	3658	3660	3665	rBV5	1884	1951	0.21%	0.025%
67	12.847	3670	3672	3673	rBV2	1329	480	0.05%	0.006%
68	12.911	3689	3692	3694	rBV3	785	604	0.06%	0.008%
69	12.963	3701	3708	3710	rBV8	1612	1257	0.13%	0.016%
70	13.072	3740	3742	3745	rVB4	1386	606	0.06%	0.008%
71	13.088	3745	3747	3750	rVB4	1293	577	0.06%	0.007%
72	13.124	3755	3758	3760	rBV4	1447	807	0.09%	0.010%
73	13.153	3760	3767	3770	rBV7	1749	2188	0.23%	0.028%
74	13.233	3790	3792	3795	rVB4	1947	1056	0.11%	0.014%
75	13.249	3795	3797	3799	rVB3	1150	462	0.05%	0.006%
76	13.265	3799	3802	3807	rBV7	1751	1976	0.21%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031163.D
 Acq On : 22 May 2023 14:08
 Operator : SY/MD
 Sample : 02866-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	13.291	3808	3810	3814	rBV5	1131	813	0.09%	0.010%
78	13.329	3819	3822	3824	rBV3	1221	698	0.07%	0.009%
79	13.400	3840	3844	3846	rBV5	1265	1111	0.12%	0.014%
80	13.455	3858	3861	3863	rVV3	1083	726	0.08%	0.009%
81	13.471	3863	3866	3869	rVB5	2399	1594	0.17%	0.021%
82	13.497	3869	3874	3875	rBV5	1967	1528	0.16%	0.020%
83	13.545	3886	3889	3893	rBV6	1824	1412	0.15%	0.018%
84	13.564	3893	3895	3898	rVV3	1395	675	0.07%	0.009%
85	13.599	3904	3906	3908	rBV3	1242	640	0.07%	0.008%
86	13.725	3943	3945	3948	rVB3	1438	734	0.08%	0.009%
87	13.741	3948	3950	3952	rBV2	1093	465	0.05%	0.006%
88	13.757	3952	3955	3959	rBV5	1613	1348	0.14%	0.017%
89	13.821	3969	3975	3979	rBV8	2374	2703	0.29%	0.035%
90	13.866	3986	3989	3994	rVV6	1312	1347	0.14%	0.017%
91	13.898	3996	3999	4001	rBV4	1471	1021	0.11%	0.013%
92	13.937	4009	4011	4012	rBV2	1329	679	0.07%	0.009%
93	13.992	4022	4028	4029	rBV5	1671	1310	0.14%	0.017%
94	14.117	4065	4067	4071	rVB4	1571	821	0.09%	0.011%
95	14.204	4091	4094	4097	rBV5	1651	1213	0.13%	0.016%
96	14.268	4111	4114	4116	rBV4	2339	961	0.10%	0.012%
97	14.333	4131	4134	4137	rBV4	1599	1122	0.12%	0.014%
98	14.451	4168	4171	4173	rBV3	1515	1031	0.11%	0.013%
99	14.564	4203	4206	4207	rBV2	1876	826	0.09%	0.011%
100	14.574	4207	4209	4211	rVB3	1665	635	0.07%	0.008%




Sum of corrected areas: 7750948

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031163.D
Acq On : 22 May 2023 14:08
Operator : SY/MD
Sample : 02866-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

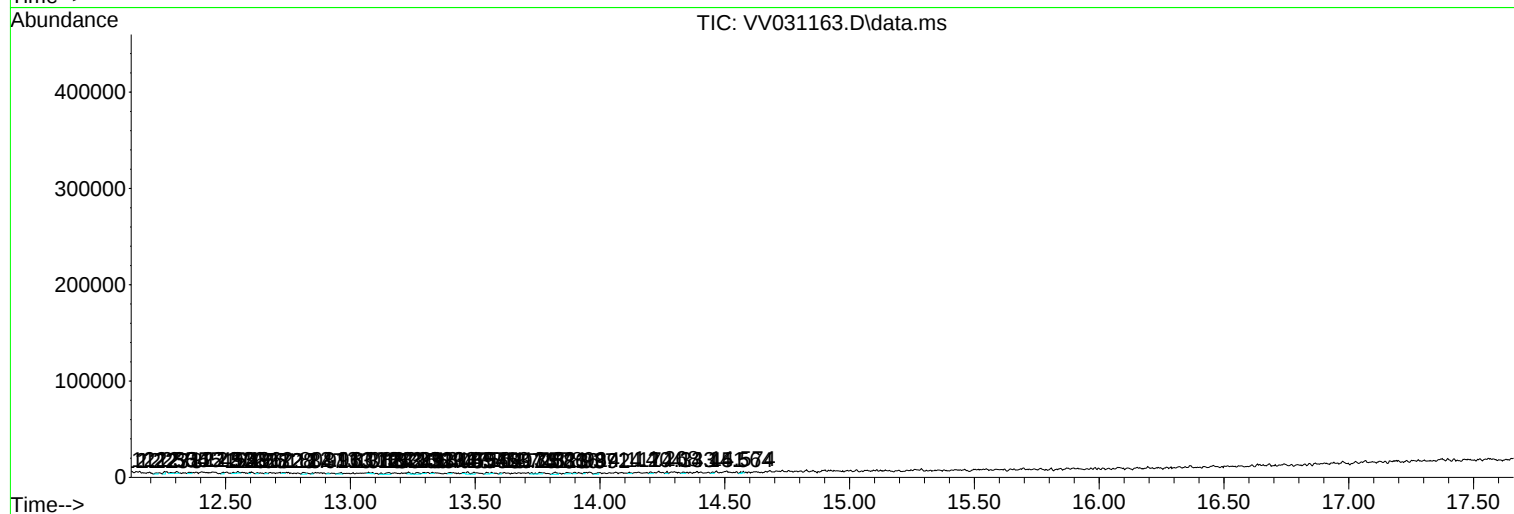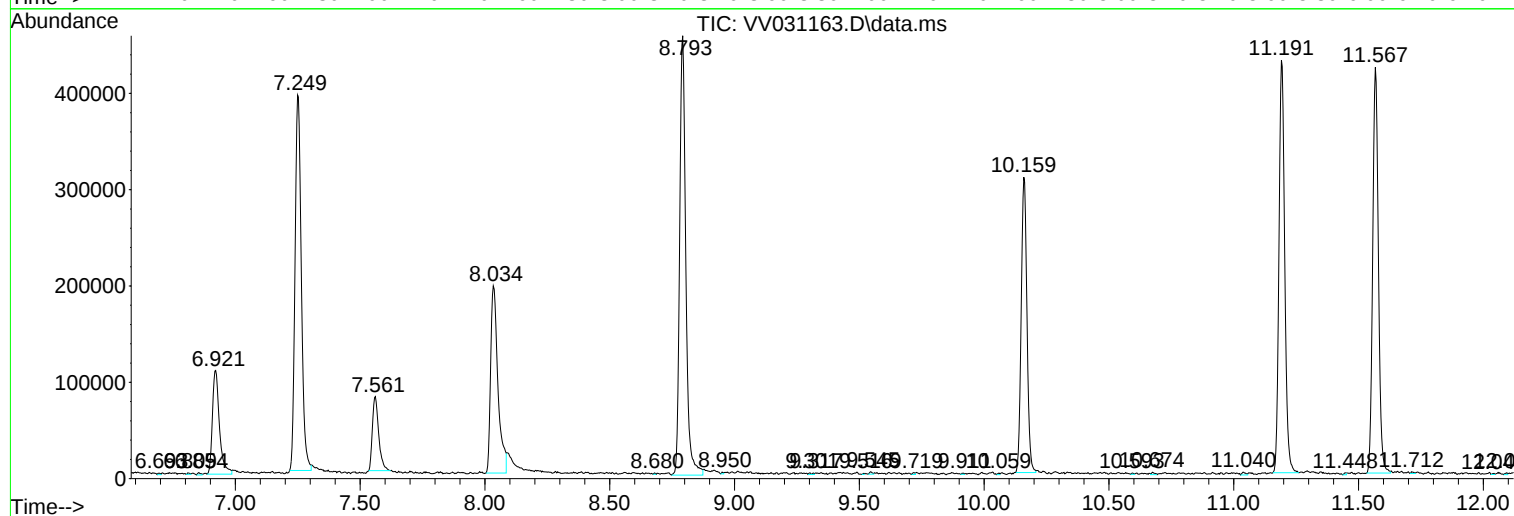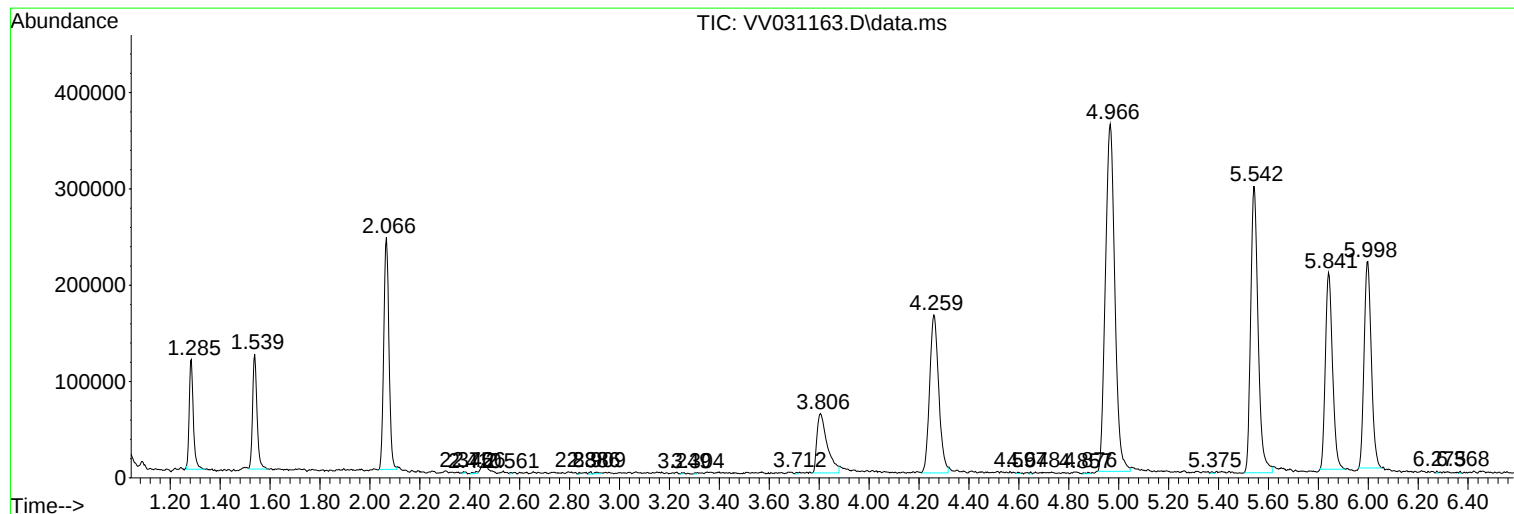

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031163.D
Acq On : 22 May 2023 14:08
Operator : SY/MD
Sample : 02866-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031163.D
Acq On : 22 May 2023 14:08
Operator : SY/MD
Sample : 02866-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------