

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031164.D
 Acq On : 22 May 2023 14:32
 Operator : SY/MD
 Sample : 02866-16DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	111332	123797	13.86%	1.686%
2	1.535	148	154	168	rVB	114654	139379	15.60%	1.898%
3	2.063	309	318	333	rBV	225371	329789	36.92%	4.491%
4	2.603	480	486	489	rBV6	1991	1888	0.21%	0.026%
5	2.883	571	573	577	rBV5	2665	1747	0.20%	0.024%
6	3.018	612	615	616	rBV3	1461	797	0.09%	0.011%
7	3.188	664	668	670	rBV5	1344	1166	0.13%	0.016%
8	3.220	673	678	680	rBV6	2325	2255	0.25%	0.031%
9	3.236	682	683	688	rVB5	1873	1352	0.15%	0.018%
10	3.314	704	707	708	rBV2	1187	773	0.09%	0.011%
11	3.439	743	746	748	rBV4	1621	816	0.09%	0.011%
12	3.490	757	762	767	rVB8	2487	2186	0.24%	0.030%
13	3.542	770	778	782	rBV9	2447	2759	0.31%	0.038%
14	3.722	831	834	836	rBV3	1793	722	0.08%	0.010%
15	3.805	850	860	885	rBV	61451	188070	21.05%	2.561%
16	4.191	977	980	982	rBV4	1379	943	0.11%	0.013%
17	4.259	989	1001	1020	rVB	147341	368483	41.25%	5.018%
18	4.510	1077	1079	1082	rBV4	1653	1013	0.11%	0.014%
19	4.619	1109	1113	1115	rBV5	1622	1203	0.13%	0.016%
20	4.641	1118	1120	1124	rBV4	968	673	0.08%	0.009%
21	4.728	1144	1147	1149	rBV4	1292	859	0.10%	0.012%
22	4.828	1176	1178	1181	rBV4	1079	708	0.08%	0.010%
23	4.847	1181	1184	1187	rBV4	1706	1406	0.16%	0.019%
24	4.873	1191	1192	1196	rBV3	1488	963	0.11%	0.013%
25	4.966	1205	1221	1249	rBV2	333888	893355	100.00%	12.165%
26	5.227	1300	1302	1306	rVB5	1957	837	0.09%	0.011%
27	5.400	1351	1356	1363	rBV9	2190	2916	0.33%	0.040%
28	5.542	1388	1400	1426	rBV	292504	611061	68.40%	8.321%
29	5.841	1482	1493	1513	rVB	119399	240573	26.93%	3.276%
30	5.995	1530	1541	1558	rBV	204411	414648	46.41%	5.646%
31	6.465	1684	1687	1688	rBV3	1245	847	0.09%	0.012%
32	6.587	1723	1725	1730	rBV5	1714	1312	0.15%	0.018%
33	6.674	1749	1752	1754	rBV4	1385	822	0.09%	0.011%
34	6.699	1759	1760	1763	rBV3	1509	1017	0.11%	0.014%
35	6.780	1781	1785	1787	rBV5	1766	1399	0.16%	0.019%
36	6.921	1820	1829	1849	rVB	99345	182138	20.39%	2.480%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031164.D
 Acq On : 22 May 2023 14:32
 Operator : SY/MD
 Sample : 02866-16DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.249	1920	1931	1950	rBV	364384	654161	73.23%	8.908%
38	7.561	2019	2028	2049	rBV	74613	140720	15.75%	1.916%
39	7.837	2111	2114	2117	rBV5	1743	749	0.08%	0.010%
40	7.860	2117	2121	2124	rBV5	2445	1886	0.21%	0.026%
41	7.963	2151	2153	2156	rBV4	1348	643	0.07%	0.009%
42	8.034	2164	2175	2190	rBV	189789	368892	41.29%	5.023%
43	8.352	2272	2274	2276	rBV3	2007	824	0.09%	0.011%
44	8.474	2308	2312	2315	rBV5	2077	1867	0.21%	0.025%
45	8.493	2315	2318	2319	rBV2	2174	1133	0.13%	0.015%
46	8.526	2326	2328	2331	rBV3	1670	828	0.09%	0.011%
47	8.583	2342	2346	2348	rBV4	1824	1356	0.15%	0.018%
48	8.731	2388	2392	2393	rBV4	2192	1434	0.16%	0.020%
49	8.792	2398	2411	2438	rBV	456031	775177	86.77%	10.556%
50	9.329	2576	2578	2582	rBV5	1437	1389	0.16%	0.019%
51	9.361	2586	2588	2591	rVV4	1403	646	0.07%	0.009%
52	9.461	2617	2619	2622	rBV5	1681	1314	0.15%	0.018%
53	9.577	2653	2655	2658	rBV4	1476	1120	0.13%	0.015%
54	9.699	2691	2693	2694	rBV2	1694	755	0.08%	0.010%
55	9.763	2710	2713	2714	rBV3	1782	873	0.10%	0.012%
56	9.921	2759	2762	2763	rBV4	1112	676	0.08%	0.009%
57	9.966	2772	2776	2781	rVB8	2119	2054	0.23%	0.028%
58	9.988	2781	2783	2784	rBV2	1617	657	0.07%	0.009%
59	10.159	2824	2836	2854	rBV	294539	477323	53.43%	6.500%
60	10.275	2869	2872	2875	rBV4	1732	1162	0.13%	0.016%
61	10.406	2910	2913	2915	rBV4	1799	1315	0.15%	0.018%
62	10.496	2939	2941	2944	rBV3	907	723	0.08%	0.010%
63	10.635	2980	2984	2990	rBV8	2118	2252	0.25%	0.031%
64	10.667	2990	2994	2996	rBV4	1849	1280	0.14%	0.017%
65	10.693	3000	3002	3004	rBV3	1977	1031	0.12%	0.014%
66	10.757	3018	3022	3024	rBV4	2042	1747	0.20%	0.024%
67	10.789	3029	3032	3033	rBV4	1753	928	0.10%	0.013%
68	10.918	3064	3072	3075	rBV10	2121	2932	0.33%	0.040%
69	10.998	3094	3097	3101	rBV6	1461	1003	0.11%	0.014%
70	11.098	3124	3128	3130	rBV5	2848	1769	0.20%	0.024%
71	11.191	3146	3157	3176	rBV	432484	690553	77.30%	9.404%
72	11.365	3208	3211	3213	rBV4	2046	1566	0.18%	0.021%
73	11.567	3262	3274	3291	rBV	395110	638892	71.52%	8.700%
74	11.802	3345	3347	3350	rBV4	1295	747	0.08%	0.010%
75	11.818	3350	3352	3357	rVB6	1760	1358	0.15%	0.018%
76	11.844	3357	3360	3364	rBV5	1555	1464	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031164.D
 Acq On : 22 May 2023 14:32
 Operator : SY/MD
 Sample : 02866-16DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.918	3381	3383	3385	rBV3	1340	804	0.09%	0.011%
78	12.239	3480	3483	3485	rBV4	1687	1187	0.13%	0.016%
79	12.320	3505	3508	3511	rVB4	1486	888	0.10%	0.012%
80	12.358	3517	3520	3522	rBV3	2161	1199	0.13%	0.016%
81	12.371	3522	3524	3528	rVV5	1667	1309	0.15%	0.018%
82	12.593	3590	3593	3598	rBV6	3579	3040	0.34%	0.041%
83	12.664	3612	3615	3617	rBV3	1388	872	0.10%	0.012%
84	12.696	3622	3625	3626	rBV3	1585	971	0.11%	0.013%
85	12.747	3637	3641	3646	rBV6	1725	1476	0.17%	0.020%
86	13.178	3773	3775	3779	rBV5	1283	847	0.09%	0.012%
87	13.207	3782	3784	3787	rBV4	1624	1045	0.12%	0.014%
88	13.329	3818	3822	3826	rVB6	2141	1966	0.22%	0.027%
89	13.352	3826	3829	3830	rBV3	2026	994	0.11%	0.014%
90	13.397	3840	3843	3846	rBV5	1692	1491	0.17%	0.020%
91	13.532	3883	3885	3889	rBV5	1226	777	0.09%	0.011%
92	13.580	3898	3900	3903	rVB4	1650	968	0.11%	0.013%
93	13.602	3903	3907	3909	rBV5	1556	1128	0.13%	0.015%
94	13.686	3931	3933	3934	rBV2	1928	649	0.07%	0.009%
95	13.750	3947	3953	3955	rBV6	1826	2200	0.25%	0.030%
96	13.789	3963	3965	3966	rBV2	1503	675	0.08%	0.009%
97	13.979	4021	4024	4026	rBV4	2726	1686	0.19%	0.023%
98	14.339	4129	4136	4137	rBV7	2570	3040	0.34%	0.041%
99	14.458	4171	4173	4176	rBV4	1827	1098	0.12%	0.015%
100	14.554	4200	4203	4204	rBV3	2185	1311	0.15%	0.018%




Sum of corrected areas: 7343492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031164.D
Acq On : 22 May 2023 14:32
Operator : SY/MD
Sample : 02866-16DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

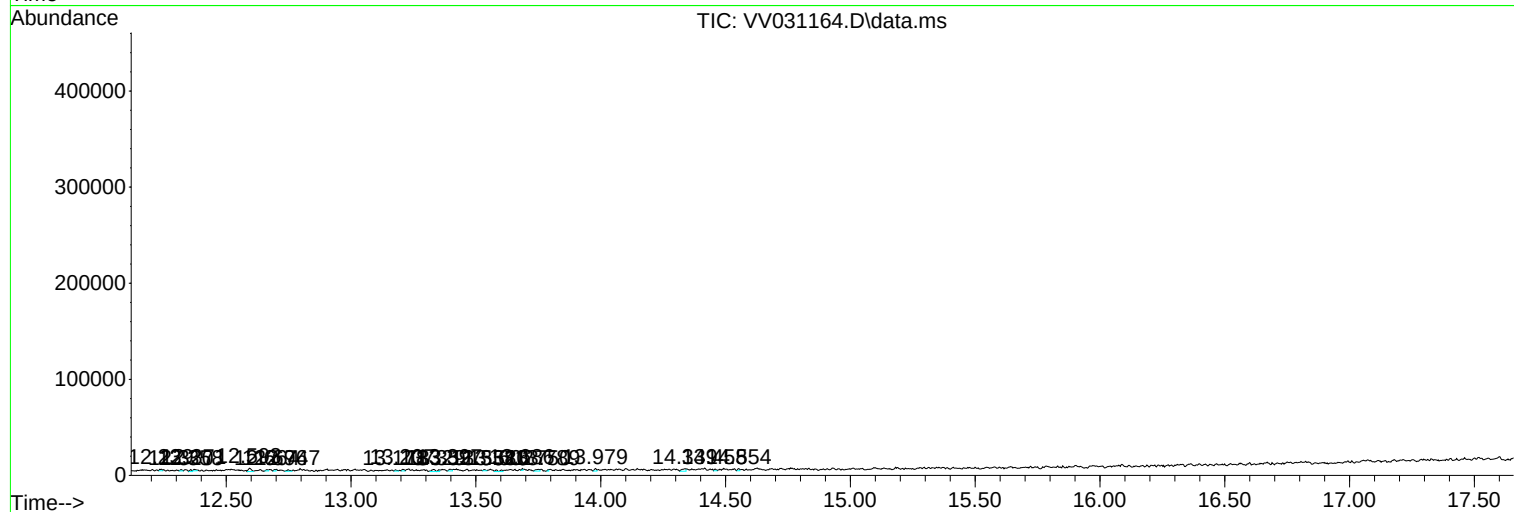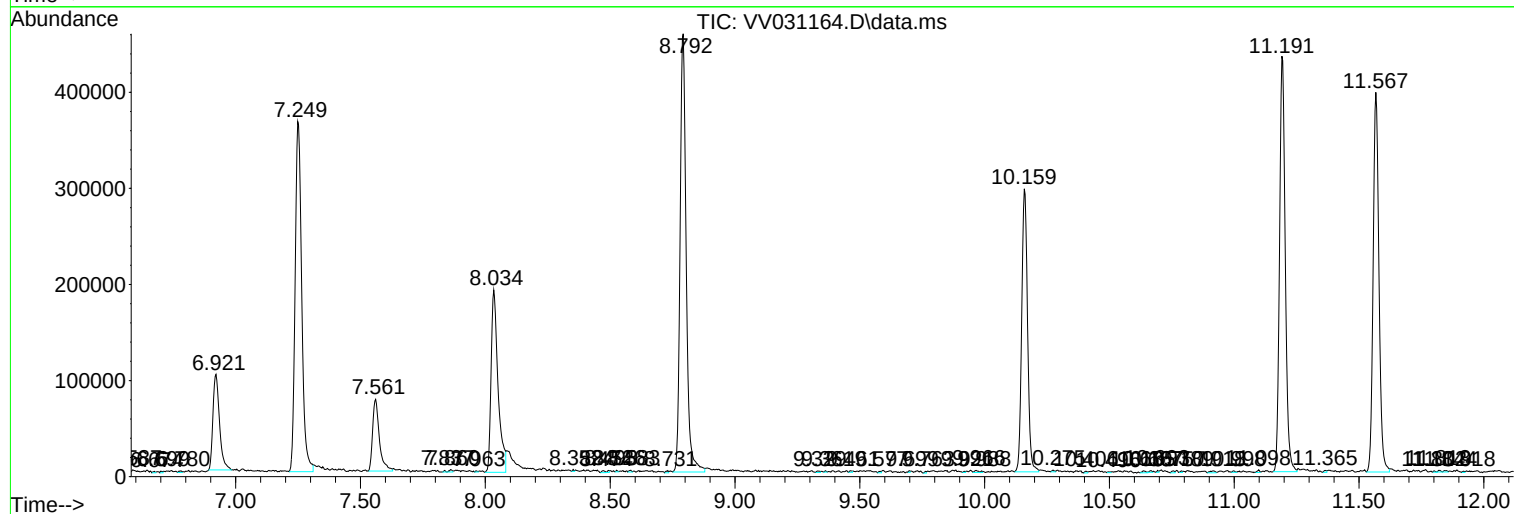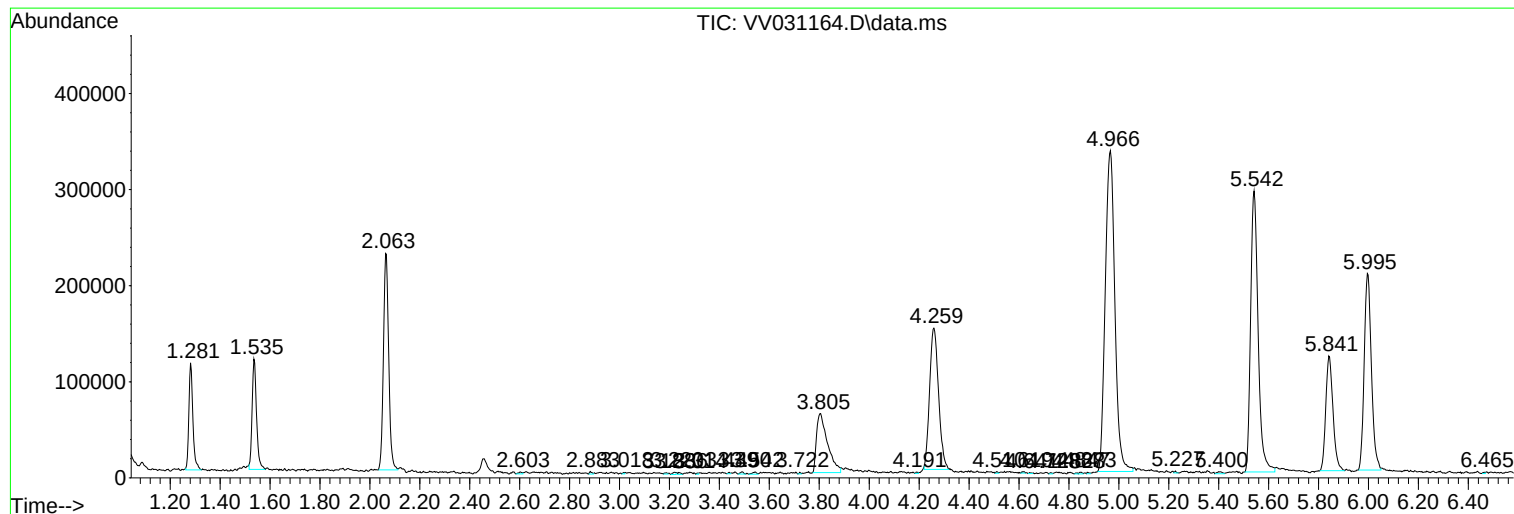

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031164.D
Acq On : 22 May 2023 14:32
Operator : SY/MD
Sample : 02866-16DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031164.D
Acq On : 22 May 2023 14:32
Operator : SY/MD
Sample : 02866-16DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------