

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031166.D
 Acq On : 22 May 2023 15:19
 Operator : SY/MD
 Sample : 02866-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rBV	100764	112008	12.99%	1.575%
2	1.535	148	154	169	rVB	96044	118936	13.79%	1.672%
3	2.066	310	319	333	rVB	210953	306377	35.52%	4.308%
4	2.407	421	425	427	rBV5	1515	1546	0.18%	0.022%
5	2.455	433	440	447	rBV3	12046	18210	2.11%	0.256%
6	2.516	457	459	461	rVB3	1569	637	0.07%	0.009%
7	2.783	540	542	544	rBV3	1677	952	0.11%	0.013%
8	2.822	551	554	558	rVB5	1916	1721	0.20%	0.024%
9	2.905	577	580	582	rBV4	1772	856	0.10%	0.012%
10	2.918	582	584	586	rVB3	1432	606	0.07%	0.009%
11	3.037	617	621	623	rBV5	1381	1048	0.12%	0.015%
12	3.146	651	655	656	rBV4	1404	868	0.10%	0.012%
13	3.442	745	747	749	rBV3	1659	931	0.11%	0.013%
14	3.481	757	759	762	rVB4	2067	1047	0.12%	0.015%
15	3.500	762	765	766	rBV2	1277	702	0.08%	0.010%
16	3.523	770	772	773	rBV2	821	370	0.04%	0.005%
17	3.587	787	792	795	rBV7	1325	1350	0.16%	0.019%
18	3.658	813	814	817	rBV3	1375	907	0.11%	0.013%
19	3.732	834	837	840	rBV5	1035	684	0.08%	0.010%
20	3.799	849	858	891	rBV	57674	180766	20.96%	2.542%
21	4.259	988	1001	1024	rVB2	144213	363285	42.12%	5.109%
22	4.725	1144	1146	1149	rBV4	1441	734	0.09%	0.010%
23	4.966	1203	1221	1247	rBV2	324946	862567	100.00%	12.129%
24	5.172	1283	1285	1287	rBV2	2222	882	0.10%	0.012%
25	5.375	1345	1348	1350	rBV3	1737	1110	0.13%	0.016%
26	5.542	1389	1400	1418	rBV	286224	586472	67.99%	8.247%
27	5.841	1482	1493	1512	rBV	250941	494062	57.28%	6.948%
28	5.998	1531	1542	1569	rVB	194908	405184	46.97%	5.698%
29	6.362	1653	1655	1657	rBV3	1960	798	0.09%	0.011%
30	6.503	1696	1699	1701	rBV4	2242	1444	0.17%	0.020%
31	6.629	1736	1738	1742	rBV4	2560	2146	0.25%	0.030%
32	6.706	1760	1762	1763	rBV2	1508	764	0.09%	0.011%
33	6.754	1772	1777	1781	rBV7	2144	2540	0.29%	0.036%
34	6.818	1793	1797	1801	rBV6	1686	1517	0.18%	0.021%
35	6.921	1818	1829	1847	rBV	93027	180091	20.88%	2.532%
36	7.252	1921	1932	1951	rBV	344508	615168	71.32%	8.651%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031166.D
 Acq On : 22 May 2023 15:19
 Operator : SY/MD
 Sample : 02866-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.561	2020	2028	2041	rBV	68544	117839	13.66%	1.657%
38	8.034	2166	2175	2207	rBV	182345	384048	44.52%	5.400%
39	8.448	2302	2304	2306	rBV3	1774	802	0.09%	0.011%
40	8.526	2325	2328	2333	rVB6	1966	1544	0.18%	0.022%
41	8.548	2333	2335	2337	rBV3	1475	581	0.07%	0.008%
42	8.567	2337	2341	2343	rBV5	1791	1200	0.14%	0.017%
43	8.583	2343	2346	2348	rBV4	1944	1278	0.15%	0.018%
44	8.622	2355	2358	2359	rBV3	1118	567	0.07%	0.008%
45	8.792	2400	2411	2435	rBV	397012	654205	75.84%	9.199%
46	9.005	2474	2477	2479	rBV4	946	575	0.07%	0.008%
47	9.111	2508	2510	2513	rVB4	1481	765	0.09%	0.011%
48	9.198	2534	2537	2543	rBV8	1717	1590	0.18%	0.022%
49	9.336	2576	2580	2583	rBV6	1452	1219	0.14%	0.017%
50	9.381	2592	2594	2597	rBB3	1541	821	0.10%	0.012%
51	9.419	2602	2606	2609	rBV5	2150	1989	0.23%	0.028%
52	9.493	2626	2629	2630	rBV4	2466	1046	0.12%	0.015%
53	9.686	2687	2689	2692	rBV4	1713	987	0.11%	0.014%
54	9.751	2707	2709	2711	rBV3	1399	837	0.10%	0.012%
55	9.783	2715	2719	2723	rBV7	2118	2351	0.27%	0.033%
56	9.834	2732	2735	2737	rVB4	2131	1314	0.15%	0.018%
57	9.847	2737	2739	2740	rBV2	1499	519	0.06%	0.007%
58	9.857	2740	2742	2745	rVV4	759	462	0.05%	0.006%
59	9.937	2763	2767	2771	rVB7	1598	1280	0.15%	0.018%
60	9.960	2771	2774	2775	rBV2	1027	431	0.05%	0.006%
61	9.992	2782	2784	2787	rBV3	1118	671	0.08%	0.009%
62	10.014	2787	2791	2792	rBV3	746	592	0.07%	0.008%
63	10.107	2817	2820	2823	rBV5	1410	1248	0.14%	0.018%
64	10.159	2826	2836	2849	rVV	237589	368110	42.68%	5.176%
65	10.275	2870	2872	2874	rBV3	1536	890	0.10%	0.013%
66	10.381	2902	2905	2911	rVB8	1933	1549	0.18%	0.022%
67	10.410	2911	2914	2916	rBV3	1304	798	0.09%	0.011%
68	10.423	2916	2918	2919	rBV2	936	374	0.04%	0.005%
69	10.471	2932	2933	2934	rBV	1082	335	0.04%	0.005%
70	10.593	2969	2971	2975	rBV4	1826	1088	0.13%	0.015%
71	10.622	2978	2980	2983	rBV5	1728	900	0.10%	0.013%
72	10.657	2988	2991	2992	rBV3	1068	531	0.06%	0.007%
73	10.728	3011	3013	3014	rBV2	1016	482	0.06%	0.007%
74	10.783	3029	3030	3035	rBV4	803	571	0.07%	0.008%
75	10.821	3040	3042	3045	rBV4	745	508	0.06%	0.007%
76	10.837	3045	3047	3049	rBV3	1046	483	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031166.D
 Acq On : 22 May 2023 15:19
 Operator : SY/MD
 Sample : 02866-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX79DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	10.889	3060	3063	3064	rBV3	1062	555	0.06%	0.008%
78	10.972	3087	3089	3090	rBV2	1757	584	0.07%	0.008%
79	11.191	3147	3157	3178	rBV	417310	658900	76.39%	9.265%
80	11.451	3236	3238	3241	rBV4	1508	858	0.10%	0.012%
81	11.529	3258	3262	3263	rBV4	2035	1352	0.16%	0.019%
82	11.567	3263	3274	3290	rVV	371642	601459	69.73%	8.458%
83	11.802	3343	3347	3348	rBV5	1838	1247	0.14%	0.018%
84	11.876	3368	3370	3372	rBV3	1237	625	0.07%	0.009%
85	11.918	3377	3383	3389	rBV3	2502	3247	0.38%	0.046%
86	12.133	3447	3450	3453	rVB4	1659	1209	0.14%	0.017%
87	12.294	3496	3500	3503	rBV6	1830	1465	0.17%	0.021%
88	12.394	3529	3531	3532	rBV2	1024	357	0.04%	0.005%
89	12.480	3557	3558	3560	rBV2	1017	332	0.04%	0.005%
90	12.574	3585	3587	3588	rBV2	1409	552	0.06%	0.008%
91	12.869	3677	3679	3681	rBV3	1215	547	0.06%	0.008%
92	13.030	3727	3729	3730	rBV2	1027	435	0.05%	0.006%
93	13.175	3770	3774	3777	rVB7	1568	1445	0.17%	0.020%
94	13.374	3834	3836	3838	rBV3	1517	663	0.08%	0.009%
95	13.455	3857	3861	3864	rBV5	2466	2045	0.24%	0.029%
96	13.606	3904	3908	3911	rBV6	1905	1899	0.22%	0.027%
97	13.660	3921	3925	3926	rBV4	1540	1154	0.13%	0.016%
98	13.712	3939	3941	3942	rBV2	1013	466	0.05%	0.007%
99	13.992	4025	4028	4031	rBV5	1648	1452	0.17%	0.020%
100	14.342	4134	4137	4141	rBV5	2054	1833	0.21%	0.026%




Sum of corrected areas: 7111347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031166.D
Acq On : 22 May 2023 15:19
Operator : SY/MD
Sample : 02866-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

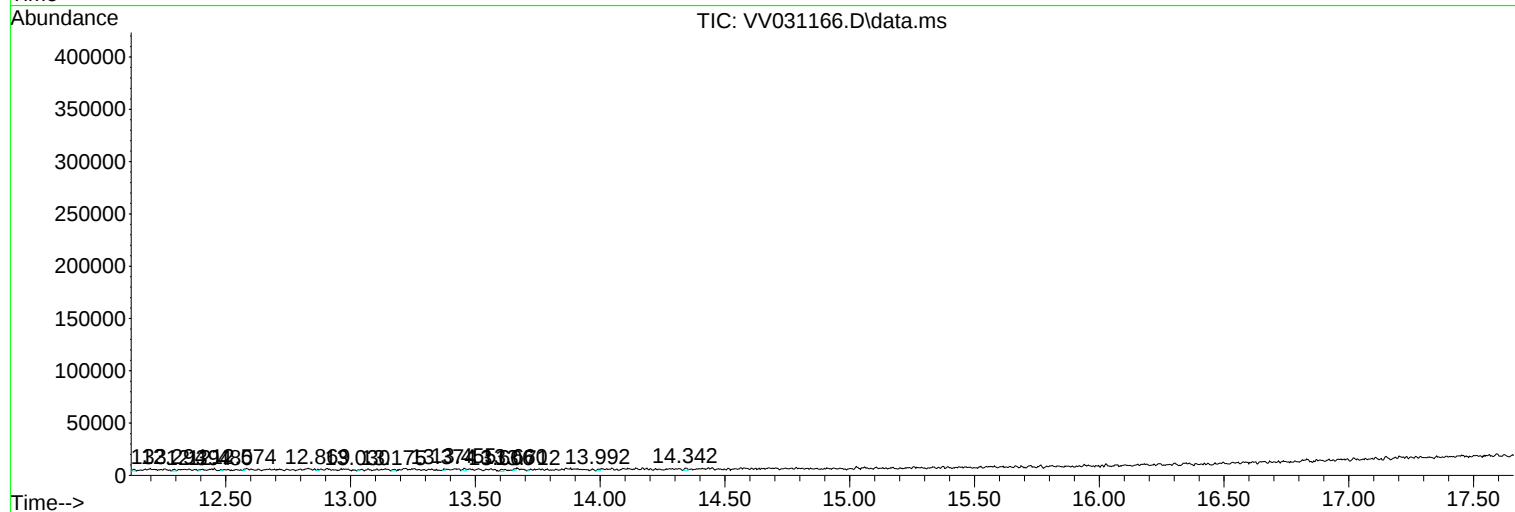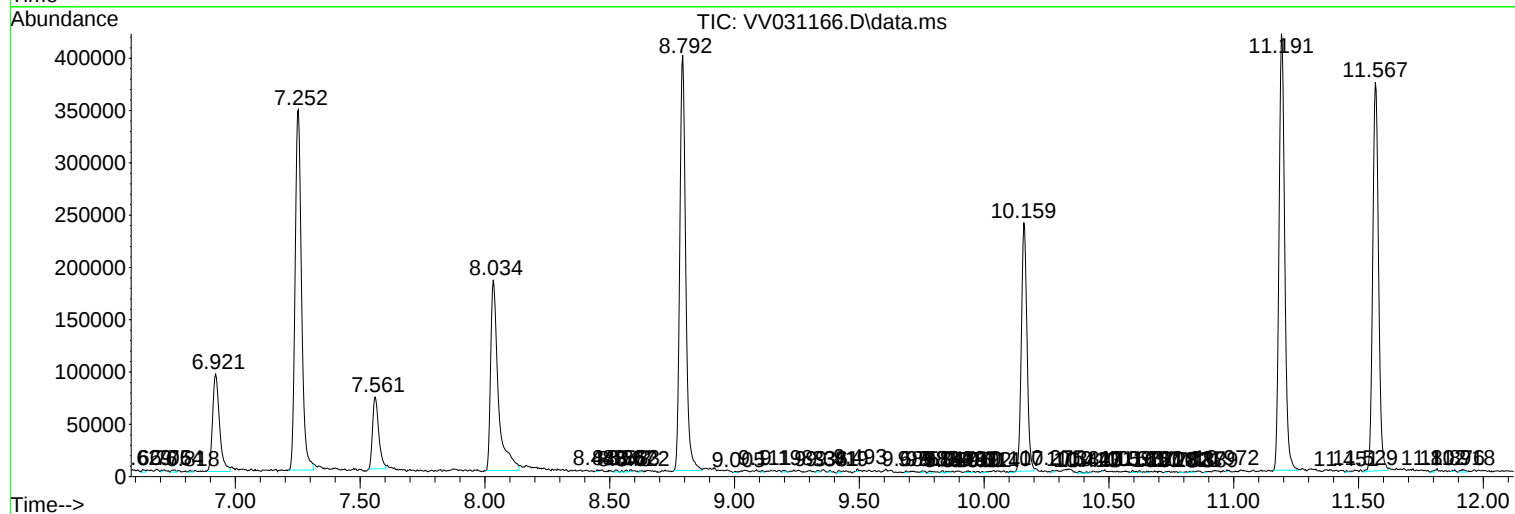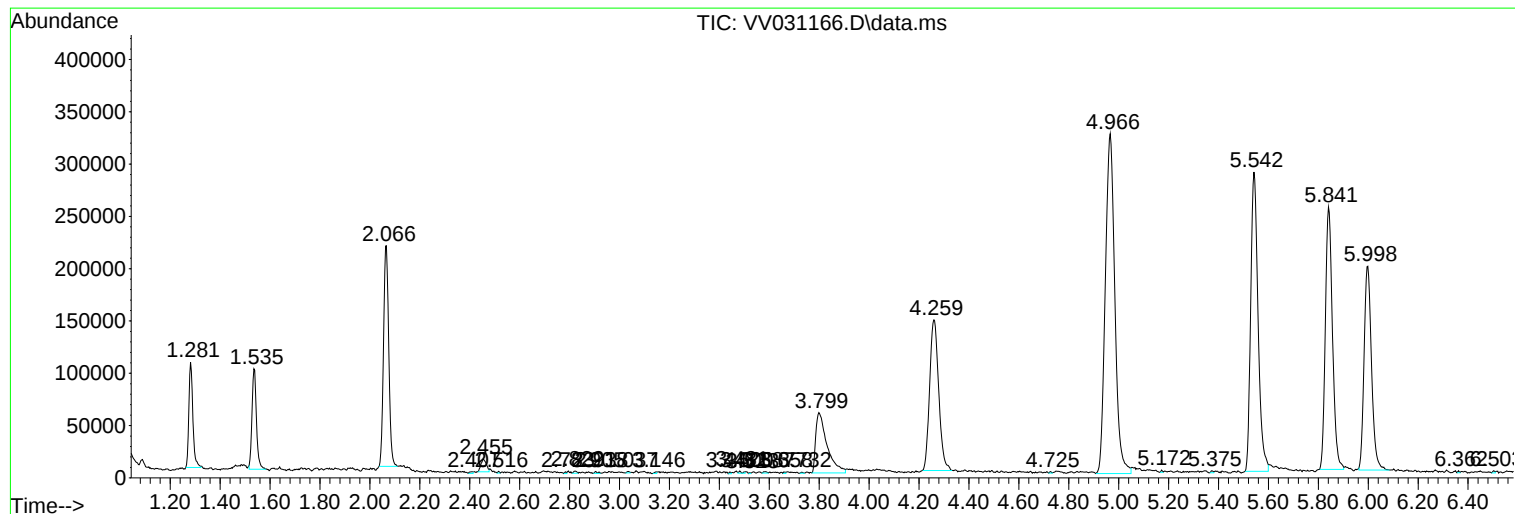

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031166.D
Acq On : 22 May 2023 15:19
Operator : SY/MD
Sample : 02866-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031166.D
Acq On : 22 May 2023 15:19
Operator : SY/MD
Sample : 02866-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX79DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------