

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031167.D
 Acq On : 22 May 2023 15:43
 Operator : SY/MD
 Sample : 02865-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	113360	121940	14.37%	1.716%
2	1.536	148	154	167	rVB	108587	127214	15.00%	1.790%
3	2.063	310	318	333	rBV	204405	294758	34.75%	4.147%
4	2.249	372	376	378	rBV5	2203	1962	0.23%	0.028%
5	2.523	457	461	463	rBV5	1225	974	0.11%	0.014%
6	2.545	463	468	470	rVV5	2056	1439	0.17%	0.020%
7	2.574	474	477	479	rBV3	1829	1165	0.14%	0.016%
8	2.664	499	505	508	rBV8	2032	2320	0.27%	0.033%
9	2.696	510	515	517	rBV6	2561	2321	0.27%	0.033%
10	2.876	567	571	572	rBV4	1763	887	0.10%	0.012%
11	2.892	574	576	579	rVB3	1808	899	0.11%	0.013%
12	2.937	588	590	593	rBV4	1276	843	0.10%	0.012%
13	3.034	614	620	622	rVB6	1693	1571	0.19%	0.022%
14	3.089	634	637	640	rBV5	1807	1446	0.17%	0.020%
15	3.118	644	646	650	rVB5	1265	958	0.11%	0.013%
16	3.179	660	665	667	rBV5	1702	1691	0.20%	0.024%
17	3.217	673	677	679	rBV5	1300	981	0.12%	0.014%
18	3.368	718	724	727	rVB7	1000	979	0.12%	0.014%
19	3.394	728	732	735	rVV6	1949	1126	0.13%	0.016%
20	3.497	761	764	767	rBV5	1420	991	0.12%	0.014%
21	3.587	788	792	793	rBV3	1867	938	0.11%	0.013%
22	3.664	814	816	821	rVB6	1705	1178	0.14%	0.017%
23	3.754	840	844	845	rBV4	1171	954	0.11%	0.013%
24	3.799	848	858	885	rBV	65894	194969	22.98%	2.743%
25	4.259	988	1001	1029	rVB	146510	368173	43.40%	5.180%
26	4.519	1077	1082	1087	rBV9	1805	2602	0.31%	0.037%
27	4.625	1112	1115	1120	rBV7	1524	1311	0.15%	0.018%
28	4.651	1120	1123	1126	rBV6	1192	898	0.11%	0.013%
29	4.732	1145	1148	1151	rBV3	1800	1075	0.13%	0.015%
30	4.796	1165	1168	1170	rBV3	1815	1243	0.15%	0.017%
31	4.841	1180	1182	1188	rVB7	1773	906	0.11%	0.013%
32	4.966	1204	1221	1244	rBV2	320505	848319	100.00%	11.936%
33	5.429	1363	1365	1368	rBV4	2616	1586	0.19%	0.022%
34	5.542	1387	1400	1419	rBV	277452	573124	67.56%	8.064%
35	5.757	1464	1467	1468	rBV3	2008	970	0.11%	0.014%
36	5.802	1478	1481	1482	rBV3	1726	893	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031167.D
 Acq On : 22 May 2023 15:43
 Operator : SY/MD
 Sample : 02865-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.841	1482	1493	1510	rVV2	150317	302531	35.66%	4.257%
38	5.995	1530	1541	1562	rVB	193861	390227	46.00%	5.491%
39	6.442	1677	1680	1686	rBV6	1926	1830	0.22%	0.026%
40	6.474	1686	1690	1694	rBV6	1765	1794	0.21%	0.025%
41	6.519	1700	1704	1710	rBV10	2451	2359	0.28%	0.033%
42	6.609	1730	1732	1739	rVB6	2061	1364	0.16%	0.019%
43	6.683	1753	1755	1760	rBV6	1196	996	0.12%	0.014%
44	6.706	1760	1762	1768	rVB7	1806	1427	0.17%	0.020%
45	6.735	1768	1771	1777	rBV8	2162	2391	0.28%	0.034%
46	6.777	1781	1784	1786	rBV4	1340	925	0.11%	0.013%
47	6.883	1815	1817	1819	rVV3	1731	899	0.11%	0.013%
48	6.921	1819	1829	1847	rVV2	93466	178046	20.99%	2.505%
49	7.175	1904	1908	1910	rBV5	1295	874	0.10%	0.012%
50	7.252	1921	1932	1947	rBV	338845	595219	70.16%	8.375%
51	7.561	2019	2028	2044	rBV	69300	123053	14.51%	1.731%
52	7.712	2073	2075	2077	rBV2	1879	978	0.12%	0.014%
53	7.934	2142	2144	2148	rVB5	2076	1050	0.12%	0.015%
54	7.973	2151	2156	2160	rVB8	2020	1883	0.22%	0.026%
55	8.034	2165	2175	2190	rBV	202052	388728	45.82%	5.470%
56	8.596	2347	2350	2351	rBV3	2207	1278	0.15%	0.018%
57	8.738	2390	2394	2397	rBV6	1310	958	0.11%	0.013%
58	8.793	2397	2411	2434	rBV	427438	719296	84.79%	10.121%
59	9.188	2530	2534	2536	rBV4	1339	998	0.12%	0.014%
60	9.384	2587	2595	2596	rBV6	2312	2507	0.30%	0.035%
61	9.664	2673	2682	2685	rBV8	4040	6516	0.77%	0.092%
62	9.831	2730	2734	2737	rBV6	1598	1371	0.16%	0.019%
63	9.902	2752	2756	2758	rBV4	1798	1115	0.13%	0.016%
64	10.088	2812	2814	2819	rBV6	1561	1388	0.16%	0.020%
65	10.159	2823	2836	2857	rBV	294010	473558	55.82%	6.663%
66	10.329	2885	2889	2891	rBV5	1823	1464	0.17%	0.021%
67	10.503	2939	2943	2946	rBV5	1412	1005	0.12%	0.014%
68	10.770	3024	3026	3029	rVV4	1654	1068	0.13%	0.015%
69	10.796	3031	3034	3037	rVB5	1882	1322	0.16%	0.019%
70	10.860	3050	3054	3059	rVB7	1970	1838	0.22%	0.026%
71	11.191	3145	3157	3176	rBV	421461	668388	78.79%	9.405%
72	11.326	3196	3199	3201	rBV4	1801	1103	0.13%	0.016%
73	11.432	3230	3232	3238	rVB6	1826	1202	0.14%	0.017%
74	11.567	3265	3274	3291	rVB	380746	618970	72.96%	8.709%
75	11.989	3402	3405	3407	rBV4	2055	1081	0.13%	0.015%
76	12.050	3421	3424	3427	rBV5	2018	1387	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031167.D
 Acq On : 22 May 2023 15:43
 Operator : SY/MD
 Sample : 02865-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.101	3437	3440	3445	rBV6	2110	2273	0.27%	0.032%
78	12.133	3448	3450	3453	rBV4	2434	1259	0.15%	0.018%
79	12.159	3456	3458	3460	rBV3	2244	1068	0.13%	0.015%
80	12.255	3485	3488	3495	rVB9	2133	2437	0.29%	0.034%
81	12.288	3495	3498	3499	rBV3	1917	955	0.11%	0.013%
82	12.458	3545	3551	3553	rBV8	2001	1852	0.22%	0.026%
83	12.558	3580	3582	3586	rVB5	1768	968	0.11%	0.014%
84	12.593	3588	3593	3595	rBV5	1403	1378	0.16%	0.019%
85	12.921	3692	3695	3697	rVB4	1480	933	0.11%	0.013%
86	12.940	3697	3701	3702	rBV3	1885	1306	0.15%	0.018%
87	13.050	3730	3735	3737	rBV5	2734	2380	0.28%	0.033%
88	13.114	3752	3755	3758	rBV5	1918	1536	0.18%	0.022%
89	13.178	3773	3775	3778	rBV4	1877	936	0.11%	0.013%
90	13.201	3780	3782	3783	rBV2	1792	846	0.10%	0.012%
91	13.291	3807	3810	3814	rVB5	1644	1136	0.13%	0.016%
92	13.648	3917	3921	3922	rBV4	1436	913	0.11%	0.013%
93	13.783	3959	3963	3965	rBV4	1597	1439	0.17%	0.020%
94	13.841	3977	3981	3984	rBV6	1608	1106	0.13%	0.016%
95	13.956	4015	4017	4021	rBV5	1268	912	0.11%	0.013%
96	14.519	4186	4192	4196	rBV9	2089	2384	0.28%	0.034%
97	14.664	4231	4237	4242	rBV9	3137	3905	0.46%	0.055%
98	14.847	4291	4294	4297	rBV4	1905	1387	0.16%	0.020%
99	15.008	4340	4344	4348	rBV7	2585	2476	0.29%	0.035%
100	15.101	4370	4373	4377	rBV6	1513	1269	0.15%	0.018%




Sum of corrected areas: 7107045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031167.D
Acq On : 22 May 2023 15:43
Operator : SY/MD
Sample : 02865-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

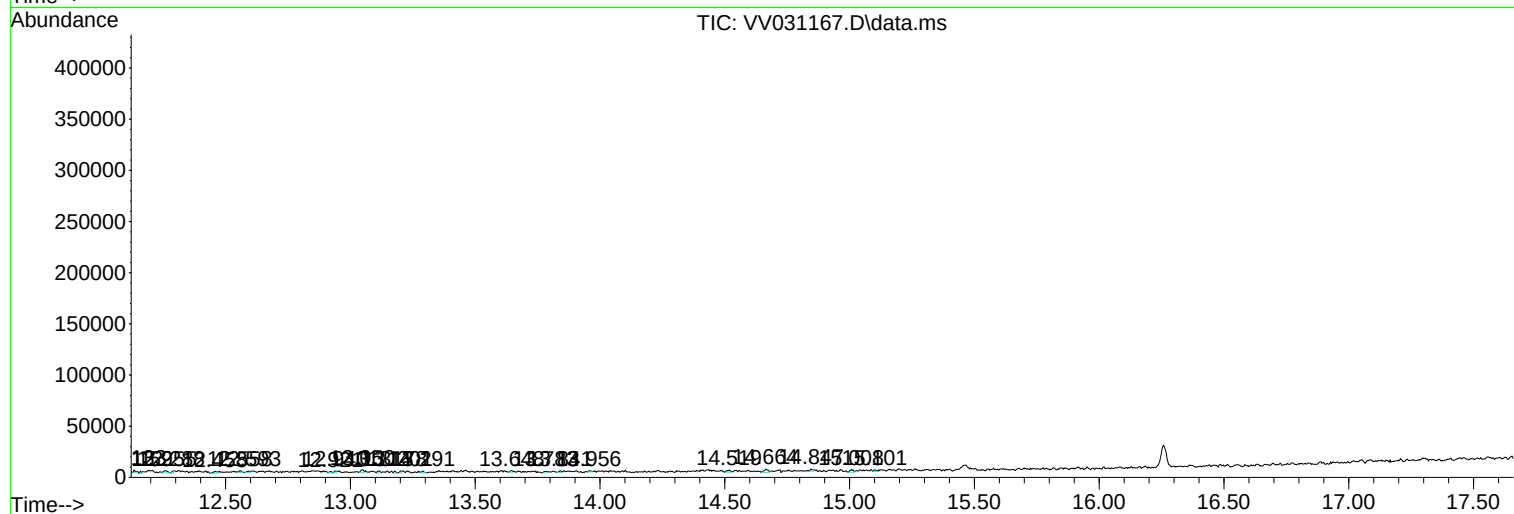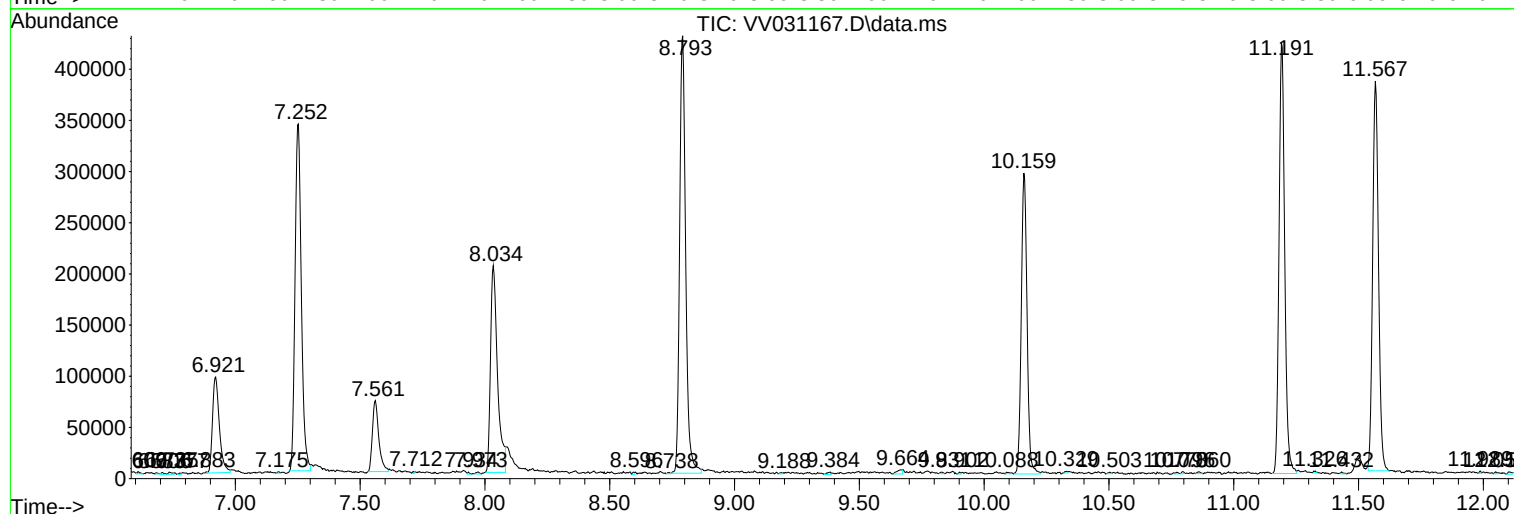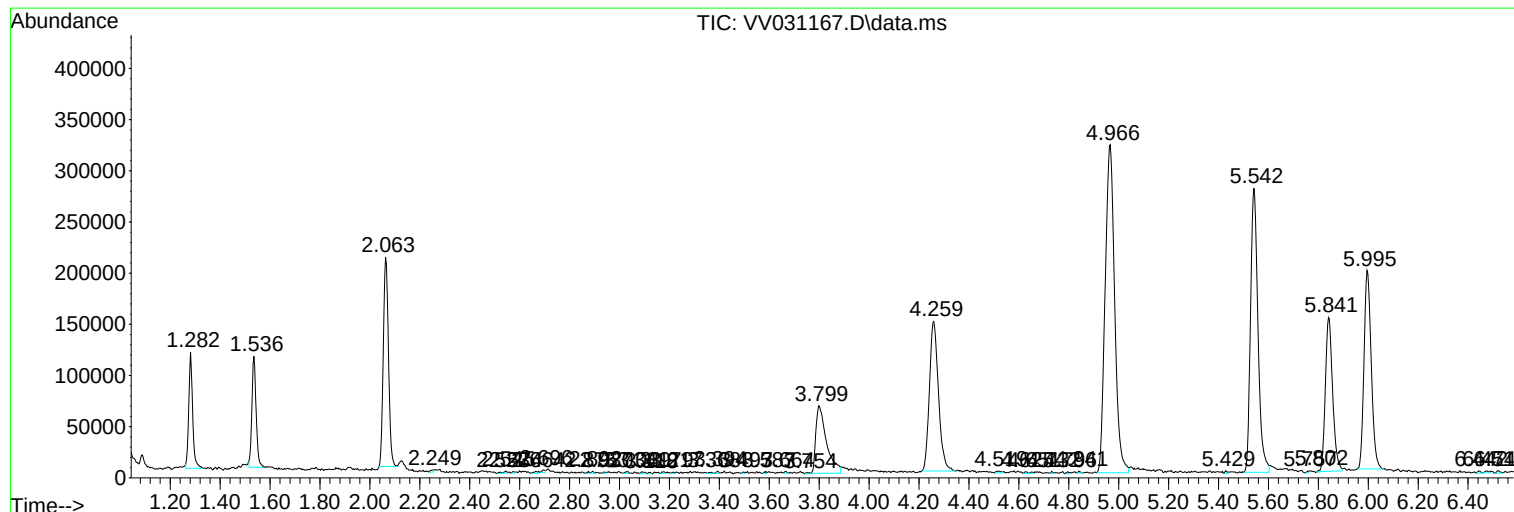

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031167.D
Acq On : 22 May 2023 15:43
Operator : SY/MD
Sample : 02865-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031167.D
Acq On : 22 May 2023 15:43
Operator : SY/MD
Sample : 02865-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc