

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031168.D
 Acq On : 22 May 2023 16:07
 Operator : SY/MD
 Sample : 02861-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rVB	99463	107410	12.66%	1.655%
2	1.536	148	154	169	rVB	96097	113105	13.33%	1.743%
3	2.063	309	318	342	rVB	213505	321867	37.93%	4.960%
4	2.320	395	398	399	rBV3	1531	966	0.11%	0.015%
5	2.770	536	538	541	rVB4	1841	896	0.11%	0.014%
6	2.847	559	562	564	rBV4	2122	804	0.09%	0.012%
7	2.860	564	566	572	rVV6	1657	1259	0.15%	0.019%
8	3.018	612	615	617	rBV4	1280	814	0.10%	0.013%
9	3.105	640	642	646	rVB4	1686	1106	0.13%	0.017%
10	3.127	646	649	651	rBV5	1896	1273	0.15%	0.020%
11	3.217	674	677	680	rBV5	1380	966	0.11%	0.015%
12	3.240	682	684	686	rBV2	2288	1036	0.12%	0.016%
13	3.310	704	706	710	rBV4	1068	825	0.10%	0.013%
14	3.339	713	715	719	rVB5	1623	893	0.11%	0.014%
15	3.446	744	748	754	rBV9	2267	2733	0.32%	0.042%
16	3.587	790	792	796	rVV5	1998	1115	0.13%	0.017%
17	3.609	797	799	804	rVB5	2050	1479	0.17%	0.023%
18	3.761	844	846	849	rBV3	1890	1110	0.13%	0.017%
19	3.802	849	859	884	rVV2	59535	168882	19.90%	2.602%
20	4.259	988	1001	1024	rVB	145980	364139	42.91%	5.611%
21	4.519	1080	1082	1085	rBV4	1796	1163	0.14%	0.018%
22	4.561	1092	1095	1096	rBV3	1479	832	0.10%	0.013%
23	4.629	1110	1116	1119	rBV8	2918	2912	0.34%	0.045%
24	4.674	1127	1130	1133	rVB5	1680	1312	0.15%	0.020%
25	4.693	1133	1136	1138	rBV4	1538	890	0.10%	0.014%
26	4.719	1138	1144	1145	rBV5	1114	1172	0.14%	0.018%
27	4.838	1178	1181	1183	rBV3	1208	1018	0.12%	0.016%
28	4.966	1204	1221	1243	rBV2	316849	848582	100.00%	13.077%
29	5.542	1388	1400	1422	rBV	273122	564359	66.51%	8.697%
30	5.822	1483	1487	1488	rBV4	3430	2101	0.25%	0.032%
31	5.995	1530	1541	1563	rBV	192910	402400	47.42%	6.201%
32	6.297	1634	1635	1640	rBV4	2052	1844	0.22%	0.028%
33	6.564	1714	1718	1719	rBV4	1632	1238	0.15%	0.019%
34	6.696	1756	1759	1760	rBV3	1505	983	0.12%	0.015%
35	6.728	1767	1769	1773	rVB4	1788	1172	0.14%	0.018%
36	6.748	1773	1775	1778	rBV4	1309	865	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031168.D
 Acq On : 22 May 2023 16:07
 Operator : SY/MD
 Sample : 02861-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.921	1818	1829	1846	rBV	96884	183389	21.61%	2.826%
38	7.249	1920	1931	1953	rVV	338394	610103	71.90%	9.402%
39	7.523	2013	2016	2018	rBV4	2354	1485	0.17%	0.023%
40	7.561	2019	2028	2046	rVV	71463	130376	15.36%	2.009%
41	8.034	2166	2175	2208	rBV	187947	394806	46.53%	6.084%
42	8.410	2289	2292	2293	rBV3	1332	771	0.09%	0.012%
43	8.558	2334	2338	2343	rVB8	1628	1541	0.18%	0.024%
44	8.584	2343	2346	2347	rBV3	1610	839	0.10%	0.013%
45	8.793	2399	2411	2435	rBV	419927	711660	83.86%	10.967%
46	9.323	2575	2576	2579	rBV3	1667	868	0.10%	0.013%
47	9.387	2593	2596	2598	rBV3	1833	1088	0.13%	0.017%
48	9.458	2616	2618	2621	rBV4	1705	1037	0.12%	0.016%
49	9.506	2630	2633	2634	rBV3	1848	1073	0.13%	0.017%
50	9.542	2641	2644	2645	rBV2	1675	950	0.11%	0.015%
51	9.654	2675	2679	2683	rBV6	1874	1796	0.21%	0.028%
52	9.696	2689	2692	2694	rBV4	1972	1126	0.13%	0.017%
53	9.796	2719	2723	2724	rBV4	1482	958	0.11%	0.015%
54	9.821	2728	2731	2733	rBV4	1326	826	0.10%	0.013%
55	9.886	2749	2751	2753	rBV3	1756	896	0.11%	0.014%
56	10.008	2787	2789	2791	rBV2	1523	830	0.10%	0.013%
57	10.159	2825	2836	2848	rBV	232449	374688	44.15%	5.774%
58	10.320	2882	2886	2887	rBV3	1660	1403	0.17%	0.022%
59	10.468	2930	2932	2935	rVB3	2036	792	0.09%	0.012%
60	10.513	2942	2946	2947	rBV4	1141	843	0.10%	0.013%
61	10.535	2951	2953	2956	rBV4	1652	953	0.11%	0.015%
62	10.712	3006	3008	3012	rVB5	1339	906	0.11%	0.014%
63	10.731	3012	3014	3019	rBV6	1858	1371	0.16%	0.021%
64	10.796	3032	3034	3037	rBV4	1925	940	0.11%	0.014%
65	11.001	3095	3098	3102	rBV6	1740	1808	0.21%	0.028%
66	11.046	3109	3112	3117	rBV6	1843	1356	0.16%	0.021%
67	11.120	3130	3135	3137	rBV6	1195	1306	0.15%	0.020%
68	11.143	3139	3142	3146	rBV4	1064	871	0.10%	0.013%
69	11.191	3146	3157	3177	rBV	364491	578794	68.21%	8.919%
70	11.403	3220	3223	3225	rBV4	1521	839	0.10%	0.013%
71	11.477	3241	3246	3248	rBV5	1567	1236	0.15%	0.019%
72	11.567	3264	3274	3291	rVB	325888	515348	60.73%	7.942%
73	11.651	3298	3300	3301	rBV2	2236	1009	0.12%	0.016%
74	11.963	3395	3397	3399	rBV3	1774	877	0.10%	0.014%
75	12.153	3452	3456	3457	rBV4	1795	1326	0.16%	0.020%
76	12.288	3496	3498	3502	rBV4	1827	1051	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031168.D
 Acq On : 22 May 2023 16:07
 Operator : SY/MD
 Sample : 02861-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.342	3511	3515	3518	rBV7	1863	1717	0.20%	0.026%
78	12.394	3528	3531	3532	rBV3	1319	829	0.10%	0.013%
79	12.448	3546	3548	3550	rVB2	1875	874	0.10%	0.013%
80	12.493	3558	3562	3567	rVB8	1688	1312	0.15%	0.020%
81	12.706	3623	3628	3630	rBV4	1659	1544	0.18%	0.024%
82	12.863	3675	3677	3679	rBV3	1728	844	0.10%	0.013%
83	12.972	3706	3711	3713	rBV6	1461	1221	0.14%	0.019%
84	13.024	3724	3727	3729	rBV4	1306	778	0.09%	0.012%
85	13.075	3741	3743	3747	rBV5	1460	1032	0.12%	0.016%
86	13.124	3754	3758	3764	rVB8	1846	2006	0.24%	0.031%
87	13.162	3768	3770	3771	rBV2	1938	921	0.11%	0.014%
88	13.207	3781	3784	3787	rVB5	1924	1103	0.13%	0.017%
89	13.336	3820	3824	3825	rBV4	2210	1626	0.19%	0.025%
90	13.702	3936	3938	3941	rVB4	2031	771	0.09%	0.012%
91	13.760	3954	3956	3961	rVB6	1348	797	0.09%	0.012%
92	13.783	3961	3963	3966	rBV3	2336	1453	0.17%	0.022%
93	14.030	4034	4040	4043	rBV8	1552	1585	0.19%	0.024%
94	14.239	4101	4105	4109	rVB8	1721	1272	0.15%	0.020%
95	14.297	4121	4123	4126	rBV4	1786	982	0.12%	0.015%
96	14.455	4170	4172	4174	rBV3	1448	863	0.10%	0.013%
97	14.503	4185	4187	4190	rBV3	1672	1077	0.13%	0.017%
98	14.869	4298	4301	4303	rBV5	3151	1760	0.21%	0.027%
99	14.914	4313	4315	4317	rBV3	2075	933	0.11%	0.014%
100	15.554	4512	4514	4519	rBV6	2770	2308	0.27%	0.036%




Sum of corrected areas: 6489264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031168.D
Acq On : 22 May 2023 16:07
Operator : SY/MD
Sample : 02861-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

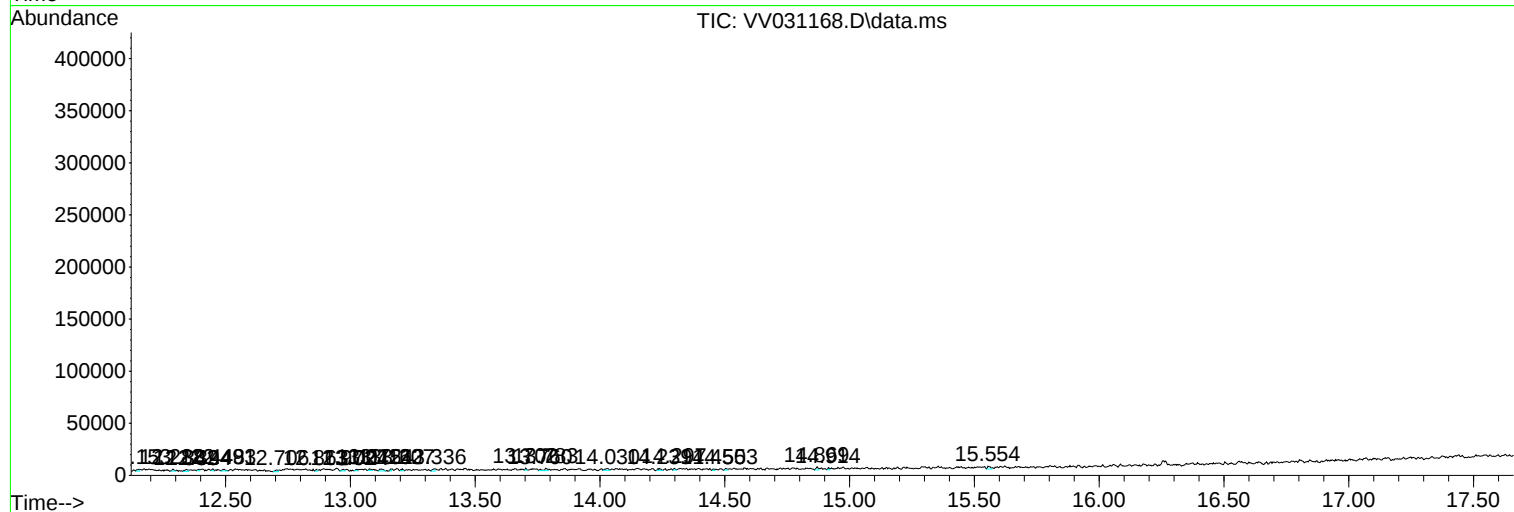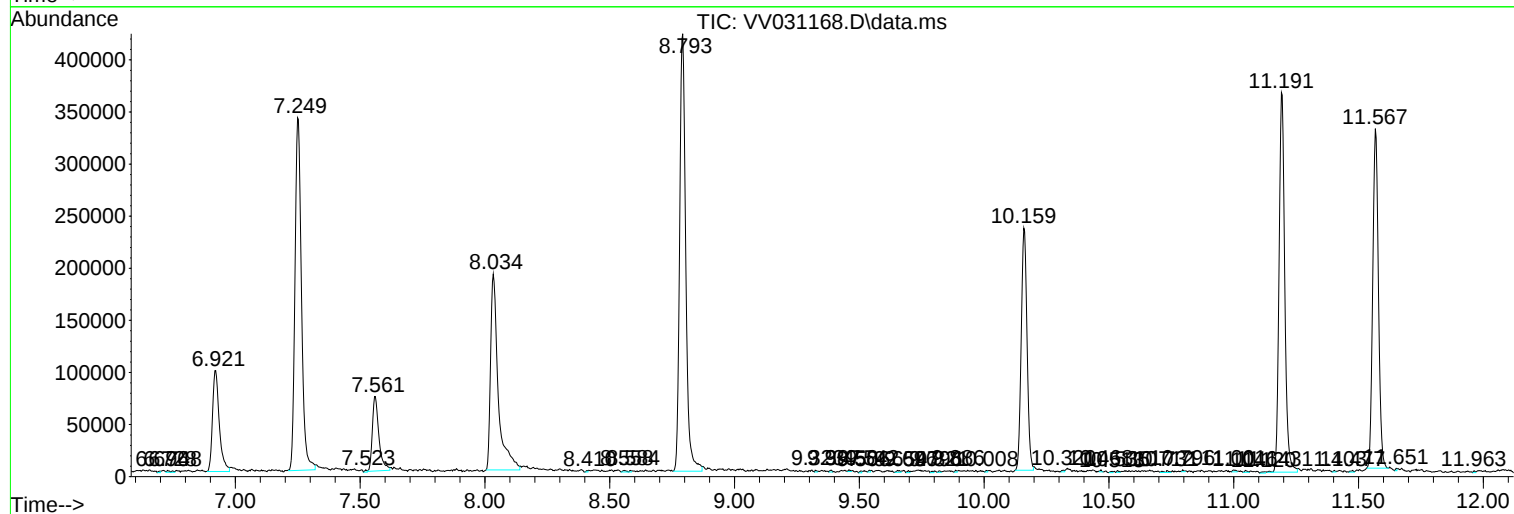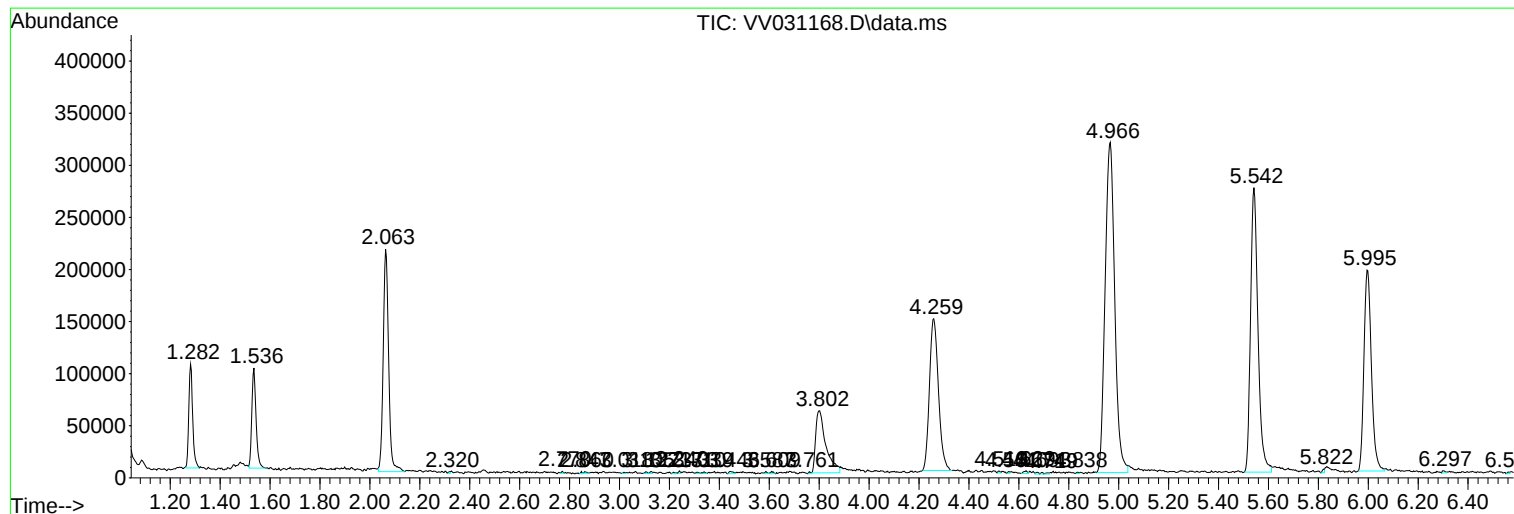

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031168.D
Acq On : 22 May 2023 16:07
Operator : SY/MD
Sample : 02861-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031168.D
Acq On : 22 May 2023 16:07
Operator : SY/MD
Sample : 02861-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------