

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031169.D
 Acq On : 22 May 2023 16:31
 Operator : SY/MD
 Sample : 02861-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOFM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rVB	95383	106474	13.04%	1.601%
2	1.536	148	154	167	rVB	93030	116174	14.22%	1.747%
3	2.063	309	318	331	rBV	201844	288488	35.32%	4.339%
4	2.401	421	423	428	rVB6	1854	1241	0.15%	0.019%
5	2.426	428	431	433	rBV4	1896	1316	0.16%	0.020%
6	2.548	467	469	473	rVB4	1437	724	0.09%	0.011%
7	2.606	485	487	490	rBV4	1144	684	0.08%	0.010%
8	2.687	507	512	513	rBV4	1879	1682	0.21%	0.025%
9	2.770	535	538	542	rVB6	2004	1115	0.14%	0.017%
10	2.899	575	578	582	rBV5	1788	1488	0.18%	0.022%
11	3.015	612	614	618	rVB5	1902	1324	0.16%	0.020%
12	3.047	620	624	626	rBV5	1896	1408	0.17%	0.021%
13	3.066	628	630	633	rBV4	1366	815	0.10%	0.012%
14	3.114	643	645	647	rBV3	1580	1012	0.12%	0.015%
15	3.349	715	718	720	rBV4	1562	952	0.12%	0.014%
16	3.388	726	730	732	rBV5	1590	1119	0.14%	0.017%
17	3.433	738	744	751	rVB10	1514	2284	0.28%	0.034%
18	3.465	751	754	755	rBV3	1225	892	0.11%	0.013%
19	3.507	764	767	769	rBV3	2037	1101	0.13%	0.017%
20	3.584	788	791	794	rVB4	1175	693	0.08%	0.010%
21	3.683	819	822	823	rBV3	1930	1052	0.13%	0.016%
22	3.799	849	858	888	rVV	57761	165413	20.25%	2.488%
23	4.124	956	959	960	rBV3	1438	949	0.12%	0.014%
24	4.163	969	971	973	rBV3	1274	733	0.09%	0.011%
25	4.259	982	1001	1026	rBV2	141077	365336	44.73%	5.495%
26	4.481	1067	1070	1073	rBV5	1340	1032	0.13%	0.016%
27	4.561	1091	1095	1098	rBV4	2559	2222	0.27%	0.033%
28	4.683	1130	1133	1134	rBV3	1687	787	0.10%	0.012%
29	4.780	1161	1163	1167	rBV5	1639	1420	0.17%	0.021%
30	4.802	1167	1170	1174	rVB5	2296	1597	0.20%	0.024%
31	4.873	1190	1192	1196	rBV4	1928	1631	0.20%	0.025%
32	4.966	1204	1221	1242	rBV2	305836	816754	100.00%	12.284%
33	5.301	1323	1325	1327	rBV3	1751	989	0.12%	0.015%
34	5.339	1335	1337	1341	rBV5	1369	992	0.12%	0.015%
35	5.439	1365	1368	1370	rBV3	1708	1173	0.14%	0.018%
36	5.542	1388	1400	1429	rBV	283802	597699	73.18%	8.989%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031169.D
 Acq On : 22 May 2023 16:31
 Operator : SY/MD
 Sample : 02861-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOFM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.995	1529	1541	1561	rBV2	191192	393874	48.22%	5.924%
38	6.667	1746	1750	1751	rBV4	1233	938	0.11%	0.014%
39	6.699	1757	1760	1762	rBV4	1701	1022	0.13%	0.015%
40	6.744	1772	1774	1780	rVB7	1044	798	0.10%	0.012%
41	6.815	1793	1796	1797	rBV3	1779	1029	0.13%	0.015%
42	6.921	1820	1829	1846	rVV	91951	168099	20.58%	2.528%
43	7.101	1880	1885	1886	rBV5	1322	1063	0.13%	0.016%
44	7.252	1921	1932	1955	rBV	327319	585316	71.66%	8.803%
45	7.561	2019	2028	2042	rBV	67901	122035	14.94%	1.835%
46	7.915	2136	2138	2141	rVB4	1962	1005	0.12%	0.015%
47	7.976	2155	2157	2160	rBV4	1653	974	0.12%	0.015%
48	8.034	2164	2175	2208	rBV	182688	394091	48.25%	5.927%
49	8.378	2280	2282	2285	rBV4	2308	1065	0.13%	0.016%
50	8.404	2288	2290	2294	rVB5	1733	686	0.08%	0.010%
51	8.731	2390	2392	2395	rVB4	1913	937	0.11%	0.014%
52	8.793	2401	2411	2429	rBV	437192	717823	87.89%	10.796%
53	8.986	2469	2471	2472	rBV2	2062	768	0.09%	0.012%
54	9.230	2542	2547	2549	rVB6	2298	1971	0.24%	0.030%
55	9.272	2556	2560	2562	rBV5	1187	907	0.11%	0.014%
56	9.432	2607	2610	2614	rBV6	1918	1279	0.16%	0.019%
57	9.455	2614	2617	2619	rBV4	2585	1524	0.19%	0.023%
58	9.815	2728	2729	2732	rVB3	2039	894	0.11%	0.013%
59	10.011	2787	2790	2792	rBV4	1349	899	0.11%	0.014%
60	10.092	2812	2815	2819	rBV6	1678	1542	0.19%	0.023%
61	10.159	2824	2836	2851	rBV	280776	440164	53.89%	6.620%
62	10.574	2961	2965	2969	rBV7	2005	1564	0.19%	0.024%
63	10.593	2969	2971	2975	rVV5	1686	1451	0.18%	0.022%
64	10.629	2979	2982	2987	rBV7	2258	1611	0.20%	0.024%
65	10.677	2994	2997	2999	rBV3	1442	931	0.11%	0.014%
66	10.767	3020	3025	3029	rBV7	1114	1158	0.14%	0.017%
67	10.799	3033	3035	3039	rVB4	2276	1497	0.18%	0.023%
68	10.992	3092	3095	3099	rBV6	1958	1598	0.20%	0.024%
69	11.040	3107	3110	3111	rBV3	1453	761	0.09%	0.011%
70	11.088	3122	3125	3127	rBV3	1094	722	0.09%	0.011%
71	11.143	3140	3142	3146	rBV5	2382	1955	0.24%	0.029%
72	11.194	3146	3158	3179	rVV	417680	671832	82.26%	10.104%
73	11.497	3248	3252	3254	rBV4	1952	1560	0.19%	0.023%
74	11.567	3262	3274	3294	rBV	377421	599860	73.44%	9.022%
75	11.899	3375	3377	3378	rBV2	1600	786	0.10%	0.012%
76	12.066	3427	3429	3431	rBV3	1436	804	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031169.D
 Acq On : 22 May 2023 16:31
 Operator : SY/MD
 Sample : 02861-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOFM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.104	3438	3441	3443	rBV4	1337	719	0.09%	0.011%
78	12.120	3443	3446	3449	rBV5	1934	1388	0.17%	0.021%
79	12.188	3464	3467	3470	rBV5	1894	1294	0.16%	0.019%
80	12.362	3518	3521	3525	rBV6	1390	1082	0.13%	0.016%
81	12.423	3535	3540	3542	rBV5	1851	1515	0.19%	0.023%
82	12.545	3576	3578	3583	rBV5	1998	1742	0.21%	0.026%
83	12.632	3603	3605	3607	rBV3	1312	699	0.09%	0.011%
84	12.783	3650	3652	3654	rBV2	1394	774	0.09%	0.012%
85	12.834	3663	3668	3670	rBV6	1714	1396	0.17%	0.021%
86	12.847	3670	3672	3674	rBV3	1374	703	0.09%	0.011%
87	13.001	3717	3720	3724	rBV6	1447	901	0.11%	0.014%
88	13.204	3781	3783	3785	rBV3	2597	1282	0.16%	0.019%
89	13.294	3805	3811	3813	rBV6	1390	1096	0.13%	0.016%
90	13.516	3875	3880	3882	rVB6	1563	1400	0.17%	0.021%
91	13.532	3882	3885	3886	rBV2	1432	807	0.10%	0.012%
92	13.651	3919	3922	3926	rVB5	1965	1188	0.15%	0.018%
93	13.921	4003	4006	4007	rBV3	1359	854	0.10%	0.013%
94	14.120	4066	4068	4070	rBV3	1829	1108	0.14%	0.017%
95	14.368	4141	4145	4147	rBV5	1600	1356	0.17%	0.020%
96	14.734	4253	4259	4262	rBV8	2485	3318	0.41%	0.050%
97	14.873	4299	4302	4304	rBV4	1952	1042	0.13%	0.016%
98	14.898	4308	4310	4311	rBV2	1913	745	0.09%	0.011%
99	14.969	4330	4332	4333	rBV2	2130	799	0.10%	0.012%
100	15.069	4361	4363	4370	rBV7	1983	2175	0.27%	0.033%




Sum of corrected areas: 6648941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031169.D
Acq On : 22 May 2023 16:31
Operator : SY/MD
Sample : 02861-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

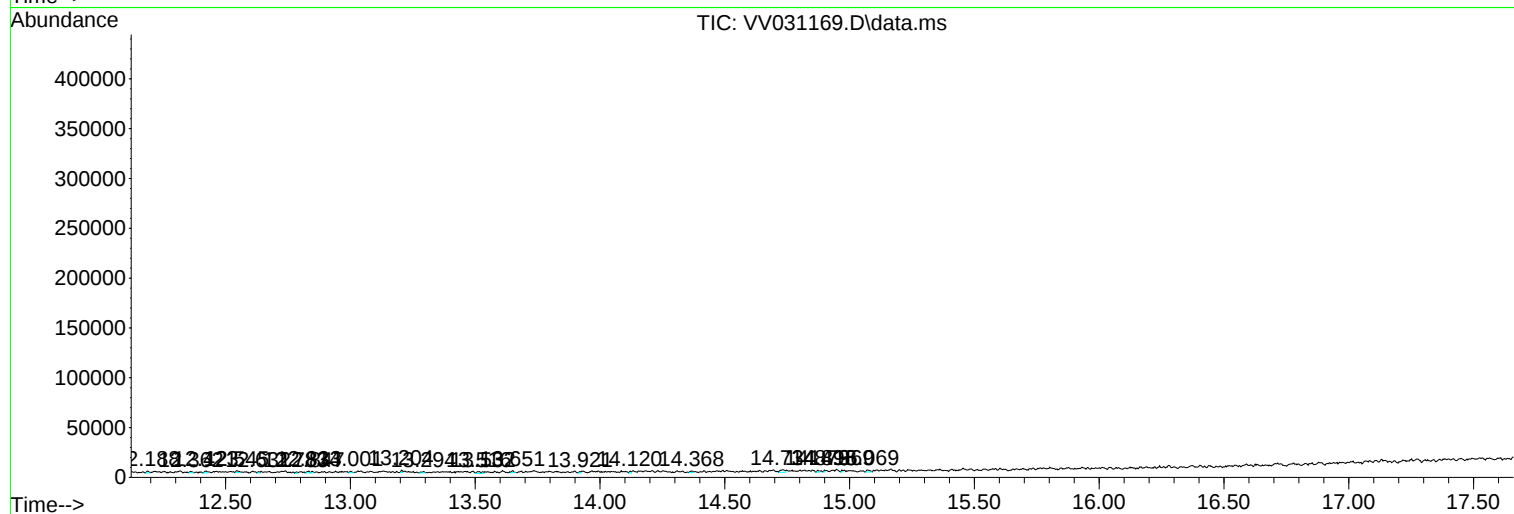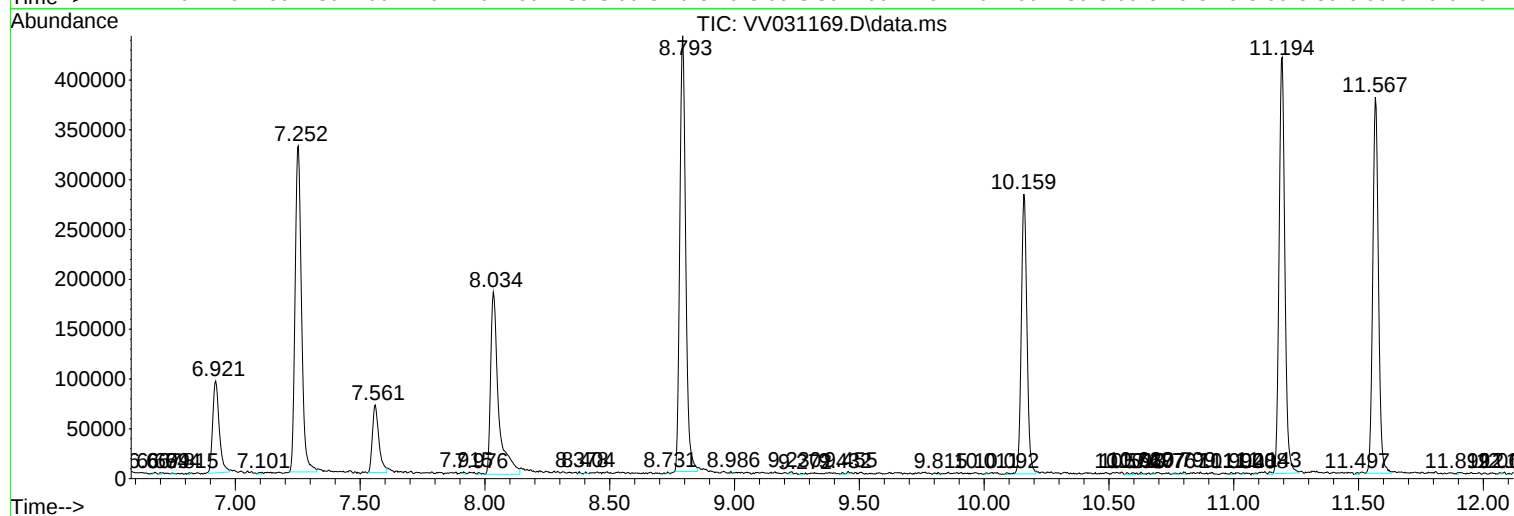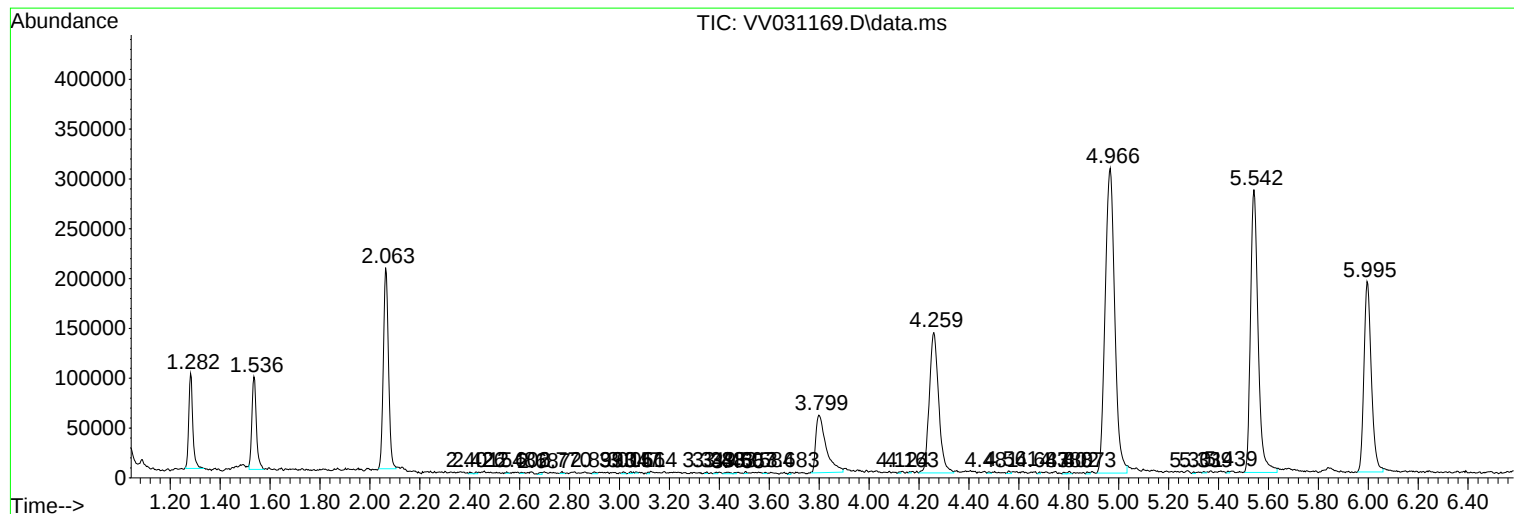

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031169.D
Acq On : 22 May 2023 16:31
Operator : SY/MD
Sample : 02861-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031169.D
Acq On : 22 May 2023 16:31
Operator : SY/MD
Sample : 02861-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------