

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031170.D
 Acq On : 22 May 2023 16:55
 Operator : SY/MD
 Sample : 02861-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rVB	97893	104986	12.30%	1.627%
2	1.535	148	154	170	rVB	102496	125875	14.75%	1.950%
3	2.063	309	318	332	rBV	206716	303154	35.51%	4.697%
4	2.230	368	370	372	rBV3	1540	730	0.09%	0.011%
5	2.301	389	392	394	rBV4	1393	1001	0.12%	0.016%
6	2.613	487	489	491	rBV3	907	460	0.05%	0.007%
7	2.767	533	537	541	rBV6	1906	1643	0.19%	0.025%
8	2.831	555	557	559	rVB3	2361	978	0.11%	0.015%
9	2.851	559	563	564	rBV4	1206	699	0.08%	0.011%
10	2.883	571	573	575	rBV3	1520	560	0.07%	0.009%
11	3.169	661	662	663	rBV	990	250	0.03%	0.004%
12	3.310	702	706	710	rBV7	2057	1622	0.19%	0.025%
13	3.339	712	715	717	rBV4	1576	1114	0.13%	0.017%
14	3.371	722	725	726	rBV3	1145	656	0.08%	0.010%
15	3.526	772	773	774	rBV	941	294	0.03%	0.005%
16	3.629	803	805	806	rBV2	1031	358	0.04%	0.006%
17	3.674	817	819	820	rBV3	781	291	0.03%	0.005%
18	3.715	830	832	833	rBV3	1265	370	0.04%	0.006%
19	3.799	849	858	882	rBV	59980	165246	19.36%	2.560%
20	4.259	989	1001	1022	rVB	144635	362307	42.44%	5.613%
21	4.706	1138	1140	1143	rBV4	1868	1039	0.12%	0.016%
22	4.780	1161	1163	1165	rBV2	1086	493	0.06%	0.008%
23	4.867	1188	1190	1194	rBV6	1406	1078	0.13%	0.017%
24	4.966	1204	1221	1244	rBV2	317041	853649	100.00%	13.225%
25	5.452	1371	1372	1373	rBV	1382	362	0.04%	0.006%
26	5.542	1384	1400	1430	rBV	275010	595646	69.78%	9.228%
27	5.786	1474	1476	1477	rBV	1148	442	0.05%	0.007%
28	5.934	1520	1522	1524	rBV3	1458	695	0.08%	0.011%
29	5.998	1529	1542	1558	rBV	194644	409508	47.97%	6.344%
30	6.378	1657	1660	1661	rBV2	1858	1249	0.15%	0.019%
31	6.448	1678	1682	1686	rBV6	2663	2713	0.32%	0.042%
32	6.571	1715	1720	1721	rBV5	1483	1265	0.15%	0.020%
33	6.921	1818	1829	1845	rBV2	96018	183147	21.45%	2.837%
34	7.249	1920	1931	1950	rBV	339509	609318	71.38%	9.440%
35	7.558	2020	2027	2047	rBV	60968	109561	12.83%	1.697%
36	7.944	2145	2147	2149	rBV3	1390	549	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031170.D
 Acq On : 22 May 2023 16:55
 Operator : SY/MD
 Sample : 02861-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	8.034	2166	2175	2190	rBV	163842	309042	36.20%	4.788%
38	8.683	2373	2377	2379	rBV4	1487	1153	0.14%	0.018%
39	8.747	2394	2397	2399	rBV4	2189	1629	0.19%	0.025%
40	8.792	2400	2411	2433	rVV	338725	572346	67.05%	8.867%
41	8.956	2459	2462	2465	rBV5	2189	1645	0.19%	0.025%
42	9.069	2494	2497	2498	rBV3	1454	871	0.10%	0.013%
43	9.149	2518	2522	2525	rBV6	1337	1232	0.14%	0.019%
44	9.210	2539	2541	2542	rBV2	826	416	0.05%	0.006%
45	9.233	2546	2548	2550	rVB3	1550	508	0.06%	0.008%
46	9.323	2575	2576	2577	rBV	862	260	0.03%	0.004%
47	9.336	2577	2580	2581	rVV3	1841	981	0.11%	0.015%
48	9.345	2581	2583	2587	rVB5	2173	951	0.11%	0.015%
49	9.419	2604	2606	2608	rBV4	1468	793	0.09%	0.012%
50	9.493	2622	2629	2633	rBV10	3289	4377	0.51%	0.068%
51	9.577	2653	2655	2656	rBV2	1155	653	0.08%	0.010%
52	9.596	2659	2661	2663	rBV3	922	486	0.06%	0.008%
53	9.673	2684	2685	2689	rVB4	1153	704	0.08%	0.011%
54	9.690	2689	2690	2695	rBV4	1498	1141	0.13%	0.018%
55	9.754	2707	2710	2712	rBV4	1222	837	0.10%	0.013%
56	9.767	2712	2714	2715	rVB2	1001	277	0.03%	0.004%
57	9.815	2727	2729	2734	rVB6	909	595	0.07%	0.009%
58	9.873	2740	2747	2752	rBV8	2896	3466	0.41%	0.054%
59	9.953	2770	2772	2775	rBV4	1258	735	0.09%	0.011%
60	10.034	2792	2797	2798	rBV5	2060	1481	0.17%	0.023%
61	10.159	2824	2836	2853	rBV	229828	379610	44.47%	5.881%
62	10.259	2865	2867	2868	rBV2	1231	630	0.07%	0.010%
63	10.342	2891	2893	2895	rBV3	1298	572	0.07%	0.009%
64	10.368	2900	2901	2903	rBV2	1088	428	0.05%	0.007%
65	10.416	2914	2916	2921	rVB6	1818	1289	0.15%	0.020%
66	10.452	2921	2927	2928	rBV6	2599	1919	0.22%	0.030%
67	10.471	2930	2933	2934	rBV3	1760	997	0.12%	0.015%
68	10.545	2952	2956	2957	rBV3	1664	1279	0.15%	0.020%
69	10.641	2983	2986	2987	rBV3	1220	460	0.05%	0.007%
70	10.670	2993	2995	2998	rBV4	1567	907	0.11%	0.014%
71	10.908	3067	3069	3071	rBV3	1195	477	0.06%	0.007%
72	11.043	3109	3111	3113	rBV3	1644	839	0.10%	0.013%
73	11.191	3145	3157	3175	rBV	407842	659662	77.28%	10.220%
74	11.509	3253	3256	3258	rBV4	1612	878	0.10%	0.014%
75	11.567	3262	3274	3291	rBV	389742	628488	73.62%	9.737%
76	11.660	3299	3303	3305	rBV4	3201	2372	0.28%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031170.D
 Acq On : 22 May 2023 16:55
 Operator : SY/MD
 Sample : 02861-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.760	3332	3334	3338	rBV4	1869	979	0.11%	0.015%
78	11.831	3354	3356	3359	rBV3	951	524	0.06%	0.008%
79	11.972	3396	3400	3404	rVB6	2107	1919	0.22%	0.030%
80	11.992	3404	3406	3408	rBV2	1481	610	0.07%	0.009%
81	12.197	3468	3470	3475	rBV6	1988	2018	0.24%	0.031%
82	12.349	3515	3517	3520	rBV5	1928	1035	0.12%	0.016%
83	12.442	3543	3546	3548	rBV4	1635	1093	0.13%	0.017%
84	12.654	3610	3612	3614	rBV3	2173	1116	0.13%	0.017%
85	12.802	3656	3658	3660	rBV2	2688	1219	0.14%	0.019%
86	12.844	3669	3671	3672	rBV2	1205	478	0.06%	0.007%
87	12.905	3689	3690	3695	rVB4	1760	939	0.11%	0.015%
88	12.979	3711	3713	3714	rBV2	1097	522	0.06%	0.008%
89	12.988	3714	3716	3718	rVV2	1192	663	0.08%	0.010%
90	13.117	3754	3756	3759	rBV4	1935	1345	0.16%	0.021%
91	13.313	3815	3817	3819	rBV3	1633	920	0.11%	0.014%
92	13.377	3835	3837	3839	rBV3	1560	586	0.07%	0.009%
93	13.648	3919	3921	3925	rBV5	1419	989	0.12%	0.015%
94	13.683	3929	3932	3934	rBV4	1738	1118	0.13%	0.017%
95	13.972	4020	4022	4024	rBV3	1013	579	0.07%	0.009%
96	14.027	4037	4039	4041	rBV3	1685	845	0.10%	0.013%
97	14.387	4149	4151	4158	rVB7	2182	2034	0.24%	0.032%
98	14.435	4164	4166	4167	rBV2	1516	488	0.06%	0.008%
99	14.445	4167	4169	4171	rVV3	1730	698	0.08%	0.011%
100	14.760	4264	4267	4270	rBV4	1867	1268	0.15%	0.020%




Sum of corrected areas: 6454679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031170.D
Acq On : 22 May 2023 16:55
Operator : SY/MD
Sample : 02861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

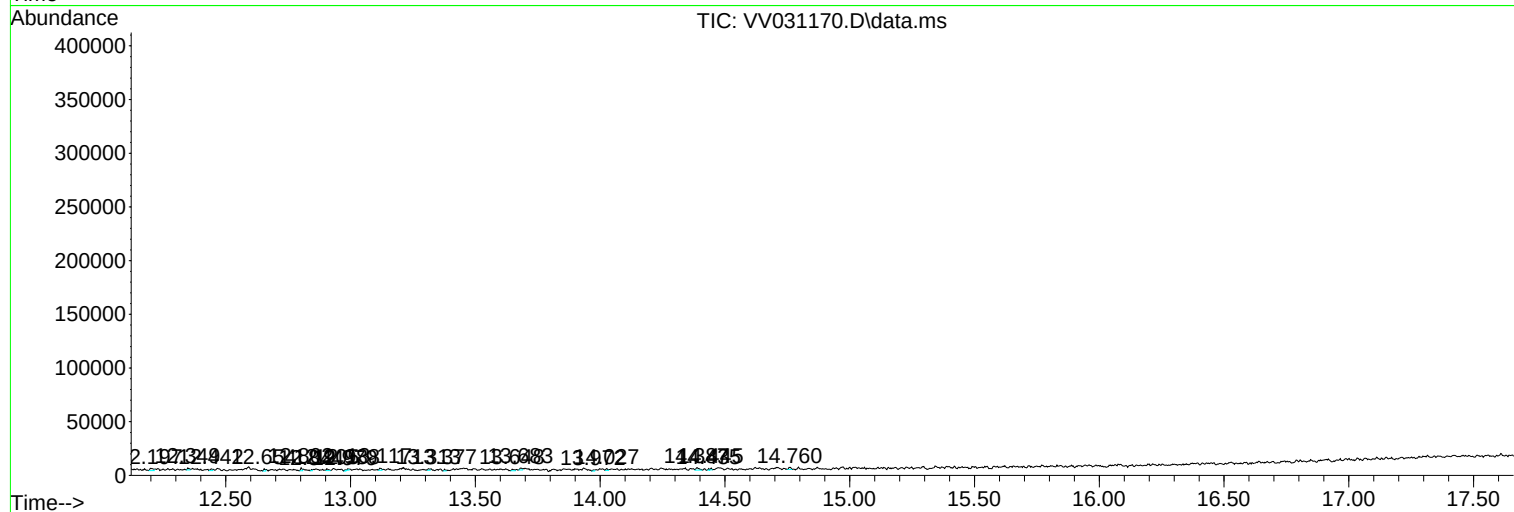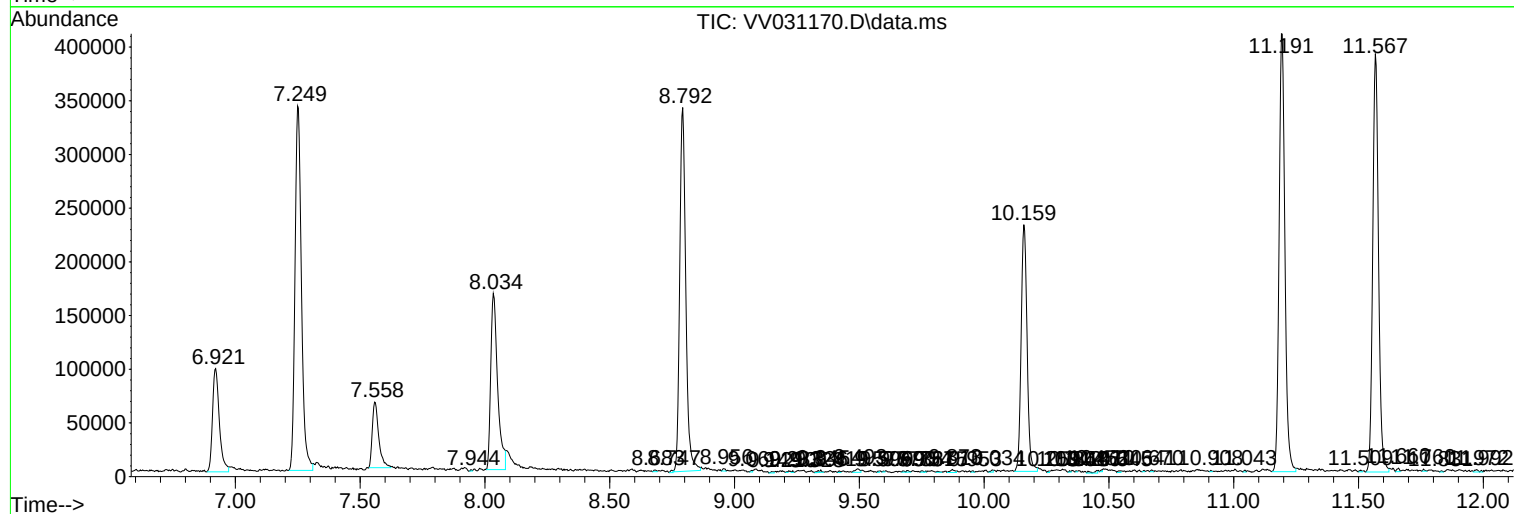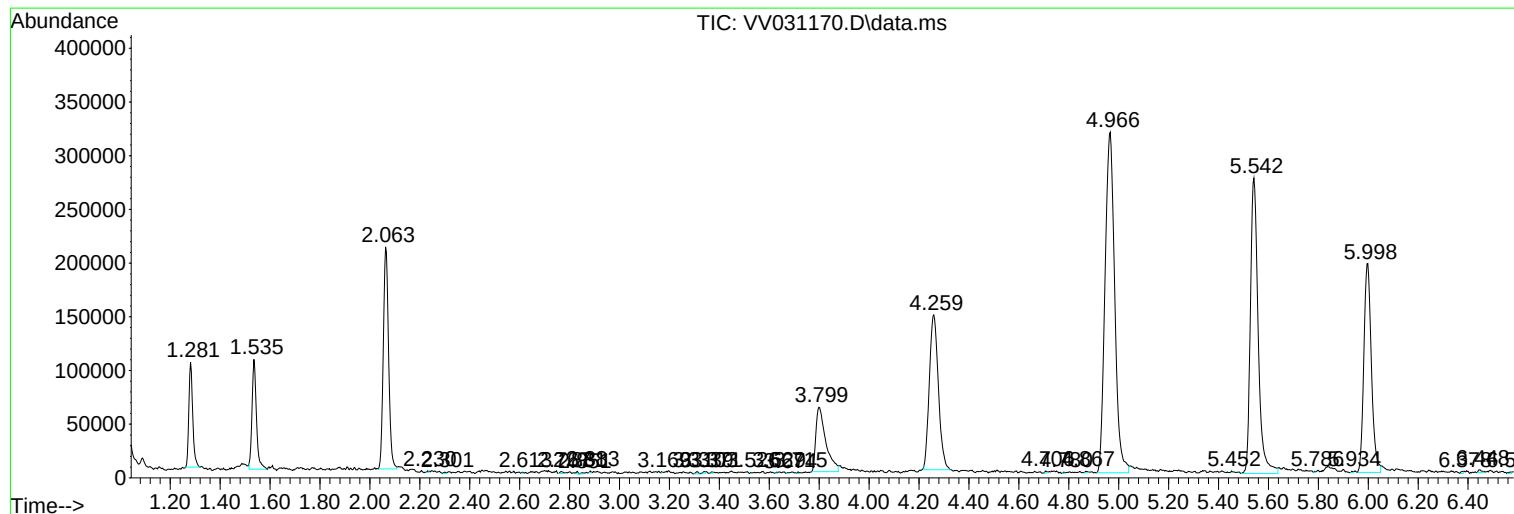

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031170.D
Acq On : 22 May 2023 16:55
Operator : SY/MD
Sample : 02861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031170.D
Acq On : 22 May 2023 16:55
Operator : SY/MD
Sample : 02861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc