

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031171.D
 Acq On : 22 May 2023 17:19
 Operator : SY/MD
 Sample : 02861-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rBV	106792	116472	12.84%	1.635%
2	1.535	148	154	170	rVB	110094	128228	14.13%	1.801%
3	2.063	310	318	331	rVB	214784	306643	33.80%	4.306%
4	2.201	359	361	363	rBV2	2344	1118	0.12%	0.016%
5	2.320	395	398	402	rVB6	2778	1838	0.20%	0.026%
6	2.381	415	417	419	rVB3	1677	625	0.07%	0.009%
7	2.535	463	465	472	rVB8	1444	1361	0.15%	0.019%
8	2.642	494	498	501	rBV6	1484	1379	0.15%	0.019%
9	2.680	508	510	512	rVB3	1691	559	0.06%	0.008%
10	2.735	525	527	529	rBV3	1097	533	0.06%	0.007%
11	2.777	537	540	543	rBV5	2411	2144	0.24%	0.030%
12	2.834	551	558	559	rBV6	1221	1202	0.13%	0.017%
13	2.918	582	584	586	rBV2	979	530	0.06%	0.007%
14	2.966	597	599	600	rBV2	1529	557	0.06%	0.008%
15	3.166	658	661	664	rBV5	1860	1299	0.14%	0.018%
16	3.230	678	681	684	rBV4	1509	1103	0.12%	0.015%
17	3.269	690	693	694	rBV3	1426	623	0.07%	0.009%
18	3.397	730	733	735	rBV3	2082	1099	0.12%	0.015%
19	3.436	743	745	747	rBV3	1428	640	0.07%	0.009%
20	3.481	755	759	762	rVB5	1787	1107	0.12%	0.016%
21	3.506	762	767	772	rBV7	1635	1671	0.18%	0.023%
22	3.529	772	774	776	rVV3	1452	610	0.07%	0.009%
23	3.542	776	778	780	rVV3	1557	645	0.07%	0.009%
24	3.568	784	786	790	rBV5	1224	1055	0.12%	0.015%
25	3.725	832	835	840	rVB7	1488	1422	0.16%	0.020%
26	3.760	840	846	847	rBV5	1452	1188	0.13%	0.017%
27	3.799	849	858	885	rBV2	63222	179365	19.77%	2.519%
28	4.259	987	1001	1018	rBV	157574	393556	43.38%	5.526%
29	4.487	1067	1072	1077	rBV9	2943	3579	0.39%	0.050%
30	4.693	1134	1136	1139	rVB4	965	577	0.06%	0.008%
31	4.715	1139	1143	1145	rBV4	1783	1536	0.17%	0.022%
32	4.764	1157	1158	1161	rBV3	1682	876	0.10%	0.012%
33	4.847	1182	1184	1188	rBV4	1350	823	0.09%	0.012%
34	4.863	1188	1189	1192	rVB3	1416	541	0.06%	0.008%
35	4.963	1205	1220	1251	rVV2	336999	907262	100.00%	12.740%
36	5.542	1388	1400	1424	rBV	279222	588535	64.87%	8.264%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031171.D
 Acq On : 22 May 2023 17:19
 Operator : SY/MD
 Sample : 02861-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.905	1511	1513	1516	rBV4	1105	529	0.06%	0.007%
38	5.995	1530	1541	1562	rBV	209766	427405	47.11%	6.002%
39	6.227	1609	1613	1615	rBV5	2386	1676	0.18%	0.024%
40	6.378	1656	1660	1662	rBV5	1075	940	0.10%	0.013%
41	6.439	1677	1679	1682	rBV4	1386	883	0.10%	0.012%
42	6.693	1754	1758	1759	rBV4	1080	716	0.08%	0.010%
43	6.918	1819	1828	1848	rBV2	101969	190281	20.97%	2.672%
44	7.249	1918	1931	1951	rBV	363763	658710	72.60%	9.249%
45	7.558	2018	2027	2042	rBV	75652	136682	15.07%	1.919%
46	7.882	2127	2128	2131	rBV2	1698	703	0.08%	0.010%
47	7.976	2155	2157	2159	rBV3	1602	641	0.07%	0.009%
48	8.034	2165	2175	2202	rBV	202194	425576	46.91%	5.976%
49	8.329	2265	2267	2270	rVB4	1688	775	0.09%	0.011%
50	8.747	2395	2397	2399	rBV3	2145	1281	0.14%	0.018%
51	8.792	2400	2411	2435	rVV	440549	736133	81.14%	10.337%
52	9.021	2480	2482	2484	rBV3	1710	822	0.09%	0.012%
53	9.442	2611	2613	2614	rBV2	1104	532	0.06%	0.007%
54	9.477	2622	2624	2625	rBV2	1141	539	0.06%	0.008%
55	9.516	2633	2636	2638	rBV4	1292	712	0.08%	0.010%
56	9.747	2706	2708	2711	rVB4	1166	553	0.06%	0.008%
57	9.783	2717	2719	2720	rBV2	1480	692	0.08%	0.010%
58	9.860	2740	2743	2745	rBV3	2045	1299	0.14%	0.018%
59	9.915	2757	2760	2761	rBV3	1474	734	0.08%	0.010%
60	9.947	2769	2770	2772	rBV2	1783	866	0.10%	0.012%
61	10.159	2823	2836	2857	rBV	306953	501554	55.28%	7.043%
62	10.288	2874	2876	2879	rVB4	1961	694	0.08%	0.010%
63	10.410	2908	2914	2918	rBV8	2908	2968	0.33%	0.042%
64	10.458	2926	2929	2934	rBV6	1198	1018	0.11%	0.014%
65	10.587	2965	2969	2971	rBV6	1727	1380	0.15%	0.019%
66	10.651	2986	2989	2992	rBV3	1007	775	0.09%	0.011%
67	10.693	2999	3002	3004	rBV4	2173	1439	0.16%	0.020%
68	10.751	3017	3020	3024	rBV6	1624	1564	0.17%	0.022%
69	10.773	3025	3027	3032	rVB5	1072	686	0.08%	0.010%
70	11.062	3113	3117	3118	rBV3	1172	869	0.10%	0.012%
71	11.072	3118	3120	3123	rVV5	1095	712	0.08%	0.010%
72	11.191	3147	3157	3176	rBV	418312	668272	73.66%	9.384%
73	11.468	3237	3243	3246	rBV8	2094	1840	0.20%	0.026%
74	11.567	3259	3274	3290	rBV	412535	665400	73.34%	9.343%
75	11.889	3372	3374	3376	rBV3	1392	635	0.07%	0.009%
76	11.940	3388	3390	3393	rBV4	1226	806	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
 Data File : VV031171.D
 Acq On : 22 May 2023 17:19
 Operator : SY/MD
 Sample : 02861-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.979	3398	3402	3406	rBV5	2733	2486	0.27%	0.035%
78	12.001	3406	3409	3412	rBV5	951	779	0.09%	0.011%
79	12.111	3437	3443	3445	rBV7	1709	1500	0.17%	0.021%
80	12.223	3475	3478	3482	rBV5	1400	1308	0.14%	0.018%
81	12.390	3527	3530	3532	rBV4	1711	952	0.10%	0.013%
82	12.586	3587	3591	3592	rBV4	1412	939	0.10%	0.013%
83	12.693	3622	3624	3628	rBV5	2418	1962	0.22%	0.028%
84	12.786	3651	3653	3657	rVB5	1687	921	0.10%	0.013%
85	12.808	3657	3660	3662	rBV4	2223	1368	0.15%	0.019%
86	12.934	3696	3699	3702	rBV5	1226	1022	0.11%	0.014%
87	12.969	3707	3710	3712	rBV4	1459	921	0.10%	0.013%
88	13.053	3732	3736	3741	rBV8	1938	2374	0.26%	0.033%
89	13.127	3757	3759	3763	rVB5	1490	1118	0.12%	0.016%
90	13.191	3776	3779	3781	rBV3	2927	1715	0.19%	0.024%
91	13.332	3820	3823	3825	rBV3	1545	885	0.10%	0.012%
92	13.355	3828	3830	3832	rBV3	1353	610	0.07%	0.009%
93	13.400	3842	3844	3845	rBV2	1331	603	0.07%	0.008%
94	13.448	3857	3859	3862	rVB4	1918	901	0.10%	0.013%
95	13.779	3957	3962	3965	rBV6	1388	1505	0.17%	0.021%
96	13.812	3970	3972	3974	rBV3	1544	803	0.09%	0.011%
97	13.869	3988	3990	3993	rBV4	2026	1205	0.13%	0.017%
98	14.435	4163	4166	4168	rBV4	1392	940	0.10%	0.013%
99	14.580	4207	4211	4213	rBV5	1613	1348	0.15%	0.019%
100	14.641	4228	4230	4231	rBV2	2277	869	0.10%	0.012%




Sum of corrected areas: 7121627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031171.D
Acq On : 22 May 2023 17:19
Operator : SY/MD
Sample : 02861-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

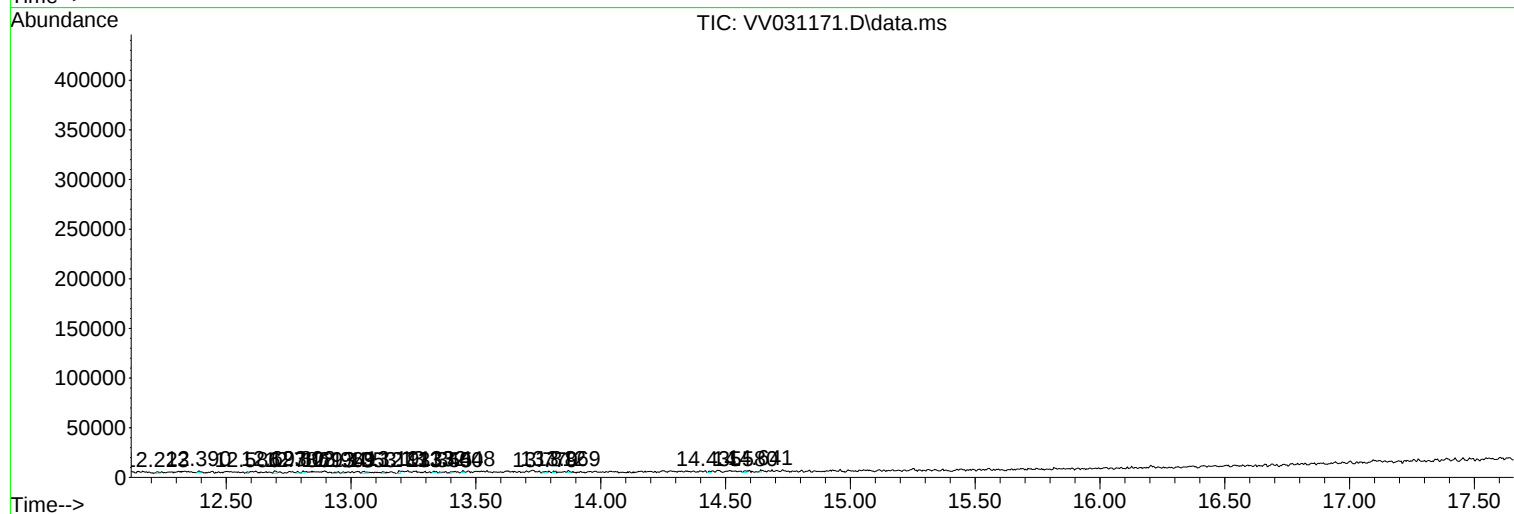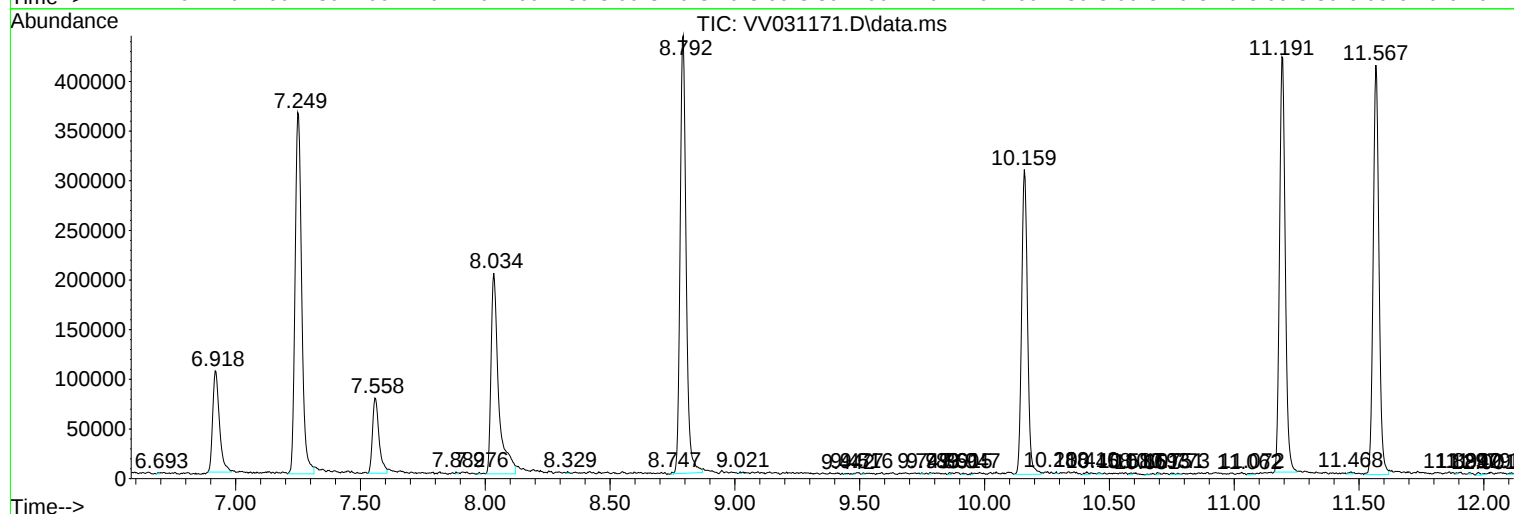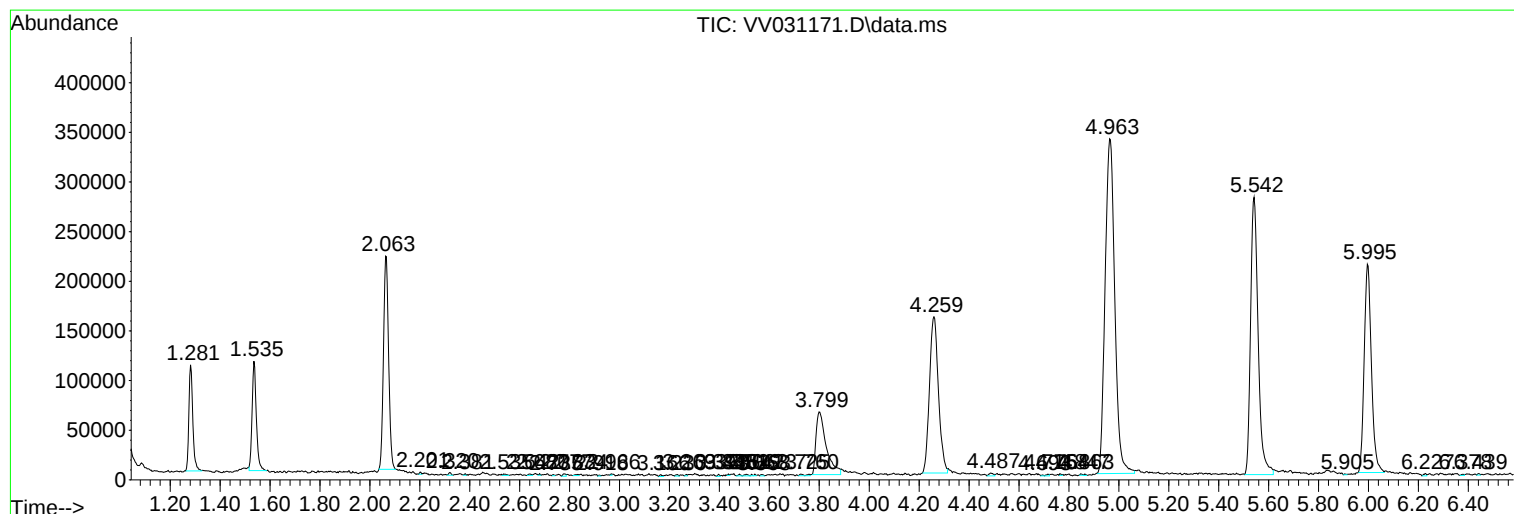

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031171.D
Acq On : 22 May 2023 17:19
Operator : SY/MD
Sample : 02861-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031171.D
Acq On : 22 May 2023 17:19
Operator : SY/MD
Sample : 02861-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------