
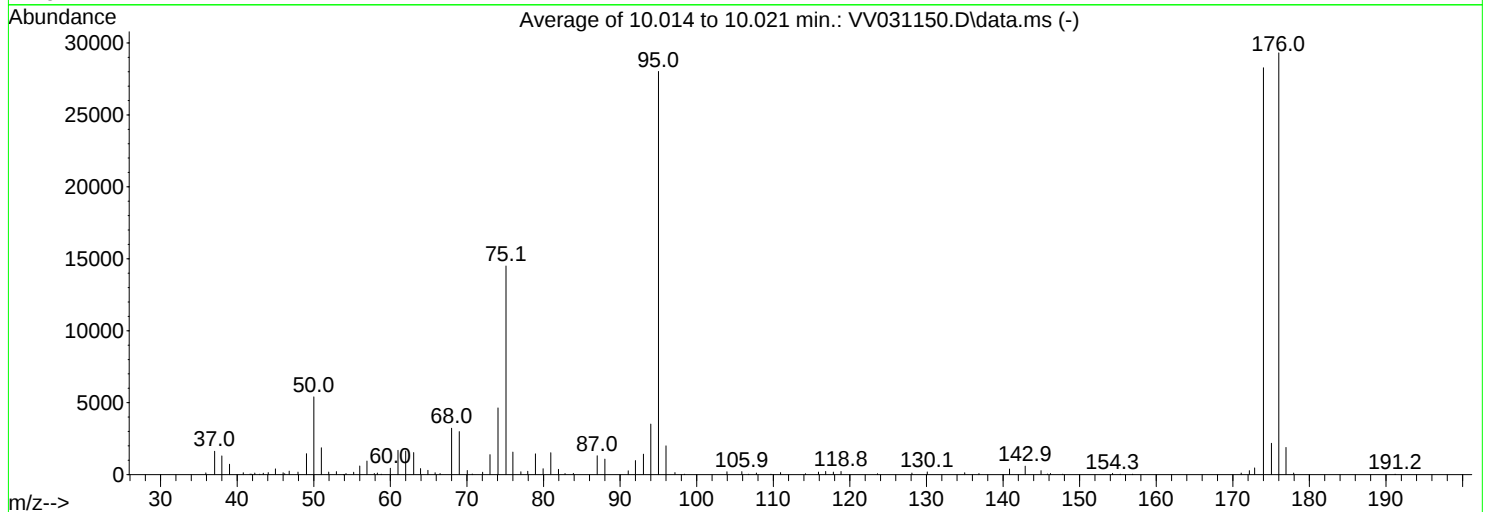


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052223\
Data File : VV031150.D
Acq On : 22 May 2023 08:32
Operator : SY/MD
Sample : BFB377
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB377

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis
Last Update : Thu May 25 01:11:46 2023

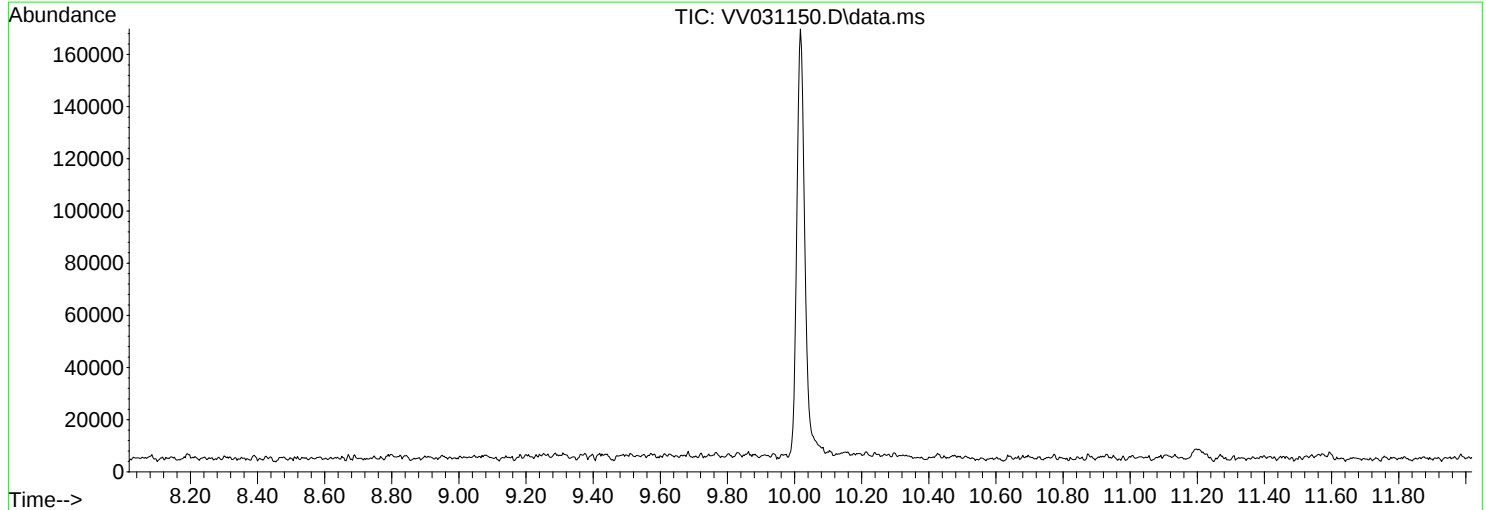

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	5407	PASS
75	95	30	80	51.7	14497	PASS
95	95	100	100	100.0	28016	PASS
96	95	5	9	7.2	2007	PASS
173	174	0.00	2	1.6	466	PASS
174	95	50	120	100.9	28272	PASS
175	174	5	9	7.7	2180	PASS
176	174	95	105	103.7	29312	PASS
177	176	5	10	6.4	1888	PASS

m/z	Abundance
35.90	950.0
36.80	254.0
38.00	451.0
39.10	129.0
40.00	176.0
41.10	143.0
43.10	135.0
44.10	223.0
46.70	140.0
47.90	153.0
51.50	123.0
52.30	119.0
53.40	105.0
54.00	118.0
55.00	147.0
55.60	122.0
56.90	133.0
59.30	106.0
71.10	121.0
71.60	102.0
72.20	119.0
72.80	121.0
74.80	107.0
77.00	169.0
79.30	129.0
80.20	121.0
83.60	107.0
85.00	148.0
88.40	140.0
92.20	101.0
98.90	113.0
103.70	105.0
117.40	103.0
139.20	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
36.00	1130.0
37.00	1656.0
38.00	1728.0
39.00	870.0
39.90	224.0
40.80	133.0
41.70	123.0
42.40	110.0
42.90	177.0
43.40	143.0
44.00	410.0
45.00	374.0
46.00	235.0
46.90	405.0
48.00	354.0
49.00	1504.0
50.00	5406.0
51.00	1953.0
51.90	139.0
53.00	179.0
53.80	128.0
54.20	112.0
55.20	162.0
56.00	630.0
57.00	1056.0
58.30	109.0
58.80	108.0
60.10	443.0
61.00	1711.0
62.00	1643.0
63.00	1573.0
64.00	391.0
64.90	274.0
65.80	136.0
68.00	3105.0
69.00	2952.0
70.10	285.0
70.70	119.0
72.00	233.0
73.00	1400.0
74.10	4736.0
75.10	14471.0
76.00	1489.0
77.10	415.0
78.00	239.0
78.90	1424.0
80.00	414.0
81.00	1435.0
81.90	362.0
82.80	114.0
83.90	119.0
87.00	1226.0
88.00	976.0
91.00	272.0
92.00	965.0
93.10	1346.0
94.00	3486.0
95.00	27456.0
96.00	2042.0
97.20	161.0
103.90	231.0
105.90	202.0
106.80	118.0
107.90	102.0
111.00	132.0
115.90	199.0
116.80	223.0
117.80	198.0
118.90	182.0
123.60	102.0
130.10	205.0
135.00	142.0
140.80	400.0
142.90	546.0
144.90	304.0
146.20	126.0
147.80	102.0
154.30	133.0
156.90	105.0
172.10	255.0
172.80	437.0
174.00	27384.0
175.00	2052.0
176.00	28208.0
176.90	1905.0
178.00	184.0
191.20	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
36.00	1080.0
37.10	1651.0
38.00	1791.0
39.00	925.0
39.80	210.0
40.80	128.0
41.20	122.0
41.90	112.0
42.30	112.0
42.90	171.0
43.40	157.0
44.00	389.0
45.00	381.0
46.00	180.0
46.90	385.0
48.00	331.0
49.10	1488.0
50.00	5471.0
51.00	1954.0
51.90	172.0
53.00	212.0
53.80	118.0
54.20	113.0
55.20	169.0
56.00	635.0
57.00	1116.0
57.90	113.0
58.30	117.0
60.00	458.0
61.00	1744.0
62.00	1647.0
63.00	1623.0
64.00	436.0
64.90	325.0
65.80	146.0
66.50	108.0
68.00	3359.0
69.00	3023.0
70.00	272.0
70.90	155.0
72.00	289.0
73.00	1469.0
74.00	4732.0
75.10	14920.0
76.00	1656.0
77.10	399.0
77.90	277.0
79.00	1480.0
80.00	407.0
80.90	1554.0
82.00	367.0
82.80	131.0
83.90	133.0
87.00	1406.0
88.00	1075.0
91.00	271.0
92.00	1161.0
93.00	1424.0
94.00	3587.0
95.00	28880.0
96.00	2077.0
97.20	159.0
104.00	196.0
105.90	230.0
107.80	109.0
110.90	144.0
114.20	103.0
115.90	182.0
116.90	209.0
117.90	184.0
118.90	235.0
123.60	113.0
128.10	147.0
130.10	180.0
135.00	146.0
136.90	110.0
140.80	380.0
142.90	605.0
144.90	293.0
146.20	121.0
154.30	129.0
171.10	162.0
172.20	285.0
172.90	468.0
174.00	29136.0
175.00	2189.0
176.00	30640.0
176.90	1960.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377

m/z	Abundance
36.00	996.0
37.10	1567.0
38.00	1738.0
39.00	763.0
40.80	148.0
41.20	138.0
42.20	121.0
42.90	168.0
44.10	319.0
45.00	436.0
46.20	185.0
46.90	349.0
48.00	313.0
49.10	1373.0
50.00	5345.0
51.00	1712.0
52.00	213.0
52.90	233.0
53.80	110.0
54.80	156.0
55.20	186.0
56.00	535.0
57.00	1081.0
57.90	130.0
58.30	119.0
59.90	426.0
61.00	1634.0
62.00	1610.0
63.10	1416.0
63.90	433.0
64.90	313.0
65.90	134.0
66.50	132.0
68.00	3227.0
69.00	3010.0
70.00	299.0
70.90	172.0
72.10	322.0
73.00	1298.0
74.10	4457.0
75.10	14099.0
76.00	1563.0
77.10	285.0
77.90	197.0
79.00	1444.0
79.90	420.0
80.90	1573.0
82.00	356.0
87.00	1300.0
88.00	1195.0
91.10	245.0
92.00	1103.0
93.00	1493.0
94.00	3483.0
95.00	27712.0
96.00	1901.0
97.10	125.0
98.40	105.0
104.00	178.0
105.90	208.0
107.70	113.0
109.70	104.0
111.00	143.0
114.20	100.0
115.90	149.0
116.90	236.0
117.90	167.0
118.80	254.0
128.10	191.0
130.10	171.0
135.00	126.0
136.80	123.0
140.90	389.0
142.90	615.0
145.00	243.0
145.80	132.0
155.30	100.0
171.10	189.0
172.10	306.0
172.90	493.0
174.00	28296.0
175.10	2298.0
176.00	29088.0
177.00	1798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB377