




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052224\
Data File : VV035676.D
Acq On : 22 May 2024 15:28
Operator : SY/MD
Sample : P2547-07
Misc : 5.14g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q0

Manual IntegrationsAPPROVED

Quant Time: May 23 02:24:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 23 02:17:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

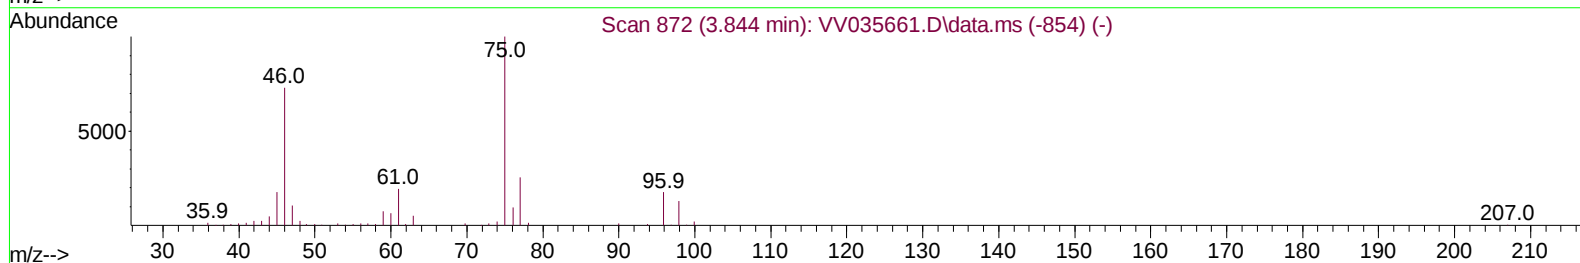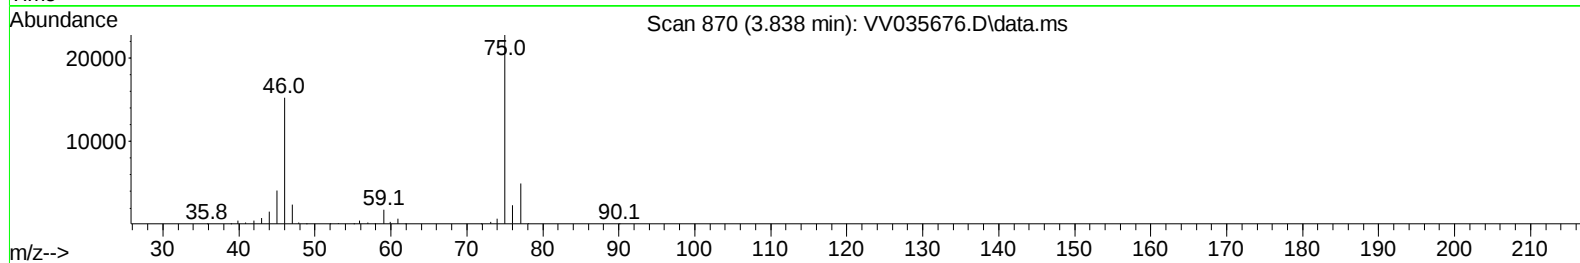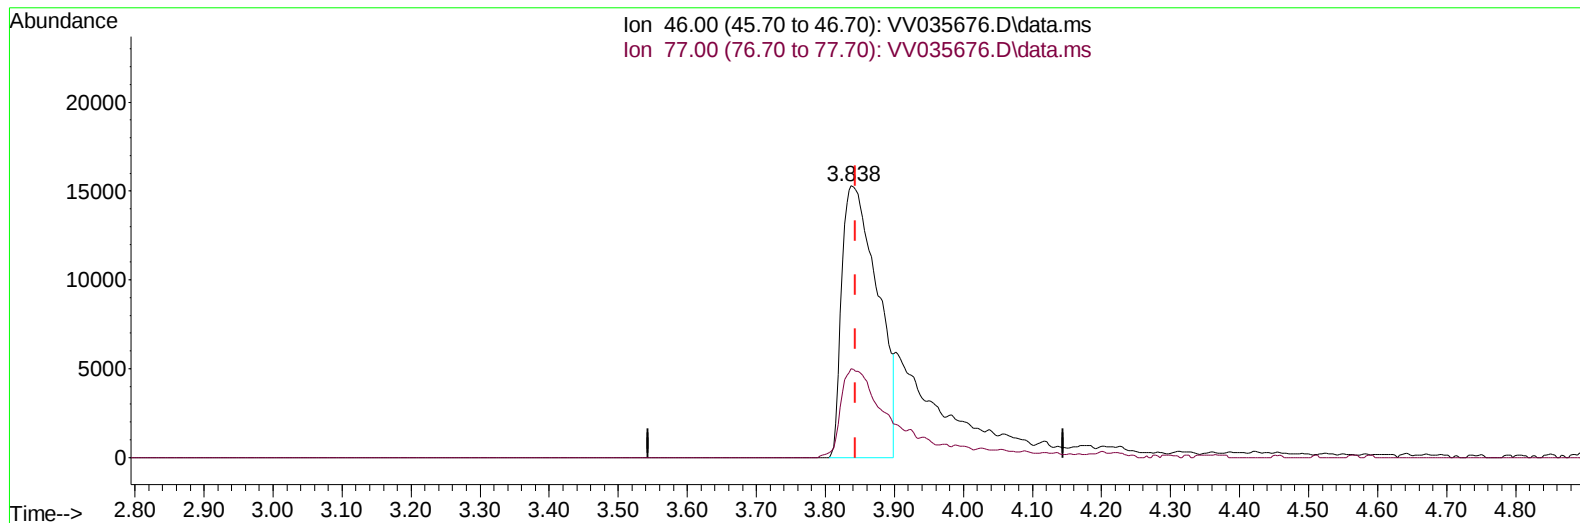

TIC: VV035676.D\data.ms

(21) 2-Butanone-d5 (S)

3.838min (-0.007) 32.76 ug/L

response 55138

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	36.55#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052224\
Data File : VV035676.D
Acq On : 22 May 2024 15:28
Operator : SY/MD
Sample : P2547-07
Misc : 5.14g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q0

Manual IntegrationsAPPROVED

Quant Time: May 23 02:24:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 23 02:17:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

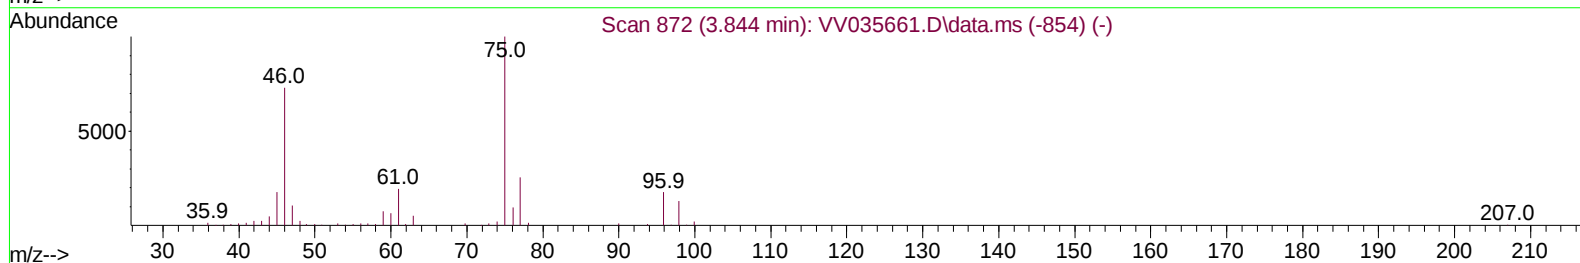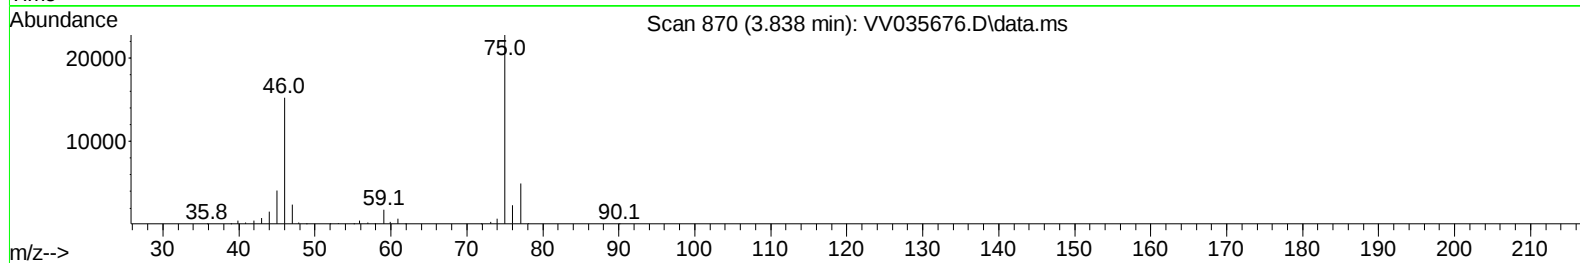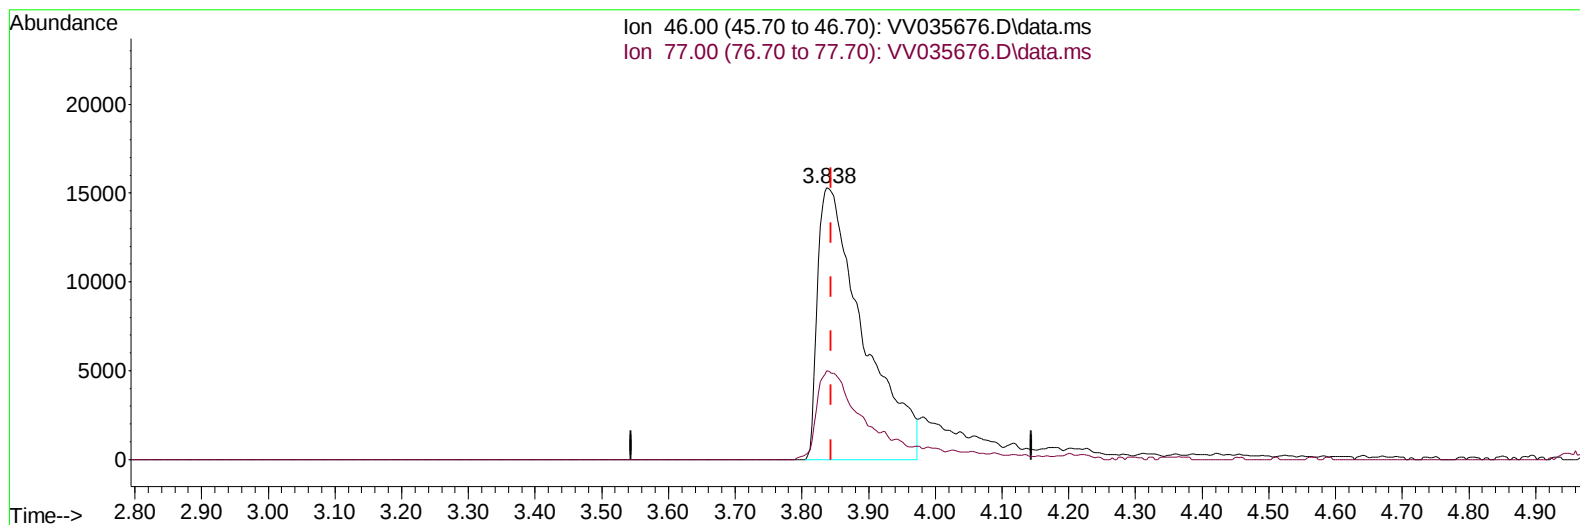

TIC: VV035676.D\data.ms

(21) 2-Butanone-d5 (S)

3.838min (-0.007) 43.07 ug/L m

response 72491

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	27.80#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052224\
 Data File : VV035676.D
 Acq On : 22 May 2024 15:28
 Operator : SY/MD
 Sample : P2547-07
 Misc : 5.14g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q0

Manual IntegrationsAPPROVED

Quant Time: May 23 02:24:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 23 02:17:29 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
 Supervised By :Mahesh Dadoda 05/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		383757	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		366043	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		144098	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		99387	16.756	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.040%		
7) Chloroethane-d5	1.526	69		94221	19.691	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	78.760%		
11) 1,1-Dichloroethene-d2	2.050	65		46064	17.542	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	70.160%		
21) 2-Butanone-d5	3.838	46		72491m	43.065	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	86.140%		
24) Chloroform-d	4.246	84		246583	21.613	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	86.440%		
26) 1,2-Dichloroethane-d4	4.940	65		140286	24.873	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	99.480%		
32) Benzene-d6	4.957	84		408628	20.394	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	81.560%		
36) 1,2-Dichloropropane-d6	5.985	67		151739	24.539	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	98.160%		
41) Toluene-d8	7.243	98		302065	16.939	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	67.760%		
43) trans-1,3-Dichloroprop...	7.558	79		47558	17.983	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.920%		
47) 2-Hexanone-d5	8.034	63		44353	39.889	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	79.780%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84		147969	24.833	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	99.320%		
66) 1,2-Dichlorobenzene-d4	11.561	152		116272	23.250	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	93.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052224\
Data File : VV035676.D
Acq On : 22 May 2024 15:28
Operator : SY/MD
Sample : P2547-07
Misc : 5.14g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q0

Manual IntegrationsAPPROVED

Quant Time: May 23 02:24:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 23 02:17:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

