


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052224\
Data File : VV035660.D
Acq On : 22 May 2024 08:22
Operator : SY/MD
Sample : BFB306
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB306

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Title : VOC Analysis
Last Update : Sat May 25 02:41:55 2024

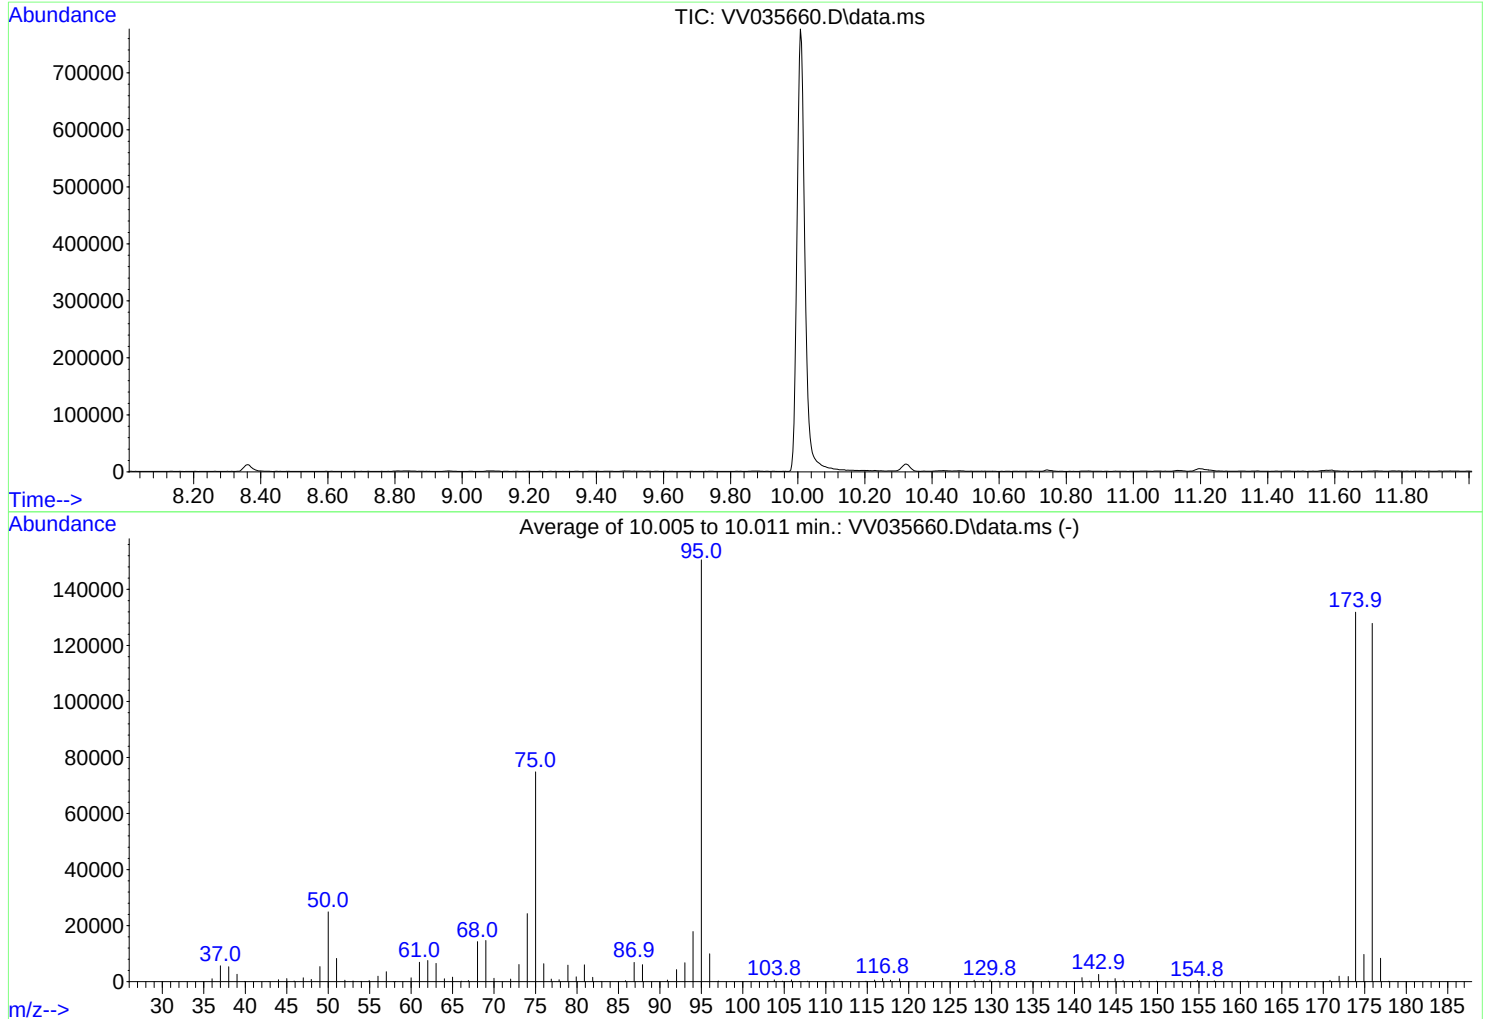

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	24893	PASS
75	95	30	80	49.7	74851	PASS
95	95	100	100	100.0	150549	PASS
96	95	5	9	6.6	9927	PASS
173	174	0.00	2	1.4	1810	PASS
174	95	50	120	87.6	131867	PASS
175	174	5	9	7.4	9705	PASS
176	174	95	101	97.0	127888	PASS
177	176	5	9	6.5	8326	PASS

m/z	Abundance
39.90	361.0
44.00	542.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
36.00	1109.0
37.00	5649.0
38.00	5112.0
39.00	2564.0
40.00	507.0
44.00	1243.0
45.00	981.0
45.90	270.0
47.00	1415.0
47.90	817.0
49.00	5481.0
50.00	24672.0
51.00	8028.0
52.00	480.0
53.00	211.0
54.00	152.0
55.00	424.0
56.00	1980.0
57.00	3453.0
57.90	129.0
60.00	1444.0
61.00	6802.0
62.00	7276.0
63.00	6649.0
64.00	1099.0
65.00	1560.0
66.10	206.0
66.90	377.0
68.00	13991.0
69.00	14395.0
70.00	1091.0
72.00	920.0
73.00	5951.0
74.00	23760.0
75.00	73224.0
76.00	6420.0
76.90	1016.0
77.90	677.0
78.90	5866.0
79.90	1695.0
80.90	5862.0
81.90	1482.0
82.80	132.0
85.90	318.0
86.90	6575.0
87.90	6216.0
90.90	543.0
92.00	4182.0
93.00	6621.0
94.00	17504.0
95.00	145792.0
96.00	9590.0
97.10	209.0
103.80	661.0
104.80	174.0
105.90	651.0
106.80	128.0
107.80	184.0
110.90	188.0
111.90	102.0
114.90	144.0
115.90	544.0
116.90	1145.0
117.80	496.0
118.90	1048.0
127.90	547.0
128.80	181.0
129.80	479.0
130.80	225.0
134.80	201.0
136.80	179.0
138.70	101.0
140.90	1340.0
141.80	144.0
142.90	2427.0
143.90	178.0
144.90	1119.0
145.80	320.0
146.90	160.0
147.90	351.0
148.80	134.0
149.90	158.0
152.90	146.0
154.80	395.0
156.80	279.0
158.70	117.0
160.80	159.0
170.80	406.0
171.90	1805.0
173.00	1739.0
173.90	124496.0
174.90	9120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

175.90	120576.0
176.90	7929.0
177.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
36.00	1098.0
37.00	5866.0
38.00	5432.0
39.00	2730.0
40.10	506.0
42.80	110.0
44.00	1274.0
45.00	1083.0
45.90	231.0
47.00	1372.0
47.90	846.0
49.00	5488.0
50.00	25648.0
51.00	8571.0
52.00	533.0
53.00	260.0
53.90	151.0
55.00	378.0
56.00	2021.0
57.00	3642.0
58.10	109.0
60.00	1469.0
61.00	7131.0
62.00	7885.0
63.00	6698.0
64.00	1057.0
65.00	1654.0
66.00	211.0
66.90	420.0
68.00	14791.0
69.00	15152.0
70.00	1235.0
72.00	961.0
73.00	6307.0
74.00	25120.0
75.00	77488.0
76.00	6652.0
76.90	908.0
77.80	730.0
78.90	6096.0
79.90	1732.0
80.90	6224.0
81.90	1631.0
82.90	128.0
85.90	345.0
86.90	7198.0
87.90	6226.0
90.90	594.0
92.00	4466.0
93.00	6939.0
94.00	18504.0
95.00	155456.0
96.00	10275.0
97.00	222.0
102.80	117.0
103.80	692.0
104.80	192.0
105.90	667.0
106.80	161.0
107.80	157.0
110.90	182.0
111.90	116.0
114.90	163.0
115.90	572.0
116.90	1193.0
117.80	510.0
118.90	1071.0
127.90	554.0
128.80	187.0
129.80	580.0
130.80	217.0
134.80	216.0
136.80	198.0
140.90	1465.0
141.80	161.0
142.90	2698.0
143.90	158.0
144.90	1144.0
145.90	331.0
146.90	133.0
147.80	334.0
148.80	140.0
149.90	153.0
152.90	182.0
154.80	456.0
156.90	328.0
158.80	111.0
160.90	190.0
170.80	477.0
171.90	2019.0
173.00	1858.0
173.90	136512.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

174.90	10069.0
175.90	132160.0
176.90	8534.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
36.00	953.0
37.00	5450.0
38.00	5389.0
39.00	2552.0
40.10	500.0
42.90	133.0
44.00	1241.0
45.00	1151.0
45.90	190.0
47.00	1267.0
48.00	800.0
49.00	5117.0
50.00	24360.0
51.00	8176.0
52.00	472.0
53.00	265.0
53.90	136.0
54.90	342.0
56.00	1908.0
57.00	3484.0
58.10	115.0
60.00	1307.0
61.00	6755.0
62.00	7539.0
63.00	6239.0
64.00	1028.0
65.00	1608.0
66.00	199.0
66.90	454.0
68.00	14029.0
69.00	14481.0
70.00	1218.0
72.00	832.0
73.00	6074.0
74.00	24024.0
75.00	73840.0
76.00	6104.0
76.90	769.0
77.80	684.0
78.90	5708.0
79.90	1640.0
80.90	5970.0
81.90	1569.0
83.00	120.0
85.80	319.0
86.90	6830.0
87.90	5776.0
90.90	587.0
92.00	4288.0
93.00	6692.0
94.00	17640.0
95.00	150400.0
96.00	9916.0
97.00	234.0
102.90	102.0
103.80	600.0
104.80	185.0
105.80	570.0
106.80	157.0
107.80	140.0
110.90	142.0
111.90	116.0
114.80	175.0
115.90	541.0
116.80	1111.0
117.80	536.0
118.90	959.0
127.90	545.0
128.80	193.0
129.80	611.0
130.80	180.0
134.70	240.0
136.90	191.0
140.90	1435.0
141.80	182.0
142.90	2675.0
144.00	144.0
144.90	1040.0
145.90	340.0
147.80	337.0
148.80	128.0
149.90	148.0
151.70	102.0
152.80	184.0
154.80	479.0
156.90	350.0
158.90	131.0
160.90	217.0
170.80	541.0
171.90	2090.0
173.00	1833.0
173.90	134592.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

174.90	9925.0
175.90	130928.0
176.90	8514.0
177.90	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306