

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV052319\
Quantitation Report (QT Reviewed)


Data File : VV011030.D
Acq On : 23 May 2019 16:38
Operator : SY/MD
Sample : K3016-12MSD
Misc : 5.53G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51C9

Manual Integrations
APPROVED

MMDadoda
5/28/2019 2:55:03 AM

Quant Time: May 24 08:33:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 08:16:13 2019
Response via : Initial Calibration

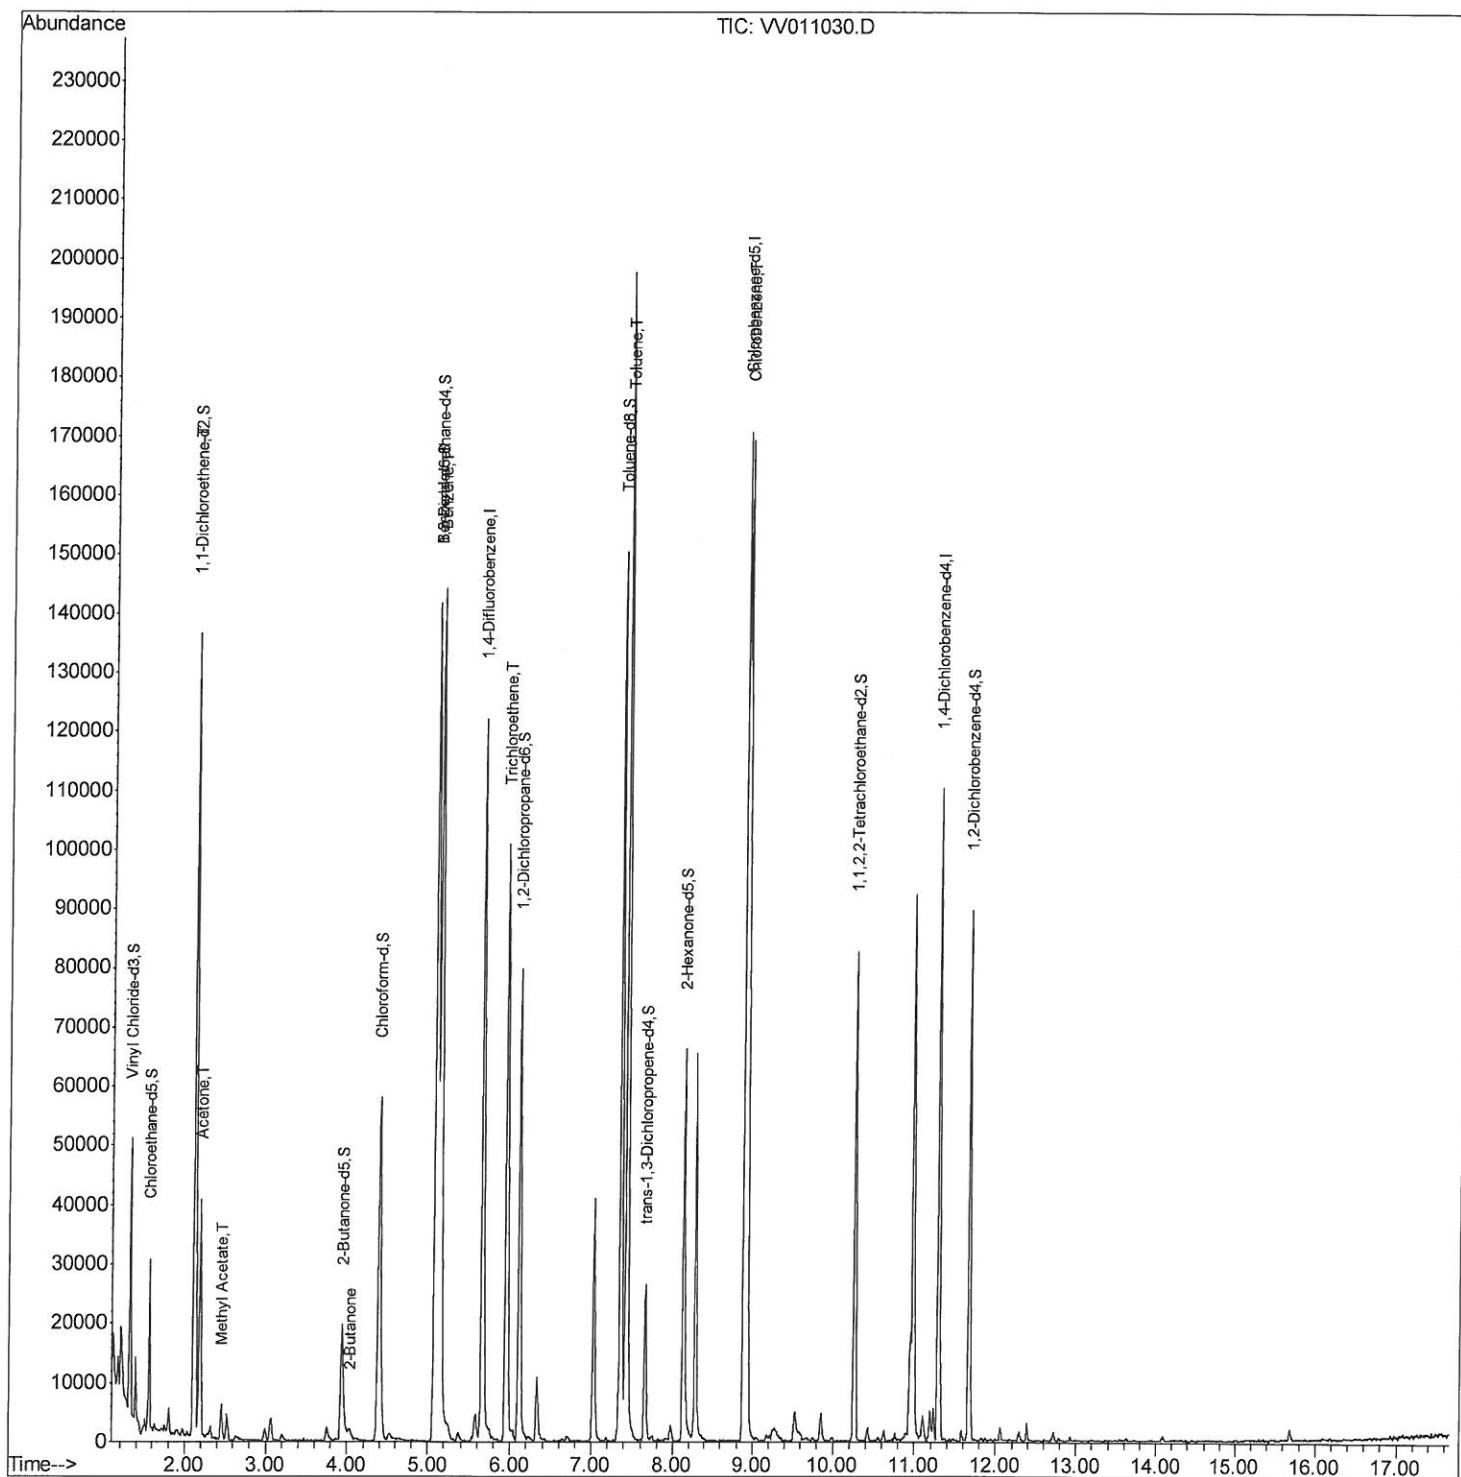

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV052319\
Quantitation Report (Qedit)




Data File : VV011030.D
Acq On : 23 May 2019 16:38
Operator : SY/MD
Sample : K3016-12MSD
Misc : 5.53G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51C9

Manual Integrations
APPROVED

MMDadoda
5/28/2019 2:55:03 AM

Quant Time: May 24 08:19:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 08:16:13 2019
Response via : Initial Calibration

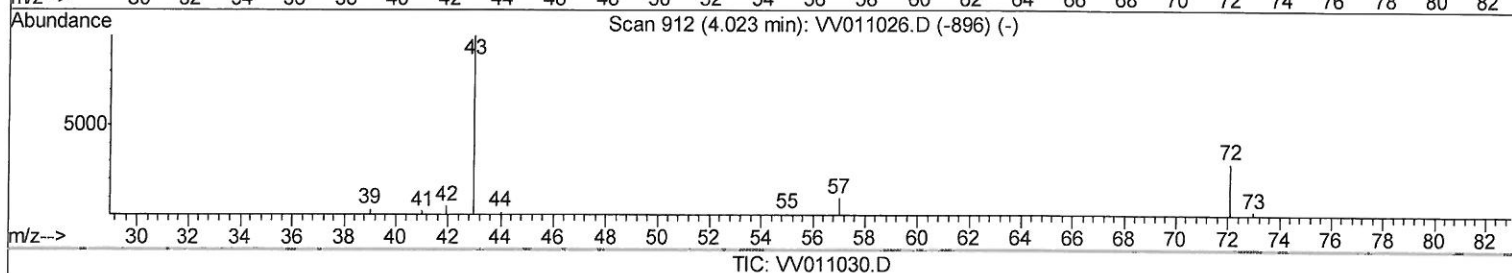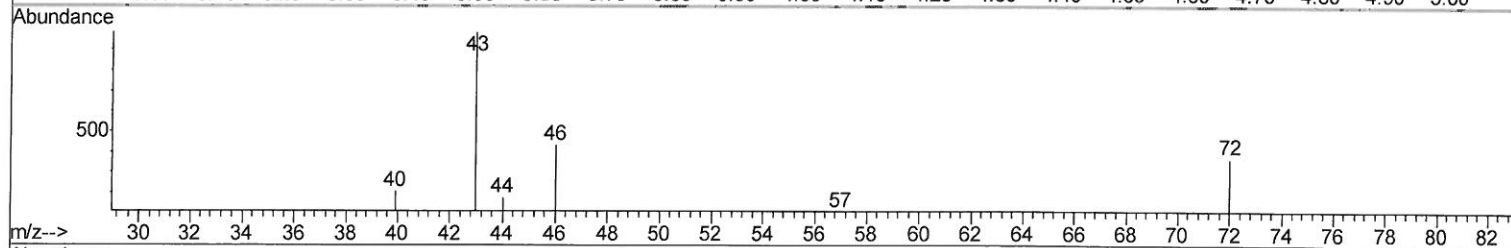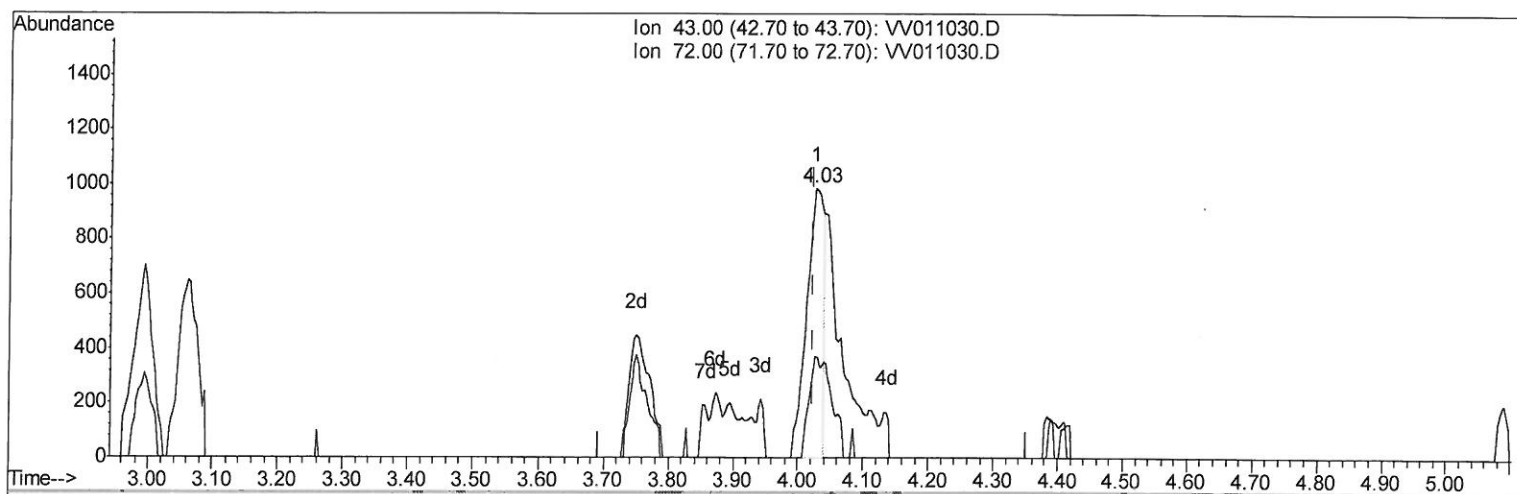

(21) 2-Butanone

4.026min (+0.003) 3.20ug/L

response 1771

Ion	Exp%	Act%
43.00	100	100
72.00	26.20	26.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV052319\
Quantitation Report (Qedit)




Data File : VV011030.D
Acq On : 23 May 2019 16:38
Operator : SY/MD
Sample : K3016-12MSD
Misc : 5.53G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51C9

Manual Integrations
APPROVED

MMDadoda
5/28/2019 2:55:03 AM

Quant Time: May 24 08:19:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 08:16:13 2019
Response via : Initial Calibration

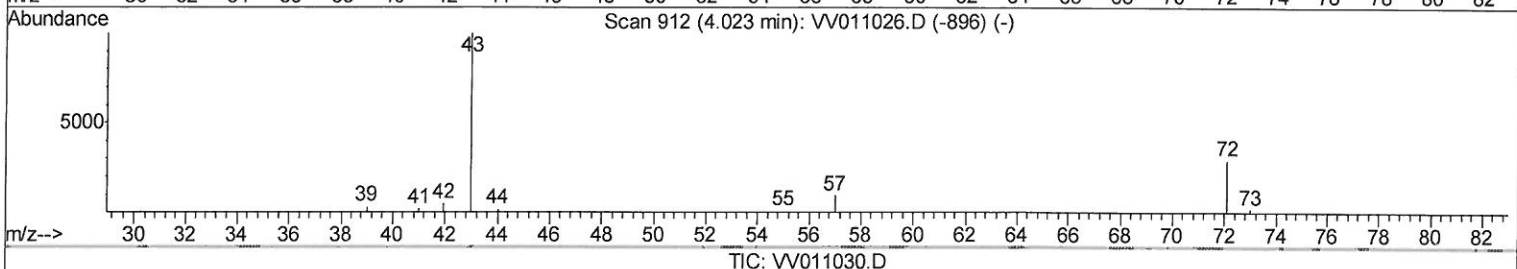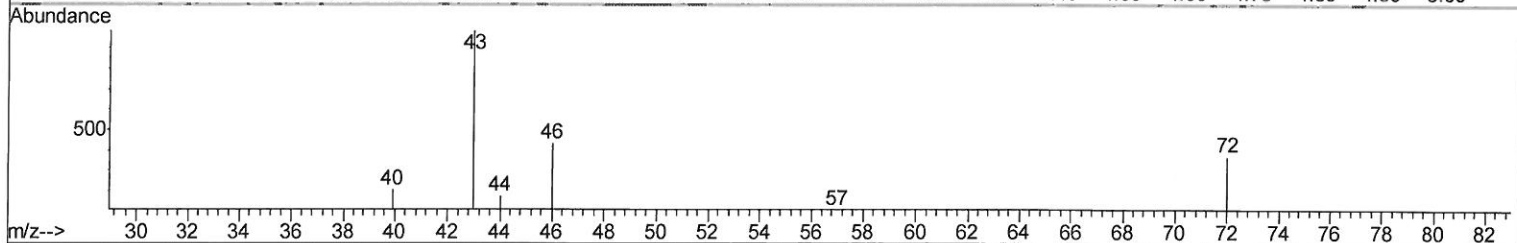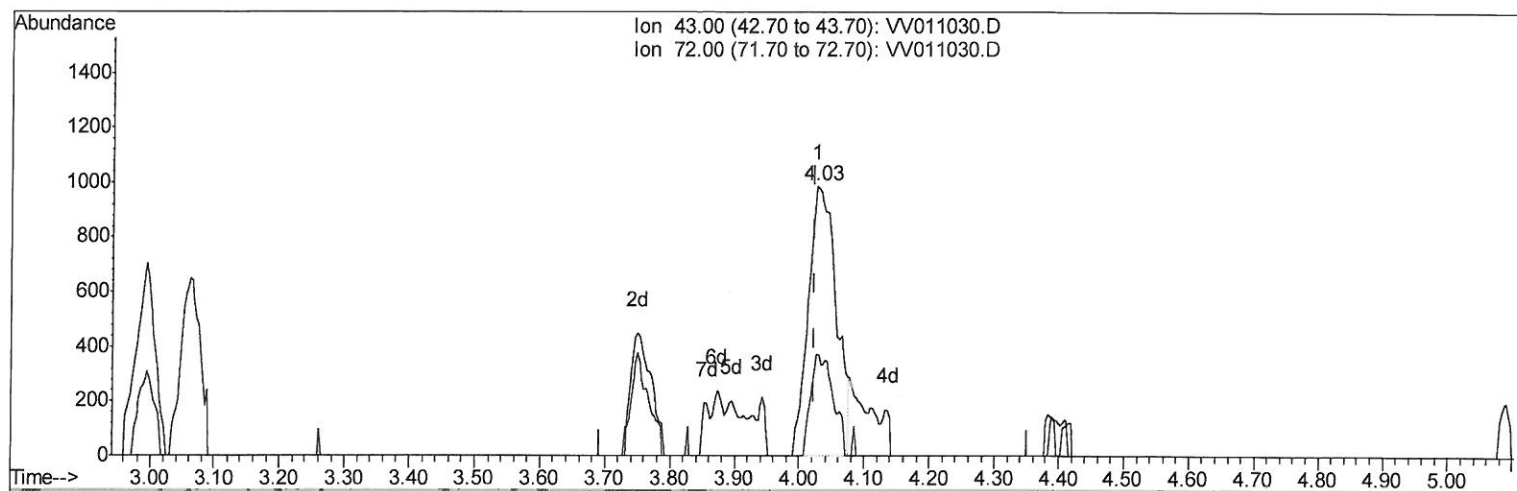

(21) 2-Butanone

4.026min (+0.003) 5.29ug/L m

205/28/19SY

response 2925

Ion	Exp%	Act%
43.00	100	100
72.00	26.20	16.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV052319\
Quantitation Report (QT Reviewed)

Data File : VV011030.D
Acq On : 23 May 2019 16:38
Operator : SY/MD
Sample : K3016-12MSD
Misc : 5.53G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51C9

Manual Integrations
APPROVED

MMDadoda
5/28/2019 2:55:03 AM

Quant Time: May 24 08:33:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 08:16:13 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	106448	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	92878	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	28277	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24723	20.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.48%
7) Chloroethane-d5	1.56	69	17451	21.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.96%
10) 1,1-Dichloroethene-d2	2.12	63	48940	20.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.88%
20) 2-Butanone-d5	3.94	46	30178	72.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	144.14%#
24) Chloroform-d	4.40	84	58767	21.31	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.24%
26) 1,2-Dichloroethane-d4	5.08	65	36442	22.43	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.72%
29) Benzene-d6	5.09	84	123709	24.40	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.60%
33) 1,2-Dichloropropane-d6	6.12	67	40997	25.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.76%
37) Toluene-d8	7.36	98	103308	21.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.68%
38) trans-1,3-Dichloropropene-	7.66	79	15423	23.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.24%
39) 2-Hexanone-d5	8.13	63	22872	76.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	152.22%#
48) 1,1,2,2-Tetrachloroethane-	10.26	84	40907	25.43	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.72%
61) 1,2-Dichlorobenzene-d4	11.67	152	22183	19.32	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.28%

Target Compounds					Qvalue
12) 1,1-Dichloroethene	2.13	96	26375	23.480 ug/L	98
13) Acetone	2.19	43	36641	90.738 ug/L	98
15) Methyl Acetate	2.45	43	6162	7.942 ug/L	96
21) 2-Butanone	4.03	43	2925m	5.293 ug/L	96
34) Benzene	5.14	78	147309	27.513 ug/L	100
35) Trichloroethene	5.96	95	36083	24.392 ug/L	95
44) Toluene	7.43	91	150114	25.265 ug/L	99
52) Chlorobenzene	8.92	112	87702	21.535 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed