


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052319\
 Data File : VV011025.D
 Acq On : 23 May 2019 11:49
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052019S.M
 Title : VOC Analysis
 Last Update : Tue May 28 02:57:33 2019

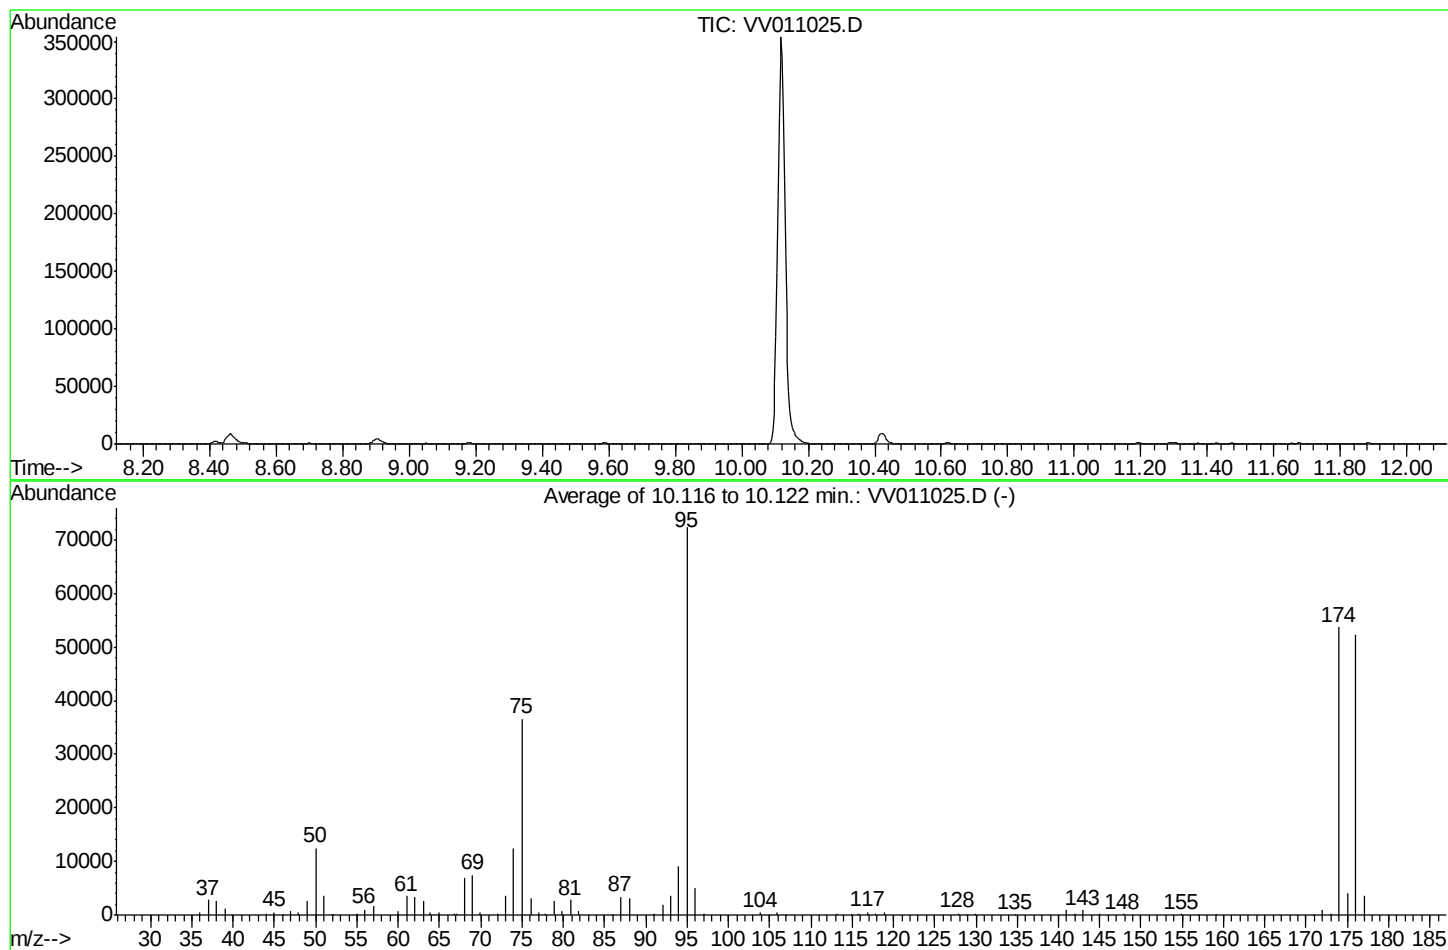

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	12500	PASS
75	95	30	80	50.5	36549	PASS
95	95	100	100	100.0	72322	PASS
96	95	5	9	6.8	4942	PASS
173	174	0.00	2	0.5	265	PASS
174	95	50	120	74.2	53672	PASS
175	174	5	9	7.4	3995	PASS
176	174	95	101	97.2	52186	PASS
177	176	5	9	6.7	3503	PASS

m/z	Abundance
39.80	130.0
44.00	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	607.0
37.00	2794.0
38.00	2835.0
39.00	1197.0
39.80	184.0
44.00	578.0
44.90	551.0
46.00	106.0
46.90	801.0
47.90	443.0
49.00	2671.0
50.00	12383.0
51.00	3650.0
51.90	152.0
55.00	255.0
55.90	1046.0
57.00	1697.0
59.90	599.0
61.00	3521.0
62.00	3486.0
63.00	2676.0
63.90	487.0
65.00	543.0
66.80	255.0
68.00	7036.0
69.00	7370.0
70.00	526.0
72.00	369.0
73.00	3496.0
74.00	12808.0
75.00	36096.0
76.10	3184.0
77.10	433.0
77.80	271.0
78.90	2538.0
79.90	732.0
80.90	2794.0
81.90	625.0
85.80	130.0
86.90	3355.0
88.00	3076.0
91.00	336.0
92.00	1965.0
93.00	3595.0
94.00	8783.0
95.00	71672.0
96.00	5091.0
97.00	132.0
103.90	405.0
106.00	362.0
106.90	111.0
113.10	144.0
115.80	289.0
116.90	587.0
117.90	258.0
118.90	475.0
127.90	279.0
128.90	106.0
130.00	237.0
140.90	859.0
142.00	148.0
143.00	917.0
145.00	236.0
147.90	118.0
154.90	181.0
156.90	118.0
159.00	108.0
171.90	806.0
174.00	51072.0
175.00	3807.0
176.00	49256.0
177.00	3463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	605.0
37.00	2893.0
38.00	2842.0
39.00	1175.0
39.80	206.0
44.00	509.0
45.00	525.0
46.90	802.0
47.90	450.0
49.00	2717.0
50.00	12989.0
51.00	3796.0
51.90	168.0
55.00	237.0
55.90	1099.0
57.00	1753.0
59.90	688.0
61.00	3709.0
62.00	3542.0
63.00	2665.0
63.90	372.0
65.00	566.0
66.80	225.0
67.10	219.0
68.00	7217.0
69.00	7730.0
69.90	590.0
72.00	372.0
73.00	3703.0
74.00	12897.0
75.00	37840.0
76.00	3281.0
77.00	512.0
77.80	300.0
79.00	2754.0
79.90	787.0
80.90	2947.0
81.90	670.0
85.80	116.0
86.90	3616.0
88.00	3150.0
91.00	335.0
92.00	2038.0
93.00	3717.0
94.00	9476.0
95.00	74888.0
96.00	5118.0
97.00	146.0
103.90	469.0
104.90	107.0
106.00	416.0
113.10	164.0
114.80	128.0
115.80	343.0
116.90	581.0
117.80	247.0
118.90	554.0
127.90	285.0
128.90	133.0
129.90	264.0
134.80	103.0
140.90	890.0
142.00	155.0
143.00	879.0
145.00	216.0
147.90	132.0
154.90	215.0
156.90	115.0
159.00	109.0
172.00	900.0
174.00	55536.0
175.00	4138.0
176.00	54272.0
177.00	3610.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	542.0
37.00	2783.0
38.00	2526.0
39.00	1105.0
39.80	204.0
44.00	469.0
45.00	458.0
47.00	763.0
47.90	388.0
49.00	2511.0
50.00	12128.0
51.00	3641.0
52.10	159.0
55.00	207.0
55.90	1083.0
57.00	1718.0
59.90	708.0
61.00	3334.0
62.00	3291.0
63.00	2480.0
63.90	261.0
65.00	513.0
66.80	171.0
67.10	187.0
68.00	6894.0
69.00	7343.0
69.90	584.0
72.00	355.0
73.00	3450.0
74.00	11797.0
75.00	35712.0
76.00	3051.0
77.00	451.0
77.80	286.0
79.00	2648.0
79.80	700.0
80.90	2764.0
81.90	659.0
85.80	107.0
87.00	3367.0
88.00	2988.0
91.00	294.0
92.00	2018.0
93.00	3266.0
94.00	9141.0
95.00	70408.0
96.00	4618.0
97.00	139.0
103.90	397.0
104.90	118.0
105.90	416.0
113.10	117.0
114.90	143.0
115.80	341.0
116.90	520.0
117.80	267.0
118.90	517.0
127.90	265.0
128.90	144.0
129.90	275.0
134.70	134.0
140.90	814.0
141.90	166.0
143.00	801.0
144.90	199.0
147.90	165.0
154.90	186.0
157.00	104.0
170.90	110.0
172.00	893.0
173.00	797.0
174.00	54408.0
175.00	4041.0
176.00	53032.0
177.00	3437.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62