

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031190.D
 Acq On : 23 May 2023 15:19
 Operator : SY/MD
 Sample : 02861-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK6

Quant Time: May 24 01:35:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 24 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	177428	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	164822	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	82548	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	68023	44.860	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.720%
7) Chloroethane-d5	1.535	69	60616	51.891	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.780%
11) 1,1-Dichloroethene-d2	2.066	65	33198	46.688	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.380%
21) 2-Butanone-d5	3.799	46	72180	89.334	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.330%
24) Chloroform-d	4.259	84	128423	47.874	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.740%
26) 1,2-Dichloroethane-d4	4.950	65	94477	52.120	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.240%
32) Benzene-d6	4.969	84	229489	51.361	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.720%
36) 1,2-Dichloropropane-d6	5.995	67	68167	50.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.980%
41) Toluene-d8	7.249	98	208075	49.895	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.800%
43) trans-1,3-Dichloroprop...	7.558	79	33657	50.178	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.360%
47) 2-Hexanone-d5	8.034	63	43720	83.873	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.870%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	87393	43.583	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.160%
66) 1,2-Dichlorobenzene-d4	11.567	152	80501	54.268	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.540%
Target Compounds						
39) cis-1,3-Dichloropropene	6.918	75	3358	2.004	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031190.D
Acq On : 23 May 2023 15:19
Operator : SY/MD
Sample : 02861-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK6

Quant Time: May 24 01:35:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 24 01:27:41 2023
Response via : Initial Calibration

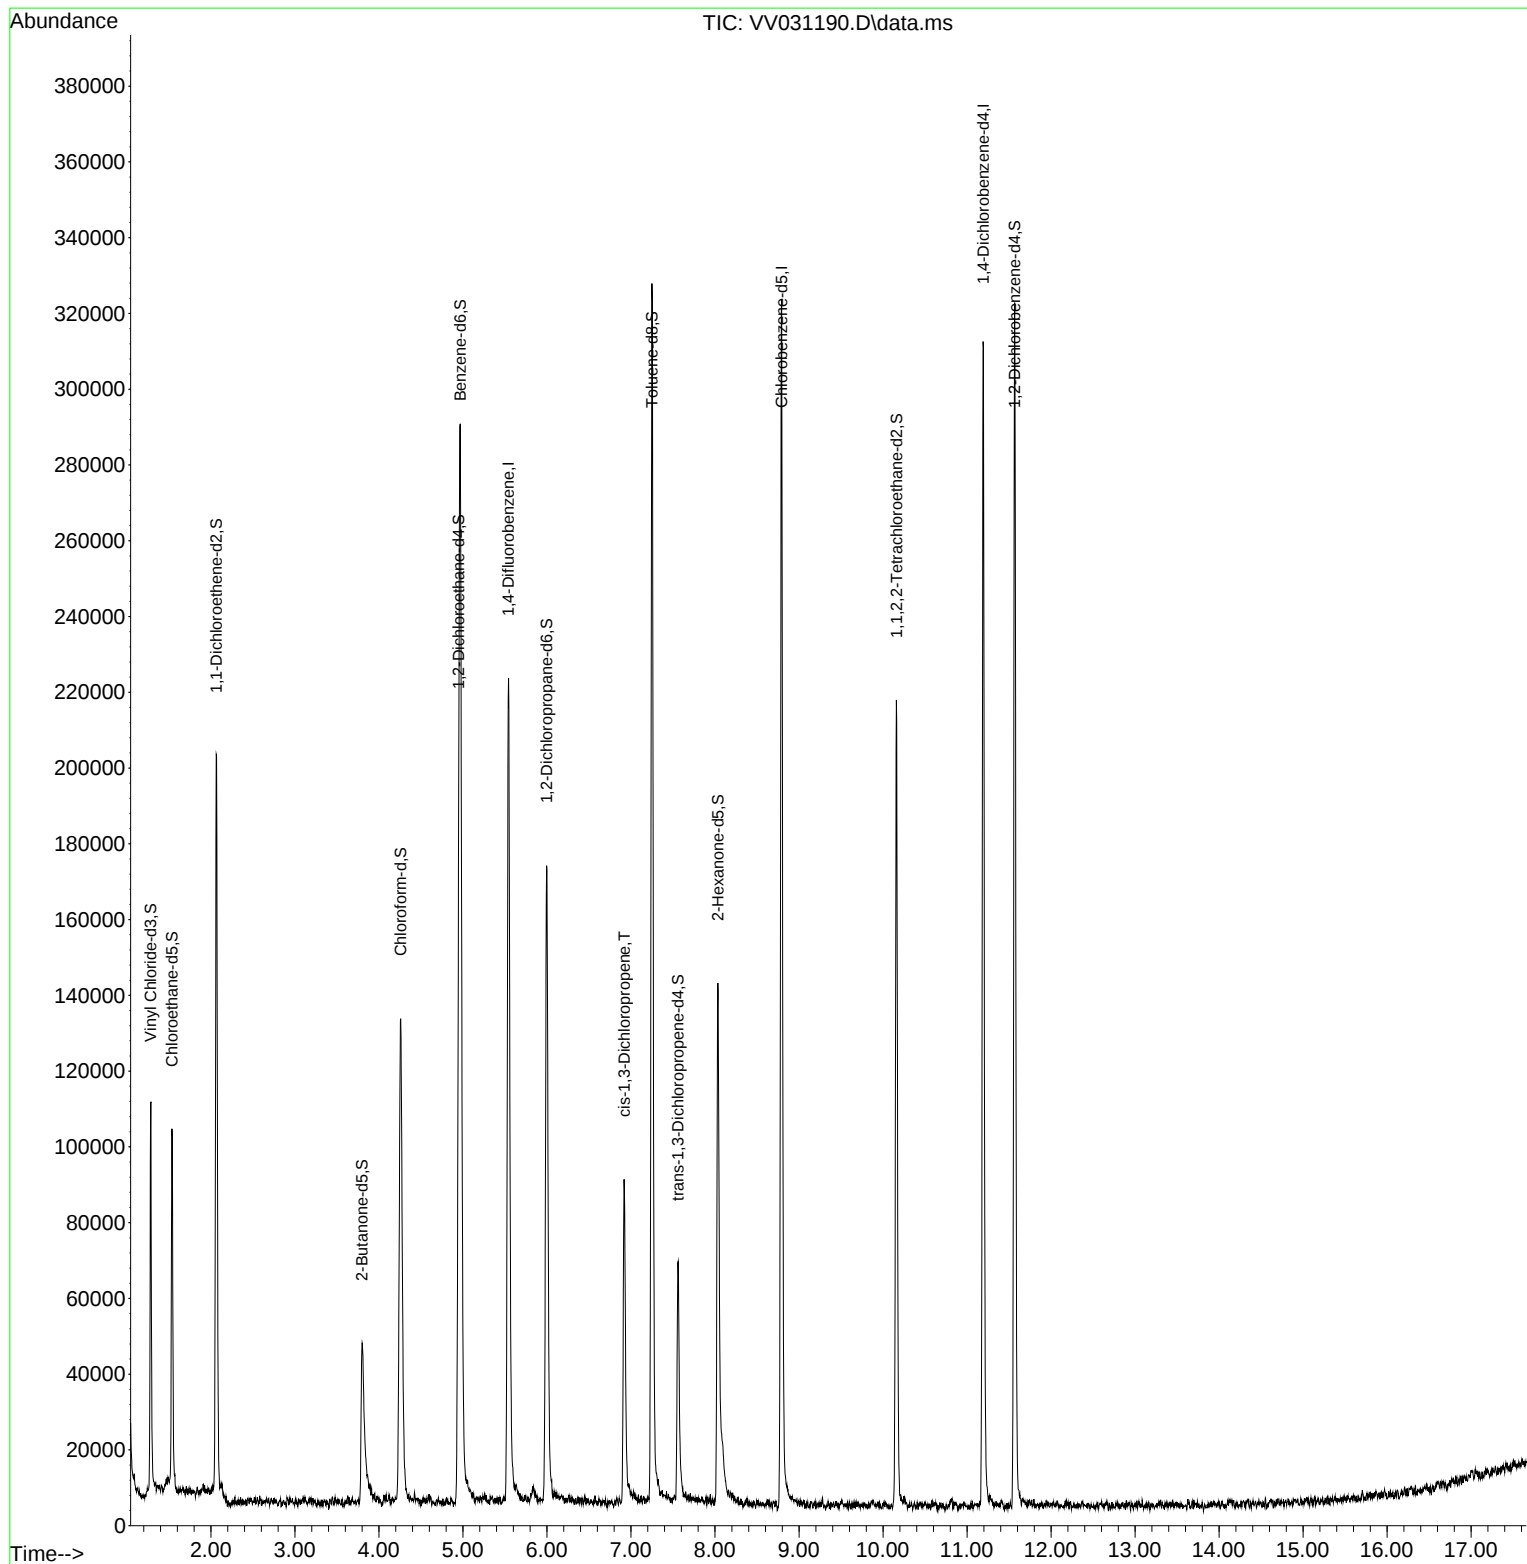

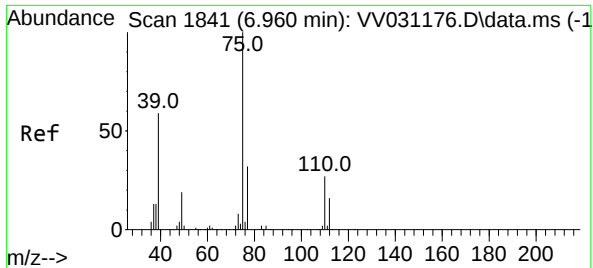

#39
 cis-1,3-Dichloropropene
 Concen: 2.004 ug/L
 RT: 6.918 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV031190.D
 Acq: 23 May 2023 15:19

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK6

Tgt Ion: 75 Resp: 3358
 Ion Ratio Lower Upper
 75 100
 77 39.4 22.3 41.3

