




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031195.D
 Acq On : 23 May 2023 17:14
 Operator : SY/MD
 Sample : 02865-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 3

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX58

Manual IntegrationsAPPROVED

Quant Time: May 24 01:36:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 24 01:27:41 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

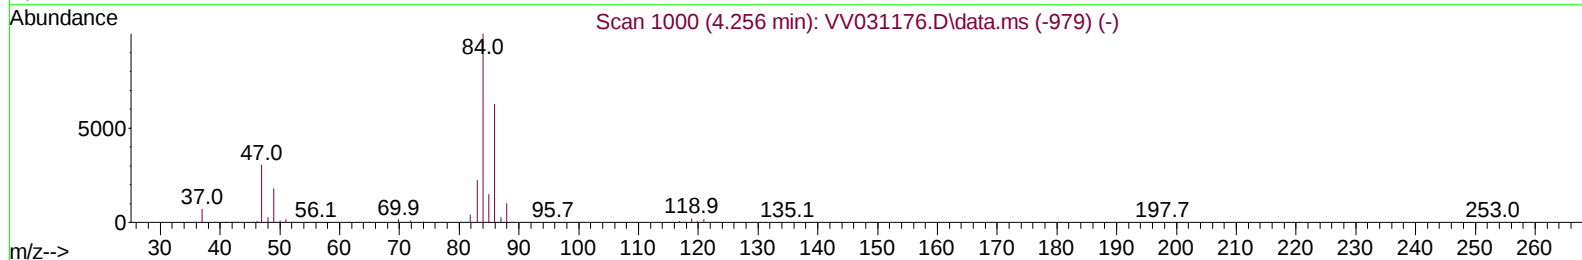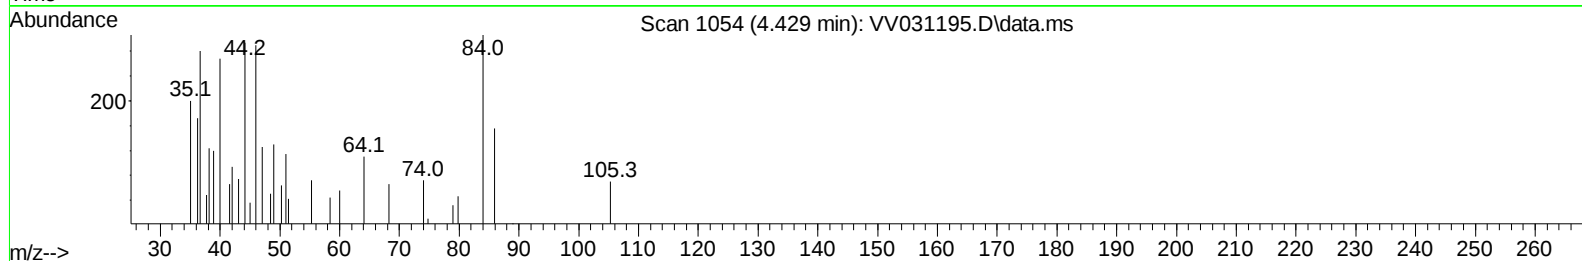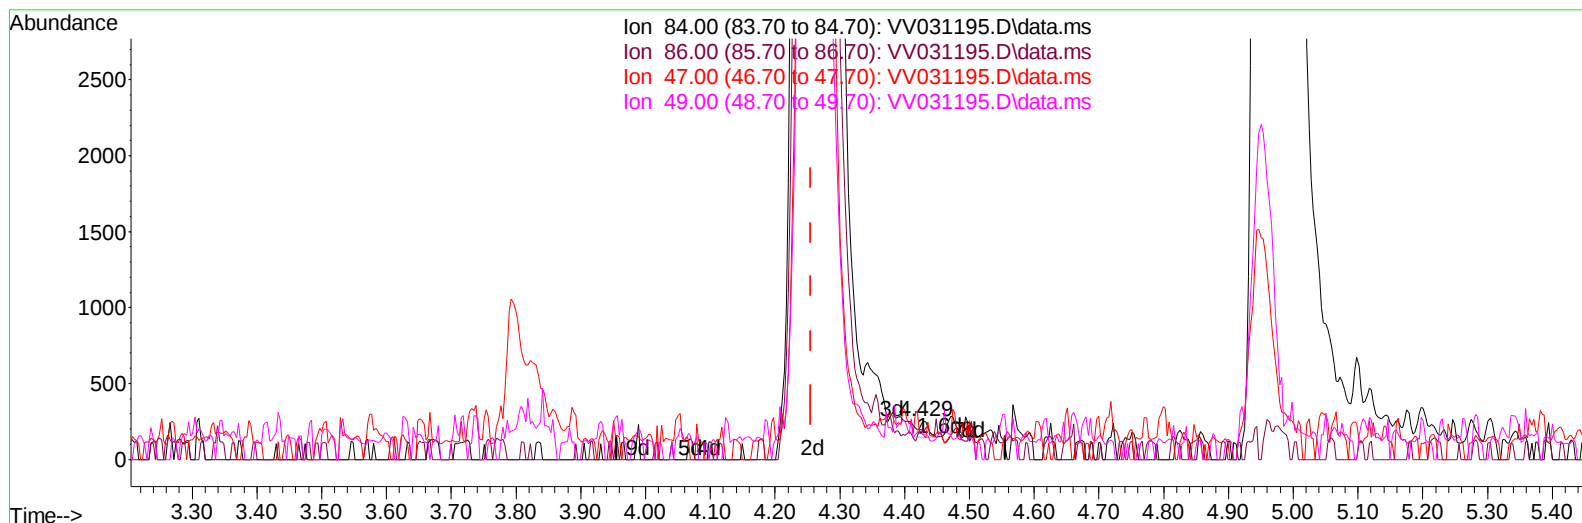

TIC: VV031195.D\data.ms

(24) Chloroform-d (S)

4.429min (+ 0.174) 0.04 ug/L

response 96

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	50.00
47.00	49.40	57.29
49.00	30.30	34.38




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031195.D
Acq On : 23 May 2023 17:14
Operator : SY/MD
Sample : 02865-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX58

Manual IntegrationsAPPROVED

Quant Time: May 24 01:36:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 24 01:27:41 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

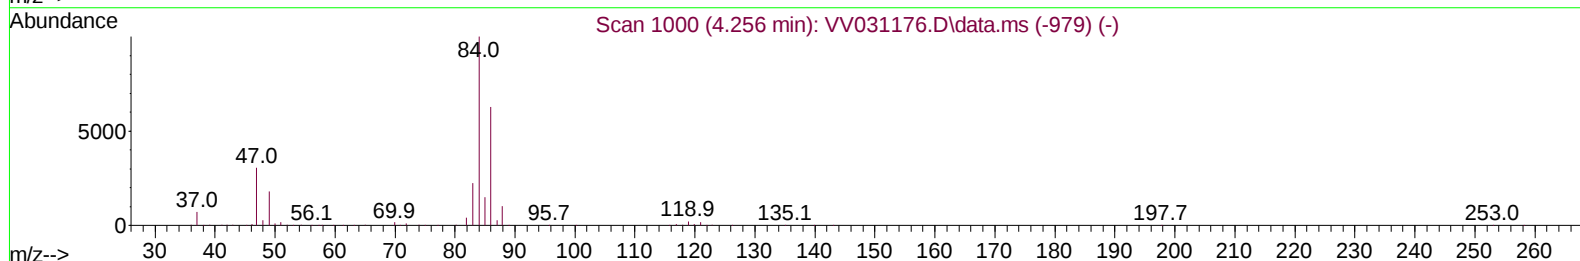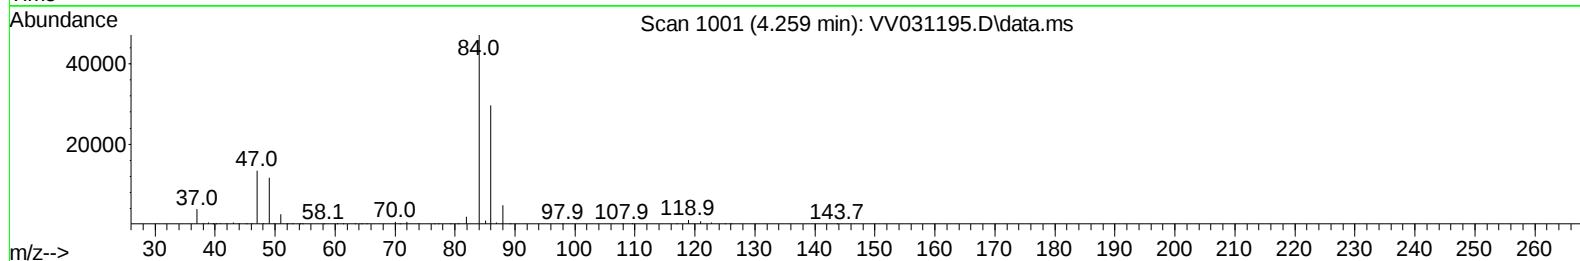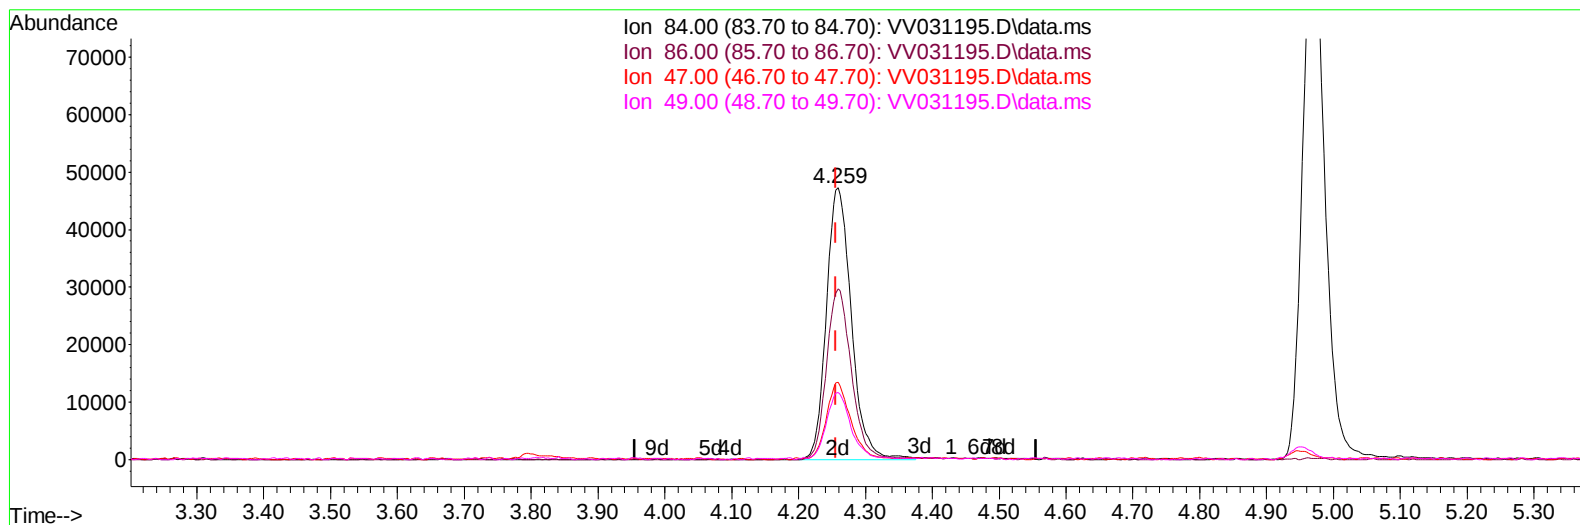

TIC: VV031195.D\data.ms

(24) Chloroform-d (S)

4.259min (+ 0.003) 49.63 ug/L m

response 122692

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.04#
47.00	49.40	0.04#
49.00	30.30	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031195.D
 Acq On : 23 May 2023 17:14
 Operator : SY/MD
 Sample : 02865-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX58

Manual IntegrationsAPPROVED

Quant Time: May 24 01:36:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 24 01:27:41 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	163508	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	169758	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	81704	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	67053	47.985	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	95.980%	
7) Chloroethane-d5	1.536	69	60010	55.746	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	111.500%	
11) 1,1-Dichloroethene-d2	2.063	65	33319	50.847	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	101.700%	
21) 2-Butanone-d5	3.799	46	83479	112.115	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	112.110%	
24) Chloroform-d	4.259	84	122692m	49.631	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.260%	
26) 1,2-Dichloroethane-d4	4.950	65	90923	54.430	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.860%	
32) Benzene-d6	4.970	84	219864	47.776	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.560%	
36) 1,2-Dichloropropane-d6	5.995	67	63121	45.841	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	91.680%	
41) Toluene-d8	7.249	98	205742	47.901	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.800%	
43) trans-1,3-Dichloroprop...	7.558	79	32900	47.624	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	95.240%	
47) 2-Hexanone-d5	8.031	63	58269	108.534	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	108.530%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	98300	47.597	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4	11.567	152	87874	59.851	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	119.700%	
Target Compounds						
					Qvalue	
13) Acetone	2.124	43	10046	10.378	ug/L	99
20) cis-1,2-Dichloroethene	3.835	96	4270	4.125	ug/L	88
34) Trichloroethene	5.841	95	47837	43.898	ug/L	96
48) 2-Hexanone	8.088	43	11938	8.321	ug/L #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031195.D
Acq On : 23 May 2023 17:14
Operator : SY/MD
Sample : 02865-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX58

Manual IntegrationsAPPROVED

Quant Time: May 24 01:36:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 24 01:27:41 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

