

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031177.D
 Acq On : 23 May 2023 10:10
 Operator : SY/MD
 Sample : VV0523WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK342

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rBV	116564	129355	14.34%	2.057%
2	1.536	147	154	165	rVB	106246	124381	13.79%	1.978%
3	2.063	310	318	332	rVB	215537	311422	34.52%	4.952%
4	2.368	409	413	417	rBV5	2482	1966	0.22%	0.031%
5	2.391	417	420	422	rBV4	1690	855	0.09%	0.014%
6	2.410	422	426	428	rBV5	1622	1022	0.11%	0.016%
7	2.455	432	440	442	rBV7	3055	3910	0.43%	0.062%
8	2.507	453	456	458	rVB4	1676	942	0.10%	0.015%
9	2.532	461	464	465	rBV3	1460	923	0.10%	0.015%
10	2.703	513	517	518	rBV4	1683	1058	0.12%	0.017%
11	2.789	541	544	546	rBV4	1505	917	0.10%	0.015%
12	2.838	556	559	560	rBV3	1830	813	0.09%	0.013%
13	2.915	581	583	586	rBV4	1228	810	0.09%	0.013%
14	2.989	601	606	609	rBV7	2091	1988	0.22%	0.032%
15	3.137	649	652	655	rVB4	1371	1027	0.11%	0.016%
16	3.227	677	680	684	rBV6	1734	1381	0.15%	0.022%
17	3.307	702	705	712	rVB8	1772	1421	0.16%	0.023%
18	3.352	717	719	720	rVV2	1807	769	0.09%	0.012%
19	3.384	727	729	731	rVV2	1829	1150	0.13%	0.018%
20	3.423	735	741	743	rBV6	2005	1528	0.17%	0.024%
21	3.474	755	757	758	rVV2	1626	750	0.08%	0.012%
22	3.568	782	786	789	rVV5	1087	901	0.10%	0.014%
23	3.645	807	810	813	rVB5	1891	1251	0.14%	0.020%
24	3.667	813	817	818	rBV4	1434	936	0.10%	0.015%
25	3.699	825	827	831	rVB5	1366	940	0.10%	0.015%
26	3.741	836	840	843	rBV6	1386	973	0.11%	0.015%
27	3.793	847	856	881	rBV	64099	169885	18.83%	2.701%
28	4.133	959	962	964	rBV4	1705	1160	0.13%	0.018%
29	4.259	987	1001	1025	rBV	152895	385362	42.71%	6.127%
30	4.635	1115	1118	1120	rBV4	1449	837	0.09%	0.013%
31	4.857	1185	1187	1192	rVB6	2137	1118	0.12%	0.018%
32	4.963	1200	1220	1244	rBV2	333763	902270	100.00%	14.346%
33	5.323	1329	1332	1333	rBV3	1401	728	0.08%	0.012%
34	5.542	1388	1400	1423	rBV	251320	524396	58.12%	8.338%
35	5.789	1474	1477	1478	rBV3	2076	935	0.10%	0.015%
36	5.995	1530	1541	1564	rBV	200599	412150	45.68%	6.553%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031177.D
 Acq On : 23 May 2023 10:10
 Operator : SY/MD
 Sample : VV0523WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK342

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.243	1616	1618	1621	rBV4	1652	815	0.09%	0.013%
38	6.365	1654	1656	1659	rVB4	1684	812	0.09%	0.013%
39	6.407	1664	1669	1670	rBV4	989	816	0.09%	0.013%
40	6.426	1673	1675	1678	rBV3	1812	902	0.10%	0.014%

41	6.497	1693	1697	1700	rBV6	1947	1645	0.18%	0.026%
42	6.722	1765	1767	1771	rBV5	1370	859	0.10%	0.014%
43	6.918	1815	1828	1848	rBV	93472	182123	20.18%	2.896%
44	7.104	1882	1886	1888	rBV5	1137	1009	0.11%	0.016%
45	7.249	1921	1931	1953	rBV	321263	578551	64.12%	9.199%

46	7.561	2018	2028	2045	rBV	69885	129384	14.34%	2.057%
47	7.751	2084	2087	2089	rBV3	1772	1157	0.13%	0.018%
48	7.780	2095	2096	2099	rBV3	1405	724	0.08%	0.012%
49	7.854	2117	2119	2123	rVB5	1965	1067	0.12%	0.017%
50	7.895	2128	2132	2134	rBV5	1719	1317	0.15%	0.021%

51	7.985	2156	2160	2164	rVB7	1453	1165	0.13%	0.019%
52	8.034	2164	2175	2203	rBV	191789	398832	44.20%	6.341%
53	8.294	2253	2256	2258	rBV4	1978	1685	0.19%	0.027%
54	8.583	2342	2346	2347	rBV3	1320	814	0.09%	0.013%
55	8.619	2354	2357	2361	rBV5	1422	993	0.11%	0.016%

56	8.641	2362	2364	2368	rBV5	1348	1046	0.12%	0.017%
57	8.735	2391	2393	2398	rBV4	1975	1580	0.18%	0.025%
58	8.792	2400	2411	2434	rVV	358518	610627	67.68%	9.709%
59	9.085	2498	2502	2504	rBV5	2018	1876	0.21%	0.030%
60	9.201	2534	2538	2541	rVB5	1534	1143	0.13%	0.018%

61	9.284	2560	2564	2566	rBV5	2055	1649	0.18%	0.026%
62	9.513	2630	2635	2637	rBV4	2376	2105	0.23%	0.033%
63	9.593	2657	2660	2661	rBV4	1386	795	0.09%	0.013%
64	9.645	2672	2676	2678	rBV5	2213	1731	0.19%	0.028%
65	10.159	2826	2836	2859	rVB	253540	409196	45.35%	6.506%

66	10.664	2991	2993	2995	rBV3	1601	974	0.11%	0.015%
67	10.847	3047	3050	3052	rBV3	2344	1952	0.22%	0.031%
68	11.191	3147	3157	3178	rBV	264870	421978	46.77%	6.709%
69	11.567	3264	3274	3295	rVB	306073	474445	52.58%	7.544%
70	12.107	3439	3442	3445	rBV5	2032	1066	0.12%	0.017%

71	12.181	3462	3465	3467	rBV4	1332	890	0.10%	0.014%
72	12.233	3478	3481	3483	rBV4	1122	745	0.08%	0.012%
73	12.252	3485	3487	3489	rBV3	1743	708	0.08%	0.011%
74	12.374	3521	3525	3528	rBV5	1822	1766	0.20%	0.028%
75	12.442	3543	3546	3549	rBV4	1392	1090	0.12%	0.017%

76	12.712	3625	3630	3633	rBV5	1227	1037	0.11%	0.016%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031177.D
 Acq On : 23 May 2023 10:10
 Operator : SY/MD
 Sample : VV0523WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK342

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.731	3633	3636	3641	rVB7	1693	1373	0.15%	0.022%
78	12.767	3641	3647	3651	rBV8	1849	2079	0.23%	0.033%
79	12.857	3671	3675	3679	rBV7	1694	1321	0.15%	0.021%
80	12.940	3698	3701	3703	rBV3	1440	869	0.10%	0.014%
81	13.008	3720	3722	3723	rBV2	1665	845	0.09%	0.013%
82	13.043	3731	3733	3736	rBV3	1497	1251	0.14%	0.020%
83	13.098	3746	3750	3751	rBV4	1511	1174	0.13%	0.019%
84	13.133	3756	3761	3763	rBV6	1668	1486	0.16%	0.024%
85	13.188	3773	3778	3779	rBV5	1370	1147	0.13%	0.018%
86	13.204	3779	3783	3784	rBV4	4338	2842	0.31%	0.045%
87	13.271	3801	3804	3807	rVB5	3166	1937	0.21%	0.031%
88	13.304	3810	3814	3816	rVB5	2678	1532	0.17%	0.024%
89	13.336	3820	3824	3827	rBV5	2158	1670	0.19%	0.027%
90	13.448	3846	3859	3871	rBV2	10370	20962	2.32%	0.333%
91	13.628	3912	3915	3919	rBV6	1685	1244	0.14%	0.020%
92	13.767	3955	3958	3959	rBV3	1527	901	0.10%	0.014%
93	14.066	4047	4051	4052	rBV3	1903	1284	0.14%	0.020%
94	14.329	4129	4133	4135	rBV5	2078	1962	0.22%	0.031%
95	14.342	4135	4137	4140	rVB4	2438	1247	0.14%	0.020%
96	14.551	4199	4202	4205	rVB5	2182	1081	0.12%	0.017%
97	14.612	4218	4221	4222	rBV3	1585	914	0.10%	0.015%
98	14.693	4242	4246	4249	rVB6	2680	2308	0.26%	0.037%
99	14.709	4249	4251	4254	rBV4	2008	1528	0.17%	0.024%
100	14.902	4309	4311	4313	rBV2	1935	1189	0.13%	0.019%




Sum of corrected areas: 6289445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031177.D
Acq On : 23 May 2023 10:10
Operator : SY/MD
Sample : VV0523WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

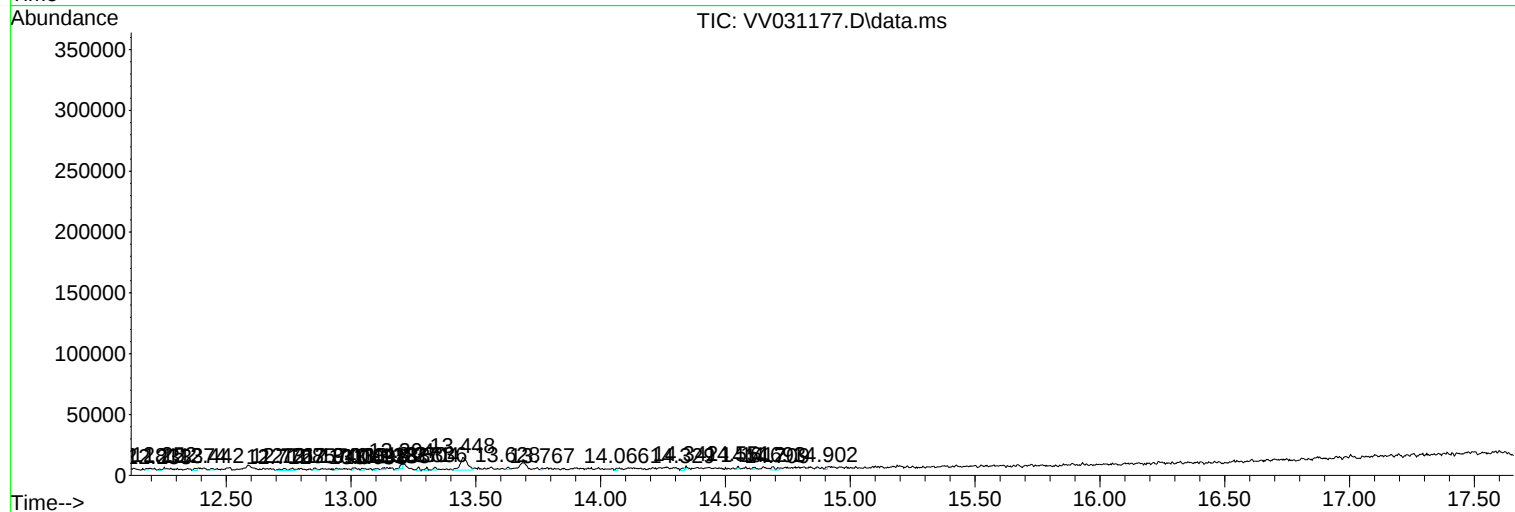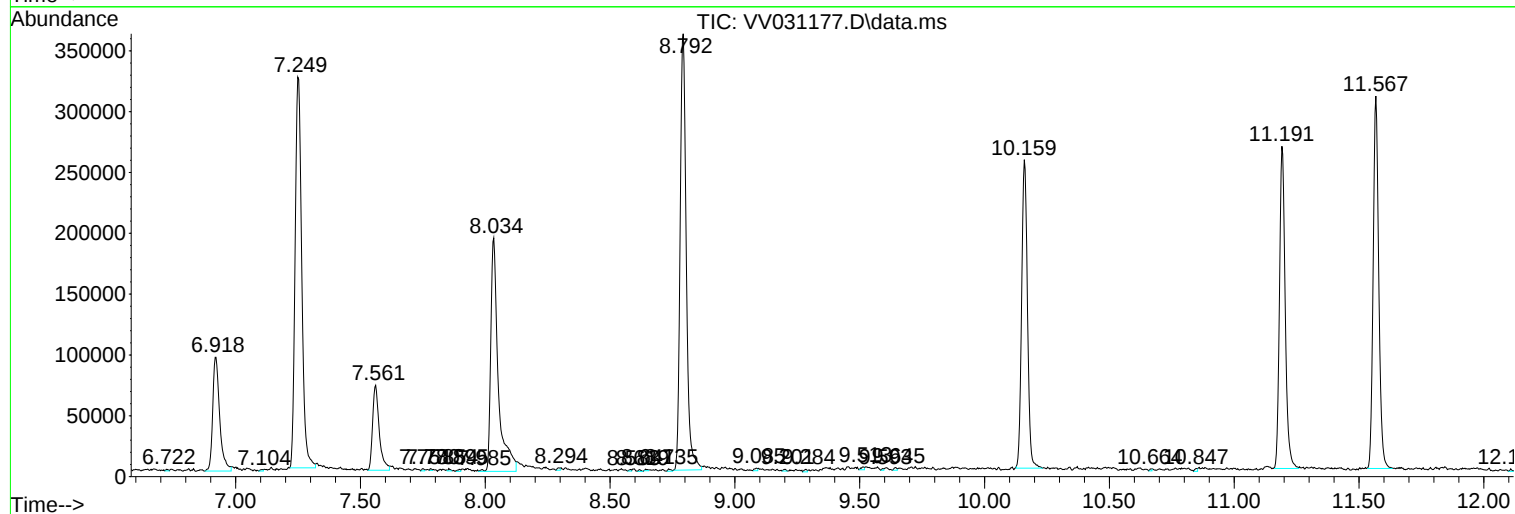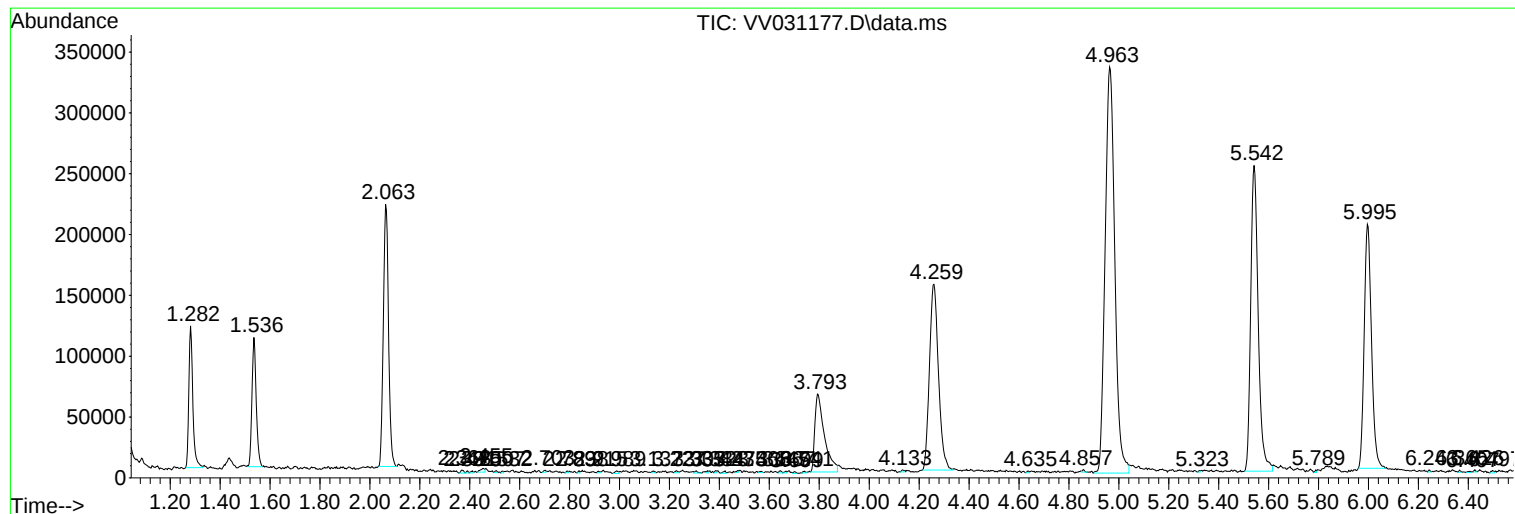

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031177.D
Acq On : 23 May 2023 10:10
Operator : SY/MD
Sample : VV0523WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031177.D
Acq On : 23 May 2023 10:10
Operator : SY/MD
Sample : VV0523WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc