

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031179.D
 Acq On : 23 May 2023 10:58
 Operator : SY/MD
 Sample : VV0523WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	148672	161789	15.63%	2.192%
2	1.535	147	154	172	rVB	120604	153866	14.86%	2.084%
3	2.063	309	318	334	rBV	286472	414873	40.08%	5.620%
4	2.236	370	372	374	rBV3	2147	1290	0.12%	0.017%
5	2.310	393	395	397	rBV3	1659	892	0.09%	0.012%
6	2.342	400	405	408	rBV7	1142	1281	0.12%	0.017%
7	2.580	476	479	482	rVB5	2134	1174	0.11%	0.016%
8	2.606	482	487	488	rBV5	1697	1278	0.12%	0.017%
9	2.680	507	510	515	rBV5	1950	1809	0.17%	0.025%
10	2.741	527	529	532	rVB3	1939	984	0.10%	0.013%
11	2.867	565	568	569	rBV3	1938	882	0.09%	0.012%
12	2.918	580	584	588	rBV7	1792	1463	0.14%	0.020%
13	2.953	592	595	598	rVB5	1518	988	0.10%	0.013%
14	3.008	609	612	616	rBV5	1767	1184	0.11%	0.016%
15	3.027	616	618	621	rVB4	2064	845	0.08%	0.011%
16	3.121	645	647	650	rBV4	1115	900	0.09%	0.012%
17	3.201	669	672	674	rBV4	1367	794	0.08%	0.011%
18	3.275	693	695	699	rVB3	1424	1156	0.11%	0.016%
19	3.323	707	710	713	rVV5	1638	1188	0.11%	0.016%
20	3.420	738	740	743	rBV4	1882	1036	0.10%	0.014%
21	3.567	783	786	789	rBV4	2170	1306	0.13%	0.018%
22	3.616	800	801	804	rVV3	1691	865	0.08%	0.012%
23	3.635	805	807	811	rVB5	1420	1031	0.10%	0.014%
24	3.661	811	815	816	rBV4	1332	849	0.08%	0.012%
25	3.731	835	837	844	rVB9	1775	1779	0.17%	0.024%
26	3.793	848	856	883	rBV	63050	168434	16.27%	2.282%
27	4.259	985	1001	1028	rBV	169225	434751	42.00%	5.890%
28	4.384	1038	1040	1042	rBV2	1585	930	0.09%	0.013%
29	4.410	1045	1048	1054	rVB8	2775	2353	0.23%	0.032%
30	4.542	1087	1089	1091	rVB3	2060	874	0.08%	0.012%
31	4.561	1091	1095	1096	rBV4	1629	819	0.08%	0.011%
32	4.583	1099	1102	1104	rBV4	1265	887	0.09%	0.012%
33	4.664	1125	1127	1130	rVB5	2060	1216	0.12%	0.016%
34	4.683	1130	1133	1138	rBV7	1639	1599	0.15%	0.022%
35	4.789	1162	1166	1169	rBV6	1230	978	0.09%	0.013%
36	4.886	1192	1196	1197	rBV4	1761	1098	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031179.D
 Acq On : 23 May 2023 10:58
 Operator : SY/MD
 Sample : VV0523WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.966	1204	1221	1244	rBV3	392372	1035181	100.00%	14.024%
38	5.391	1346	1353	1354	rBV7	1377	1484	0.14%	0.020%
39	5.464	1374	1376	1378	rVB3	1652	808	0.08%	0.011%
40	5.481	1379	1381	1384	rBV4	1391	976	0.09%	0.013%
41	5.542	1388	1400	1422	rBV	266296	551356	53.26%	7.469%
42	5.995	1530	1541	1560	rBV	203979	416017	40.19%	5.636%
43	6.918	1818	1828	1846	rBV	101308	191170	18.47%	2.590%
44	7.249	1921	1931	1952	rVV	394375	693530	67.00%	9.395%
45	7.558	2019	2027	2049	rBV	81330	146717	14.17%	1.988%
46	8.030	2166	2174	2191	rBV	190319	362596	35.03%	4.912%
47	8.792	2400	2411	2435	rBV	399351	685685	66.24%	9.289%
48	8.947	2456	2459	2461	rBV4	1995	919	0.09%	0.012%
49	8.998	2473	2475	2478	rBV4	1720	1211	0.12%	0.016%
50	9.062	2493	2495	2498	rBV4	1889	1033	0.10%	0.014%
51	9.278	2558	2562	2563	rVB4	1620	1002	0.10%	0.014%
52	9.461	2617	2619	2620	rBV2	1835	867	0.08%	0.012%
53	9.577	2652	2655	2658	rBV4	1458	870	0.08%	0.012%
54	9.943	2767	2769	2774	rBV6	1519	1151	0.11%	0.016%
55	10.027	2789	2795	2799	rBV8	2640	2998	0.29%	0.041%
56	10.046	2799	2801	2804	rVB4	1713	1059	0.10%	0.014%
57	10.104	2816	2819	2821	rBV4	1290	911	0.09%	0.012%
58	10.159	2825	2836	2854	rVV	305258	487634	47.11%	6.606%
59	10.329	2887	2889	2893	rBV5	1299	1026	0.10%	0.014%
60	10.416	2913	2916	2919	rBV5	2140	1235	0.12%	0.017%
61	10.442	2922	2924	2929	rVV6	1268	961	0.09%	0.013%
62	10.676	2995	2997	3002	rBV6	1929	1180	0.11%	0.016%
63	10.702	3002	3005	3007	rBV3	1334	959	0.09%	0.013%
64	10.728	3011	3013	3017	rBV4	1348	1112	0.11%	0.015%
65	10.818	3037	3041	3045	rBV6	2114	1566	0.15%	0.021%
66	10.869	3050	3057	3060	rBV7	2755	3042	0.29%	0.041%
67	10.982	3089	3092	3095	rVB5	1674	922	0.09%	0.012%
68	11.059	3111	3116	3117	rBV5	1283	925	0.09%	0.013%
69	11.191	3146	3157	3177	rBV	394852	642357	62.05%	8.702%
70	11.365	3206	3211	3213	rBV6	2549	2142	0.21%	0.029%
71	11.422	3226	3229	3230	rBV2	1928	1212	0.12%	0.016%
72	11.567	3263	3274	3289	rBV	457461	725031	70.04%	9.822%
73	11.754	3327	3332	3336	rBV7	1879	1614	0.16%	0.022%
74	11.776	3336	3339	3342	rVV4	1106	900	0.09%	0.012%
75	11.811	3345	3350	3353	rBV7	2006	2086	0.20%	0.028%
76	12.004	3404	3410	3412	rVV6	1785	1816	0.18%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031179.D
 Acq On : 23 May 2023 10:58
 Operator : SY/MD
 Sample : VV0523WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.165	3458	3460	3464	rBV5	1611	1381	0.13%	0.019%
78	12.204	3469	3472	3477	rVB6	2143	1838	0.18%	0.025%
79	12.410	3535	3536	3540	rVB4	2505	1269	0.12%	0.017%
80	12.432	3540	3543	3544	rBV2	1692	852	0.08%	0.012%
81	12.445	3544	3547	3551	rBV6	1678	1172	0.11%	0.016%
82	12.503	3562	3565	3568	rVB5	1577	899	0.09%	0.012%
83	12.657	3609	3613	3616	rVB5	1654	1158	0.11%	0.016%
84	12.866	3676	3678	3681	rBV3	1460	914	0.09%	0.012%
85	13.217	3784	3787	3792	rBV5	2145	1593	0.15%	0.022%
86	13.287	3806	3809	3812	rBV4	2056	1509	0.15%	0.020%
87	13.400	3840	3844	3846	rBV5	1651	853	0.08%	0.012%
88	13.448	3854	3859	3867	rBV9	3589	5671	0.55%	0.077%
89	13.528	3880	3884	3885	rBV4	1754	1156	0.11%	0.016%
90	13.593	3900	3904	3906	rBV4	1572	1050	0.10%	0.014%
91	13.651	3919	3922	3925	rBV5	1569	1310	0.13%	0.018%
92	13.741	3947	3950	3955	rVB6	2908	2082	0.20%	0.028%
93	14.053	4043	4047	4048	rBV4	1598	943	0.09%	0.013%
94	14.110	4062	4065	4070	rBV6	1615	1746	0.17%	0.024%
95	14.358	4139	4142	4148	rBV8	2606	3134	0.30%	0.042%
96	14.615	4220	4222	4225	rVB4	1986	1038	0.10%	0.014%
97	14.641	4225	4230	4233	rBV6	2105	2121	0.20%	0.029%
98	14.680	4239	4242	4243	rBV3	2193	1213	0.12%	0.016%
99	14.718	4252	4254	4255	rBV2	1812	824	0.08%	0.011%
100	15.175	4393	4396	4399	rBV5	2125	1274	0.12%	0.017%


Sum of corrected areas: 7381702

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031179.D
Acq On : 23 May 2023 10:58
Operator : SY/MD
Sample : VV0523WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK343

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

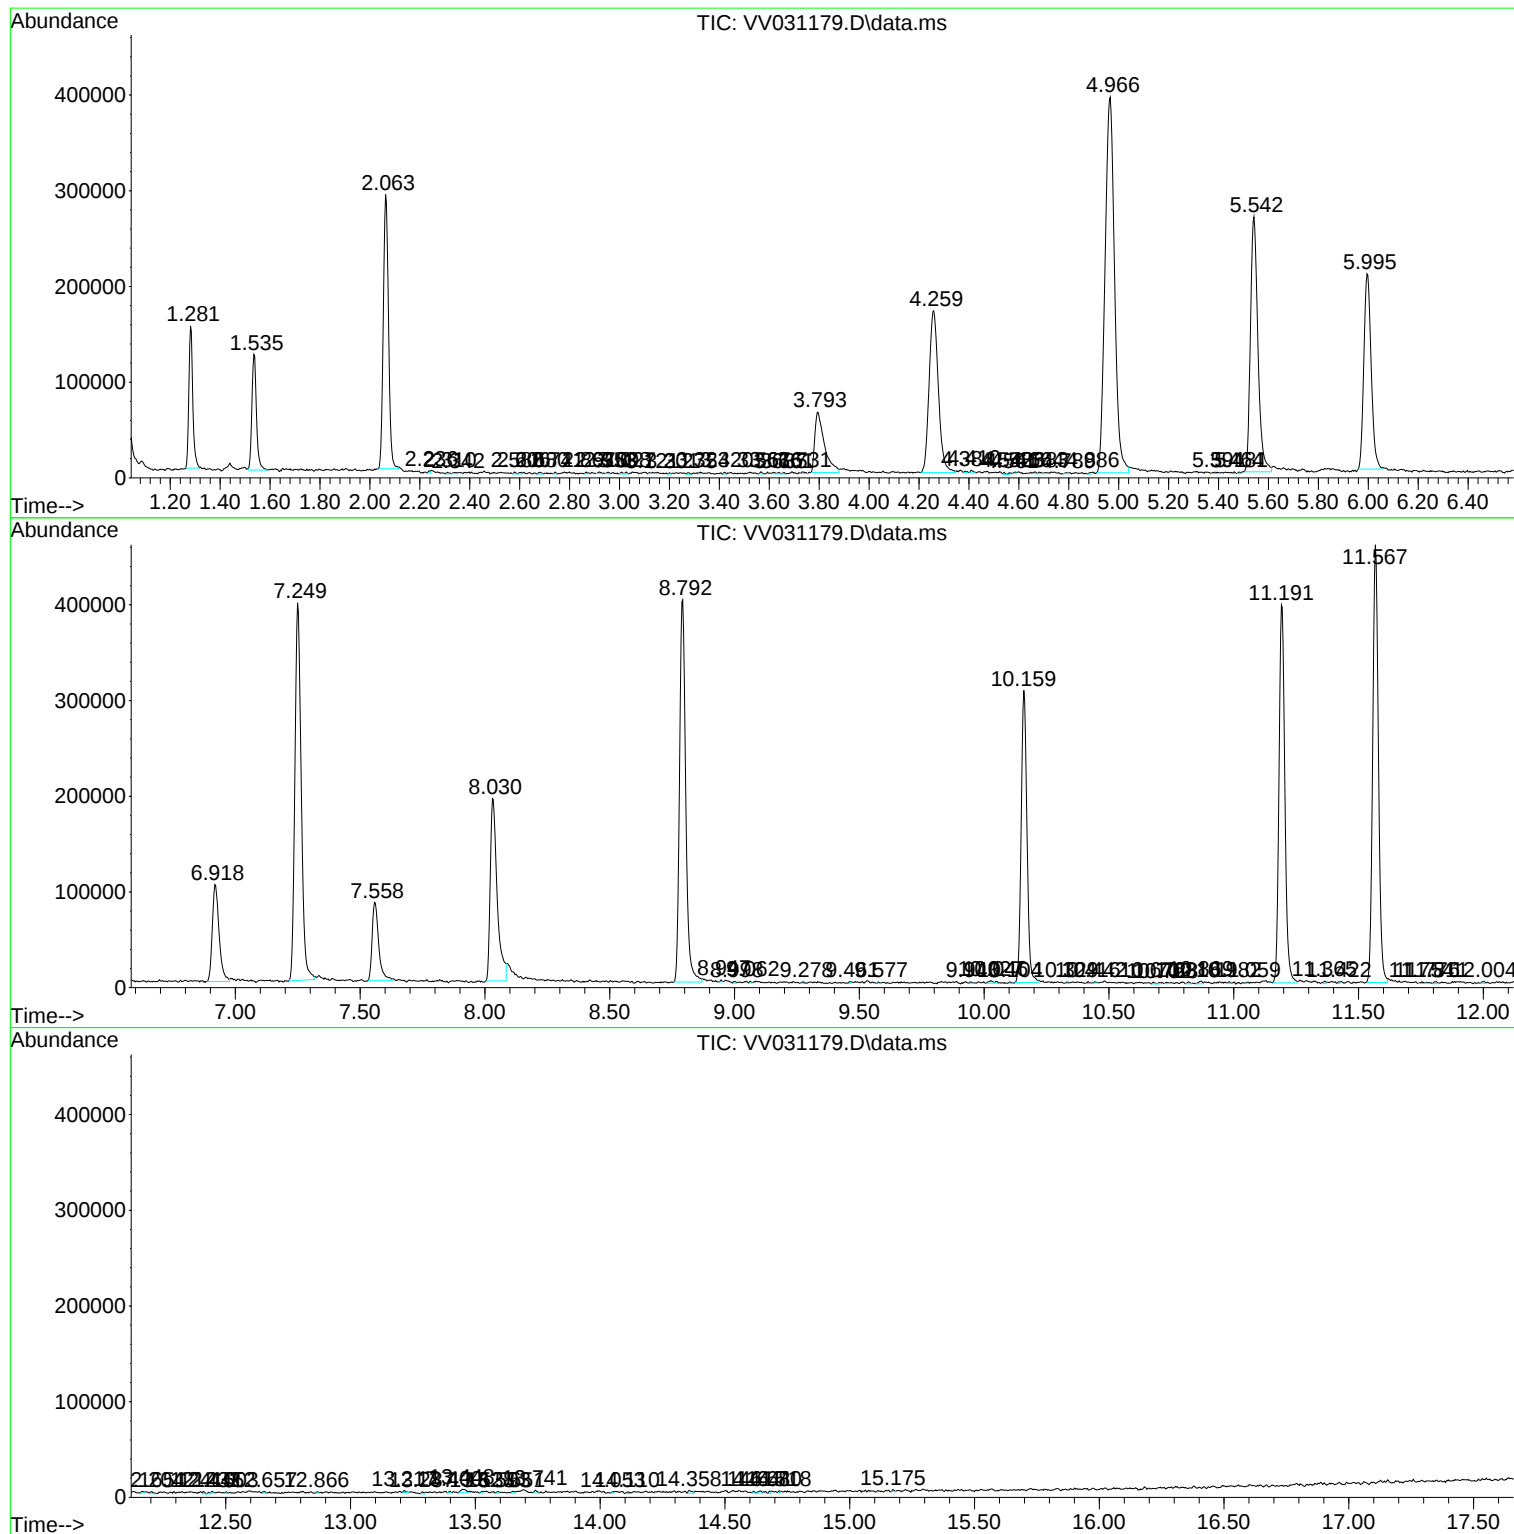

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031179.D
Acq On : 23 May 2023 10:58
Operator : SY/MD
Sample : VV0523WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK343

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031179.D
Acq On : 23 May 2023 10:58
Operator : SY/MD
Sample : VV0523WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK343

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------