

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031180.D
 Acq On : 23 May 2023 11:22
 Operator : SY/MD
 Sample : 02861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	94	rVB	151674	169179	16.14%	2.269%
2	1.535	147	154	166	rBV	126386	147407	14.06%	1.977%
3	2.008	298	301	304	rBV5	2853	2390	0.23%	0.032%
4	2.063	309	318	334	rVV	278119	409655	39.08%	5.495%
5	2.233	368	371	373	rBV4	1830	831	0.08%	0.011%
6	2.301	388	392	397	rVB7	2536	2311	0.22%	0.031%
7	2.333	397	402	405	rVB5	1532	1575	0.15%	0.021%
8	2.349	405	407	410	rBV4	1147	897	0.09%	0.012%
9	2.397	417	422	426	rBV6	2050	2014	0.19%	0.027%
10	2.674	505	508	511	rBV5	1358	878	0.08%	0.012%
11	2.773	535	539	541	rVV4	1593	1094	0.10%	0.015%
12	2.947	592	593	597	rBV4	1685	1125	0.11%	0.015%
13	2.995	605	608	612	rVB5	1621	893	0.09%	0.012%
14	3.021	612	616	620	rBV6	1578	1289	0.12%	0.017%
15	3.104	640	642	644	rVB3	2050	1105	0.11%	0.015%
16	3.378	723	727	730	rBV5	1626	1002	0.10%	0.013%
17	3.452	748	750	754	rVB4	2177	1101	0.11%	0.015%
18	3.471	754	756	758	rBV3	1671	1083	0.10%	0.015%
19	3.535	774	776	779	rVB4	1911	773	0.07%	0.010%
20	3.696	821	826	830	rBV7	2152	1685	0.16%	0.023%
21	3.796	844	857	884	rBV	62923	179623	17.14%	2.409%
22	4.101	950	952	955	rBV4	1607	1106	0.11%	0.015%
23	4.256	984	1000	1019	rBV	171726	442583	42.22%	5.937%
24	4.680	1123	1132	1135	rBV	2043	2589	0.25%	0.035%
25	4.738	1148	1150	1155	rVB7	1523	1284	0.12%	0.017%
26	4.764	1155	1158	1159	rBV3	1386	865	0.08%	0.012%
27	4.802	1168	1170	1173	rVB3	2227	1360	0.13%	0.018%
28	4.902	1197	1201	1202	rBV3	2113	1149	0.11%	0.015%
29	4.963	1204	1220	1244	rVV2	392215	1048254	100.00%	14.061%
30	5.333	1332	1335	1336	rBV3	1766	889	0.08%	0.012%
31	5.420	1360	1362	1364	rBV2	1562	937	0.09%	0.013%
32	5.542	1385	1400	1423	rBV	256354	538411	51.36%	7.222%
33	5.995	1529	1541	1562	rBV	217114	432236	41.23%	5.798%
34	6.362	1653	1655	1658	rBV4	2317	1095	0.10%	0.015%
35	6.918	1817	1828	1848	rBV	95587	184824	17.63%	2.479%
36	7.249	1921	1931	1951	rBV	362438	640540	61.11%	8.592%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031180.D
 Acq On : 23 May 2023 11:22
 Operator : SY/MD
 Sample : 02861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.558	2018	2027	2048	rBV	74713	137202	13.09%	1.840%
38	8.034	2165	2175	2206	rBV	197215	417063	39.79%	5.594%
39	8.455	2303	2306	2307	rBV2	1958	1163	0.11%	0.016%
40	8.503	2319	2321	2324	rVB4	1848	1128	0.11%	0.015%
41	8.554	2335	2337	2342	rBV6	1635	1424	0.14%	0.019%
42	8.657	2365	2369	2375	rBV10	1711	2232	0.21%	0.030%
43	8.792	2397	2411	2435	rBV	429417	728276	69.48%	9.769%
44	9.181	2529	2532	2537	rBV7	1891	1895	0.18%	0.025%
45	9.262	2555	2557	2563	rVB6	1391	840	0.08%	0.011%
46	9.287	2563	2565	2568	rBV4	1263	950	0.09%	0.013%
47	9.500	2628	2631	2634	rVB4	2062	1037	0.10%	0.014%
48	9.564	2648	2651	2652	rBV3	2065	874	0.08%	0.012%
49	9.609	2661	2665	2669	rBV6	1750	1536	0.15%	0.021%
50	9.664	2680	2682	2685	rBV3	1369	1059	0.10%	0.014%
51	9.815	2726	2729	2730	rBV3	1301	796	0.08%	0.011%
52	10.017	2789	2792	2799	rVB8	2357	2289	0.22%	0.031%
53	10.159	2825	2836	2861	rVB	300888	488330	46.59%	6.550%
54	10.326	2884	2888	2890	rBV5	1601	933	0.09%	0.013%
55	10.394	2907	2909	2912	rVB4	1777	930	0.09%	0.012%
56	10.628	2980	2982	2987	rVB6	1888	1054	0.10%	0.014%
57	10.651	2987	2989	2991	rBV2	1650	851	0.08%	0.011%
58	10.673	2995	2996	3001	rBV5	1572	1047	0.10%	0.014%
59	10.699	3001	3004	3006	rBV4	1322	759	0.07%	0.010%
60	10.844	3046	3049	3052	rBV4	1284	913	0.09%	0.012%
61	10.892	3062	3064	3068	rVB5	1525	957	0.09%	0.013%
62	11.017	3100	3103	3105	rBV4	1848	1189	0.11%	0.016%
63	11.049	3110	3113	3116	rVB4	1263	884	0.08%	0.012%
64	11.091	3124	3126	3129	rBV3	1221	945	0.09%	0.013%
65	11.191	3146	3157	3177	rBV	413706	663392	63.29%	8.898%
66	11.394	3216	3220	3221	rBV4	1315	934	0.09%	0.013%
67	11.429	3229	3231	3236	rBV6	1400	1067	0.10%	0.014%
68	11.455	3236	3239	3242	rVB5	1112	766	0.07%	0.010%
69	11.567	3263	3274	3292	rVV	462228	725792	69.24%	9.735%
70	11.712	3317	3319	3321	rBV3	1594	888	0.08%	0.012%
71	11.911	3379	3381	3383	rBV4	1548	1002	0.10%	0.013%
72	11.959	3394	3396	3401	rVB6	2013	1428	0.14%	0.019%
73	11.988	3401	3405	3408	rBV5	1624	1401	0.13%	0.019%
74	12.066	3425	3429	3432	rBV6	1396	1179	0.11%	0.016%
75	12.168	3458	3461	3464	rBV5	1599	945	0.09%	0.013%
76	12.185	3464	3466	3469	rBV3	1066	959	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031180.D
 Acq On : 23 May 2023 11:22
 Operator : SY/MD
 Sample : 02861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.249	3484	3486	3493	rVB7	1427	1609	0.15%	0.022%
78	12.307	3499	3504	3506	rBV5	1559	1316	0.13%	0.018%
79	12.374	3522	3525	3527	rVV3	1742	1054	0.10%	0.014%
80	12.419	3536	3539	3542	rBV4	1512	1193	0.11%	0.016%
81	12.583	3588	3590	3593	rBV4	2136	1217	0.12%	0.016%
82	12.615	3598	3600	3604	rVB4	2116	1036	0.10%	0.014%
83	12.680	3618	3620	3622	rBV2	1371	763	0.07%	0.010%
84	12.734	3635	3637	3643	rVV7	1603	1407	0.13%	0.019%
85	12.805	3654	3659	3662	rBV7	1484	1812	0.17%	0.024%
86	12.844	3667	3671	3677	rVB8	1482	2293	0.22%	0.031%
87	12.898	3686	3688	3694	rVB7	2212	1197	0.11%	0.016%
88	12.930	3694	3698	3700	rBV5	1328	858	0.08%	0.012%
89	12.988	3714	3716	3719	rVV3	1465	876	0.08%	0.012%
90	13.201	3779	3782	3783	rBV3	2598	1585	0.15%	0.021%
91	13.284	3804	3808	3812	rBV6	1784	1827	0.17%	0.025%
92	13.307	3812	3815	3819	rBV6	1333	1094	0.10%	0.015%
93	13.361	3830	3832	3836	rVB5	2236	1163	0.11%	0.016%
94	13.541	3886	3888	3891	rVB4	2248	1009	0.10%	0.014%
95	13.557	3891	3893	3896	rBV3	1437	897	0.09%	0.012%
96	13.577	3896	3899	3903	rBV5	2092	1326	0.13%	0.018%
97	13.799	3966	3968	3971	rBV4	1209	943	0.09%	0.013%
98	13.918	4001	4005	4008	rBV6	2663	2673	0.25%	0.036%
99	14.316	4127	4129	4132	rBV4	1426	857	0.08%	0.011%
100	14.377	4146	4148	4150	rBV3	1619	777	0.07%	0.010%




Sum of corrected areas: 7455123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031180.D
Acq On : 23 May 2023 11:22
Operator : SY/MD
Sample : 02861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

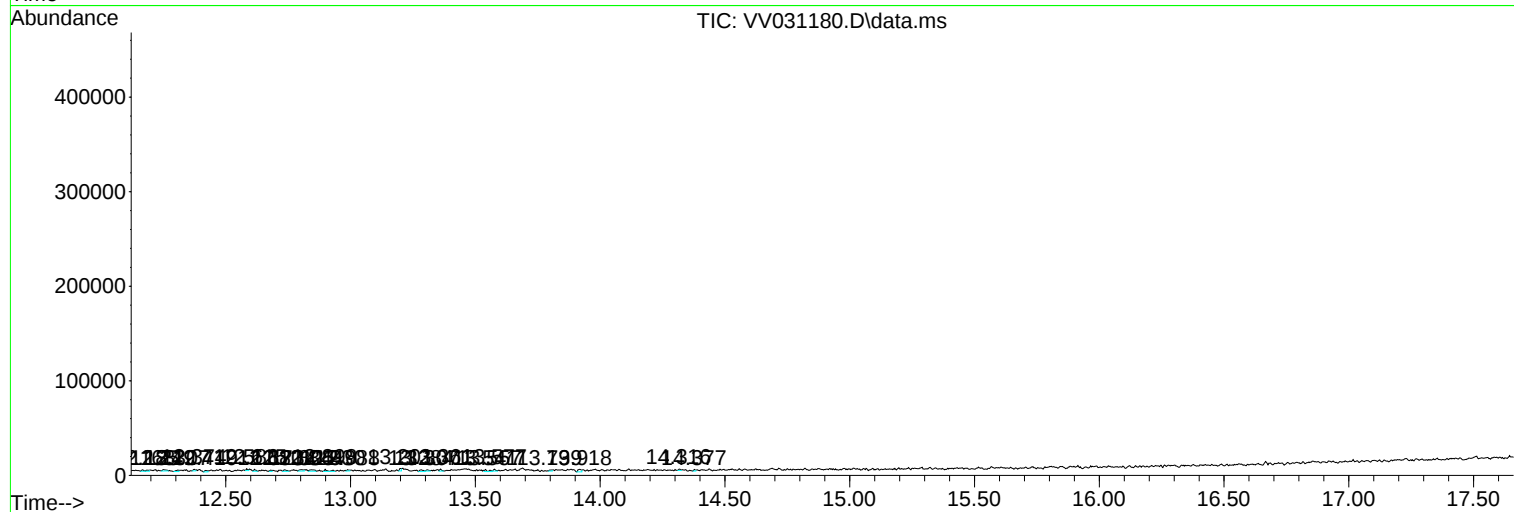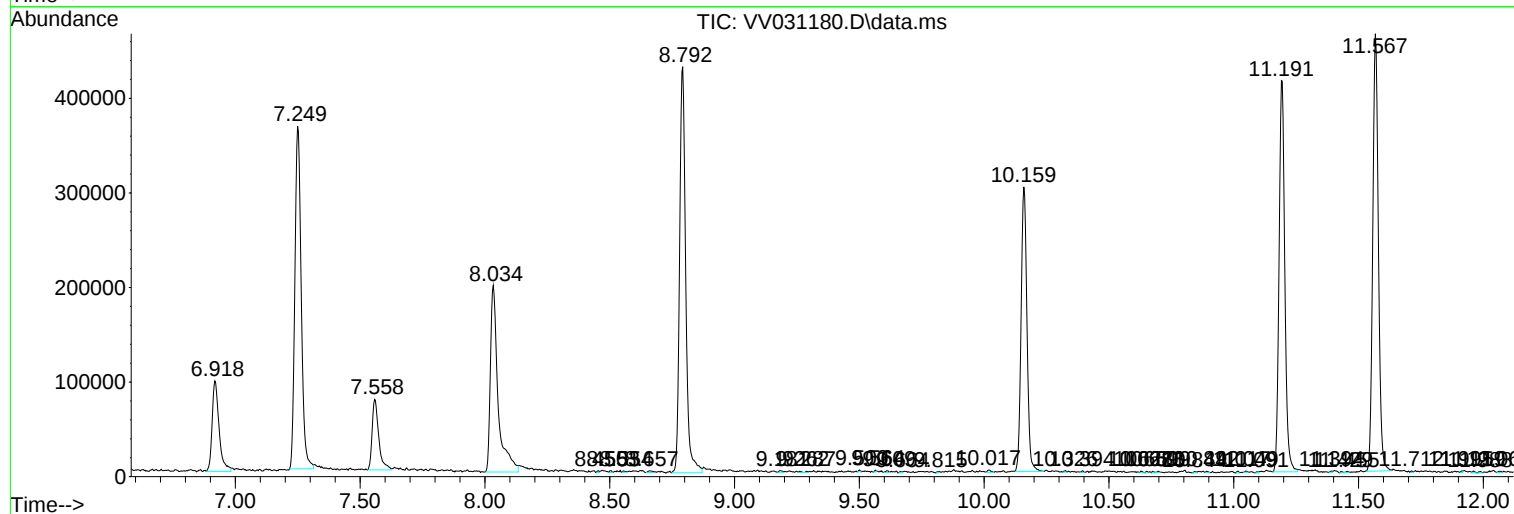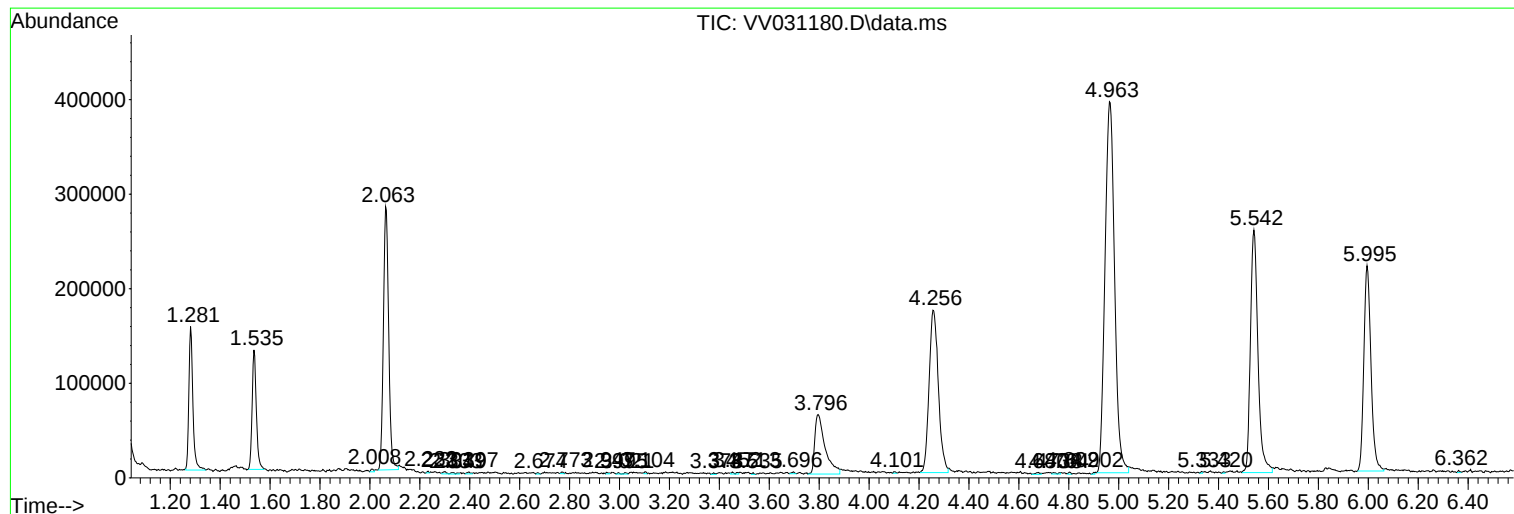

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031180.D
Acq On : 23 May 2023 11:22
Operator : SY/MD
Sample : 02861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031180.D
Acq On : 23 May 2023 11:22
Operator : SY/MD
Sample : 02861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc