

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031182.D
 Acq On : 23 May 2023 12:09
 Operator : SY/MD
 Sample : 02861-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	149418	163485	15.52%	2.217%
2	1.535	148	154	165	rVB	133391	158833	15.08%	2.154%
3	2.063	310	318	331	rVB	252580	366757	34.82%	4.973%
4	2.217	364	366	370	rBV5	1574	1180	0.11%	0.016%
5	2.400	421	423	427	rBV5	2001	1561	0.15%	0.021%
6	2.490	447	451	453	rBV5	2115	1298	0.12%	0.018%
7	2.516	457	459	461	rBV3	1499	873	0.08%	0.012%
8	2.571	474	476	481	rBV5	1306	1331	0.13%	0.018%
9	2.648	497	500	502	rBV3	1896	1161	0.11%	0.016%
10	2.860	564	566	569	rBV4	1265	728	0.07%	0.010%
11	2.873	569	570	574	rVV4	1389	840	0.08%	0.011%
12	2.931	581	588	590	rBV8	1887	1814	0.17%	0.025%
13	2.960	594	597	599	rBV4	799	543	0.05%	0.007%
14	2.976	600	602	604	rBV3	1128	494	0.05%	0.007%
15	3.056	625	627	630	rVB4	2735	1448	0.14%	0.020%
16	3.162	658	660	665	rVB7	1804	1437	0.14%	0.019%
17	3.195	665	670	673	rBV7	1908	1847	0.18%	0.025%
18	3.211	673	675	678	rBV4	1061	651	0.06%	0.009%
19	3.285	695	698	700	rVV4	1212	965	0.09%	0.013%
20	3.297	700	702	707	rVV6	1877	1527	0.14%	0.021%
21	3.368	721	724	725	rBV4	985	592	0.06%	0.008%
22	3.394	730	732	735	rVV5	1535	929	0.09%	0.013%
23	3.416	735	739	740	rVV3	1501	1208	0.11%	0.016%
24	3.445	747	748	753	rVB4	1273	695	0.07%	0.009%
25	3.529	771	774	776	rBV4	1960	1387	0.13%	0.019%
26	3.561	780	784	789	rVV6	1446	1764	0.17%	0.024%
27	3.587	789	792	793	rVV3	1739	1206	0.11%	0.016%
28	3.609	797	799	800	rVV2	1441	537	0.05%	0.007%
29	3.625	800	804	806	rVV4	1041	689	0.07%	0.009%
30	3.638	806	808	812	rVB5	1305	705	0.07%	0.010%
31	3.725	832	835	838	rBV4	2091	1677	0.16%	0.023%
32	3.799	849	858	878	rBV2	57723	158771	15.07%	2.153%
33	4.127	958	960	961	rBV2	1962	936	0.09%	0.013%
34	4.256	987	1000	1027	rVB2	172406	434609	41.26%	5.893%
35	4.474	1065	1068	1071	rBV5	1613	999	0.09%	0.014%
36	4.523	1081	1083	1084	rBV2	1222	509	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031182.D
 Acq On : 23 May 2023 12:09
 Operator : SY/MD
 Sample : 02861-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOFLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.828	1176	1178	1182	rVB5	1612	737	0.07%	0.010%
38	4.863	1187	1189	1191	rVB3	1407	641	0.06%	0.009%
39	4.883	1193	1195	1198	rBV4	1410	819	0.08%	0.011%
40	4.963	1203	1220	1247	rBV2	389581	1053359	100.00%	14.282%
41	5.442	1367	1369	1372	rVB4	1385	719	0.07%	0.010%
42	5.481	1378	1381	1385	rBV6	1262	992	0.09%	0.013%
43	5.542	1388	1400	1421	rBV	275813	574340	54.52%	7.787%
44	5.995	1529	1541	1569	rBV	233191	481033	45.67%	6.522%
45	6.461	1682	1686	1690	rBV6	1515	1499	0.14%	0.020%
46	6.481	1690	1692	1694	rBV3	1149	673	0.06%	0.009%
47	6.529	1706	1707	1713	rBV6	1371	1427	0.14%	0.019%
48	6.677	1751	1753	1757	rVB4	1469	903	0.09%	0.012%
49	6.702	1757	1761	1764	rBV5	2554	1800	0.17%	0.024%
50	6.809	1791	1794	1797	rBV3	1559	1224	0.12%	0.017%
51	6.844	1802	1805	1808	rBV5	1066	719	0.07%	0.010%
52	6.879	1814	1816	1818	rBV3	1056	495	0.05%	0.007%
53	6.918	1818	1828	1851	rVV	114276	222839	21.16%	3.021%
54	7.249	1920	1931	1953	rBV	447119	788705	74.88%	10.694%
55	7.558	2019	2027	2042	rBV2	82452	143808	13.65%	1.950%
56	8.034	2166	2175	2207	rBV	188122	395477	37.54%	5.362%
57	8.291	2252	2255	2256	rBV3	2303	1061	0.10%	0.014%
58	8.374	2279	2281	2285	rBV5	1580	1206	0.11%	0.016%
59	8.513	2322	2324	2326	rBV3	1667	620	0.06%	0.008%
60	8.571	2340	2342	2344	rBV3	1509	813	0.08%	0.011%
61	8.744	2393	2396	2398	rBV3	1703	1216	0.12%	0.016%
62	8.789	2400	2410	2434	rVV	429294	718944	68.25%	9.748%
63	9.018	2475	2481	2483	rBV5	1551	1445	0.14%	0.020%
64	9.317	2572	2574	2577	rBV4	1458	822	0.08%	0.011%
65	9.352	2581	2585	2587	rBV5	2253	1843	0.17%	0.025%
66	9.410	2600	2603	2608	rBV6	2754	2629	0.25%	0.036%
67	9.458	2616	2618	2622	rVB4	2007	1258	0.12%	0.017%
68	9.931	2763	2765	2769	rBV5	2806	2389	0.23%	0.032%
69	10.072	2806	2809	2813	rBV6	2655	2161	0.21%	0.029%
70	10.159	2826	2836	2854	rBV	274114	430462	40.87%	5.836%
71	10.654	2987	2990	2994	rBV6	2160	1968	0.19%	0.027%
72	10.915	3069	3071	3074	rBV4	1327	604	0.06%	0.008%
73	11.133	3136	3139	3142	rBV5	2185	1694	0.16%	0.023%
74	11.191	3147	3157	3174	rVV	386124	592605	56.26%	8.035%
75	11.374	3210	3214	3218	rBV7	2495	2659	0.25%	0.036%
76	11.477	3243	3246	3248	rBV4	1955	1322	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031182.D
 Acq On : 23 May 2023 12:09
 Operator : SY/MD
 Sample : 02861-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FLO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3293	rBV	372163	593958	56.39%	8.053%
78	11.722	3320	3322	3325	rBV4	1939	1244	0.12%	0.017%
79	11.979	3400	3402	3405	rBV3	1211	770	0.07%	0.010%
80	12.455	3548	3550	3552	rBV3	1484	671	0.06%	0.009%
81	12.709	3627	3629	3630	rBV2	1453	504	0.05%	0.007%
82	12.969	3707	3710	3711	rBV3	2048	1108	0.11%	0.015%
83	13.040	3730	3732	3733	rBV2	1856	656	0.06%	0.009%
84	13.387	3838	3840	3844	rBV4	1803	1167	0.11%	0.016%
85	13.432	3852	3854	3858	rVB5	1479	776	0.07%	0.011%
86	13.455	3858	3861	3866	rBV6	2872	2961	0.28%	0.040%
87	13.503	3874	3876	3878	rBV3	2315	1118	0.11%	0.015%
88	13.606	3906	3908	3911	rVB4	1473	707	0.07%	0.010%
89	13.731	3944	3947	3949	rBV4	2277	1358	0.13%	0.018%
90	13.760	3954	3956	3959	rVB4	1873	972	0.09%	0.013%
91	13.808	3969	3971	3976	rVB6	2210	1680	0.16%	0.023%
92	13.831	3976	3978	3979	rBV2	1459	635	0.06%	0.009%
93	13.898	3997	3999	4001	rBV3	1393	541	0.05%	0.007%
94	14.049	4043	4046	4048	rBV4	1414	912	0.09%	0.012%
95	14.165	4078	4082	4085	rVB5	2373	1849	0.18%	0.025%
96	14.249	4105	4108	4111	rBV5	2018	1849	0.18%	0.025%
97	14.326	4128	4132	4133	rBV3	1726	942	0.09%	0.013%
98	14.535	4195	4197	4199	rBV3	2071	834	0.08%	0.011%
99	14.586	4210	4213	4214	rBV3	1912	997	0.09%	0.014%
100	15.008	4340	4344	4346	rBV4	1965	1391	0.13%	0.019%




Sum of corrected areas: 7375516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031182.D
Acq On : 23 May 2023 12:09
Operator : SY/MD
Sample : 02861-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

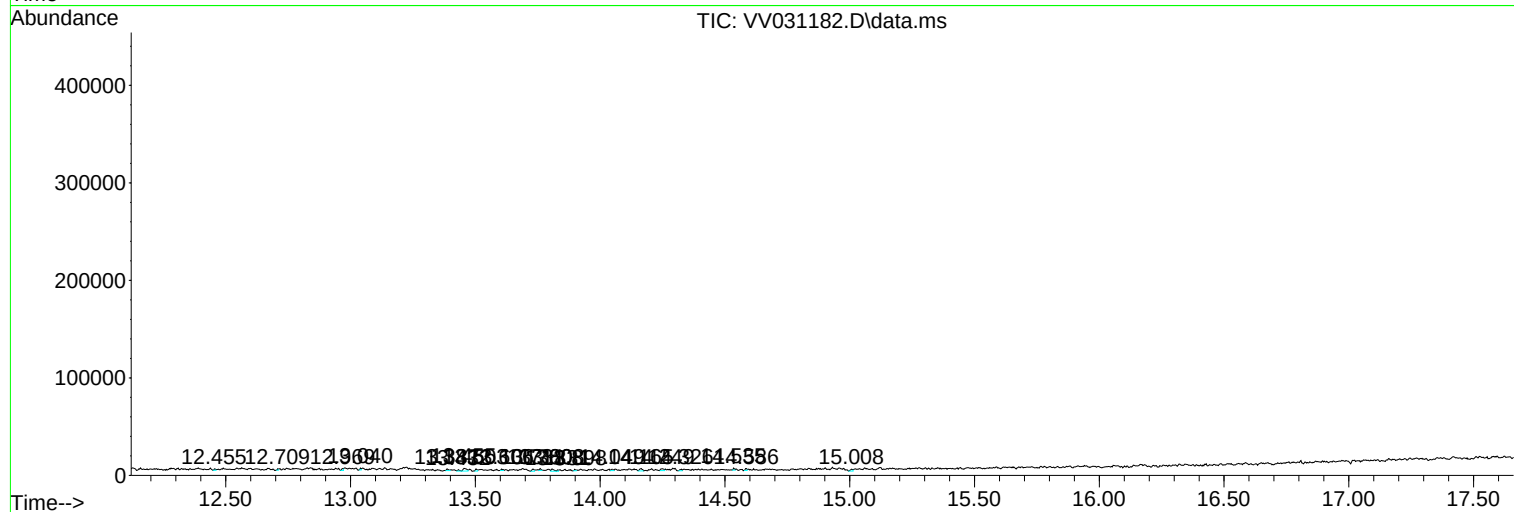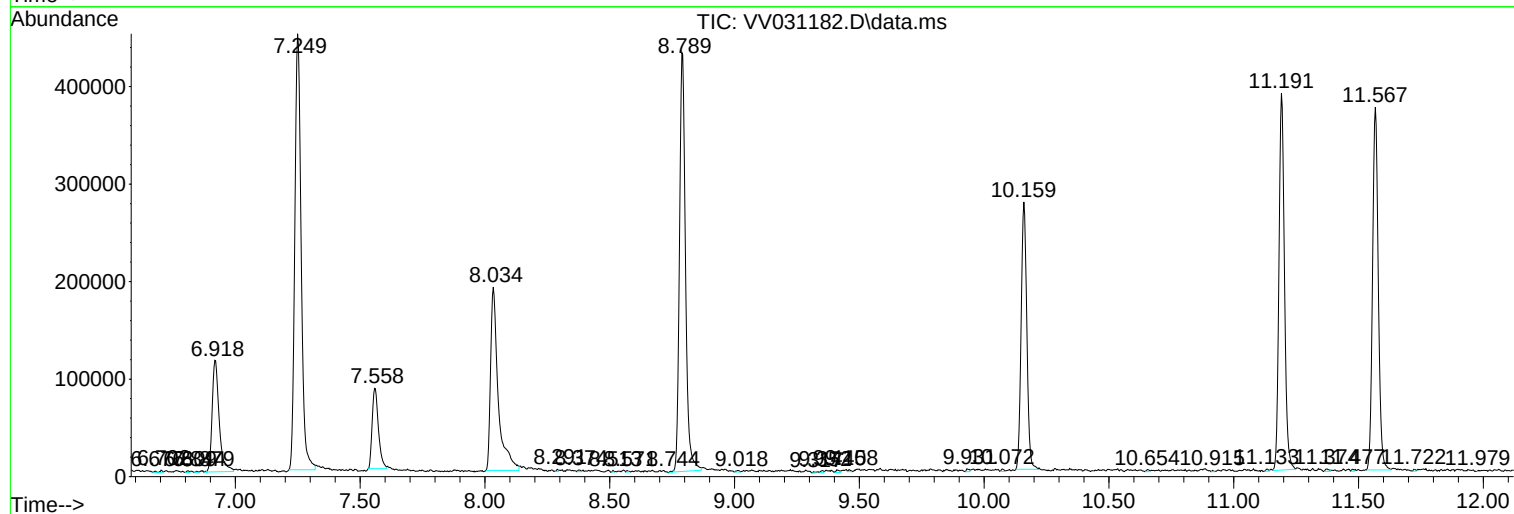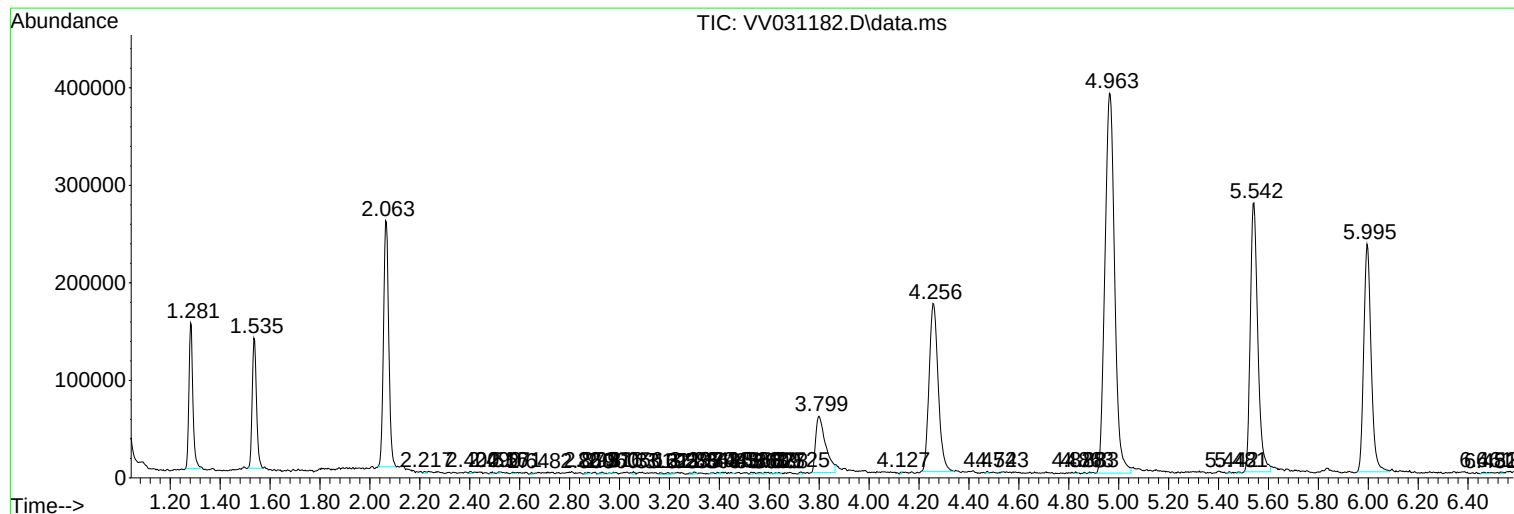

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031182.D
Acq On : 23 May 2023 12:09
Operator : SY/MD
Sample : 02861-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031182.D
Acq On : 23 May 2023 12:09
Operator : SY/MD
Sample : 02861-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FLO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------