

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031183.D
 Acq On : 23 May 2023 12:33
 Operator : SY/MD
 Sample : 02861-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rBV	141503	154775	15.64%	2.139%
2	1.535	148	154	165	rVB	117637	140922	14.24%	1.948%
3	1.728	212	214	217	rBV4	2304	1227	0.12%	0.017%
4	2.063	309	318	332	rBV	268035	398570	40.26%	5.509%
5	2.355	407	409	413	rVB4	1019	736	0.07%	0.010%
6	2.378	414	416	420	rBV4	1559	989	0.10%	0.014%
7	2.394	420	421	425	rBV4	1198	679	0.07%	0.009%
8	2.433	431	433	437	rVB5	1418	857	0.09%	0.012%
9	2.545	464	468	471	rBV5	1649	1637	0.17%	0.023%
10	2.709	517	519	523	rVB5	1922	1235	0.12%	0.017%
11	2.831	552	557	560	rBV6	2030	1949	0.20%	0.027%
12	2.863	565	567	570	rVV4	1289	773	0.08%	0.011%
13	2.941	587	591	596	rBV7	1322	1116	0.11%	0.015%
14	3.018	612	615	616	rBV3	1856	957	0.10%	0.013%
15	3.040	620	622	624	rVV3	1232	633	0.06%	0.009%
16	3.076	629	633	635	rBV4	1994	1163	0.12%	0.016%
17	3.195	666	670	674	rBV7	1058	1094	0.11%	0.015%
18	3.233	680	682	684	rBV3	1360	784	0.08%	0.011%
19	3.246	684	686	690	rVV4	1158	992	0.10%	0.014%
20	3.387	728	730	736	rVB5	2326	2247	0.23%	0.031%
21	3.420	736	740	741	rBV4	1381	944	0.10%	0.013%
22	3.439	742	746	749	rBV6	1876	1577	0.16%	0.022%
23	3.706	827	829	831	rVV3	1337	802	0.08%	0.011%
24	3.799	849	858	876	rBV	55247	152761	15.43%	2.112%
25	4.198	980	982	983	rBV2	1724	657	0.07%	0.009%
26	4.256	988	1000	1022	rVB2	161265	406869	41.10%	5.624%
27	4.680	1128	1132	1134	rBV4	1267	1101	0.11%	0.015%
28	4.809	1170	1172	1177	rVB6	1783	902	0.09%	0.012%
29	4.847	1182	1184	1186	rBV3	1612	916	0.09%	0.013%
30	4.879	1191	1194	1197	rVB4	1585	939	0.09%	0.013%
31	4.899	1197	1200	1201	rBV3	1732	898	0.09%	0.012%
32	4.963	1205	1220	1246	rBV2	372231	989870	100.00%	13.682%
33	5.439	1366	1368	1369	rBV2	1382	601	0.06%	0.008%
34	5.542	1388	1400	1420	rBV	278852	573812	57.97%	7.931%
35	5.883	1503	1506	1510	rVB6	2503	1574	0.16%	0.022%
36	5.918	1514	1517	1519	rBV3	1769	945	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031183.D
 Acq On : 23 May 2023 12:33
 Operator : SY/MD
 Sample : 02861-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.995	1530	1541	1565	rVB	221191	445972	45.05%	6.164%
38	6.143	1584	1587	1589	rBV4	2699	1761	0.18%	0.024%
39	6.346	1647	1650	1653	rBV4	1600	1263	0.13%	0.017%
40	6.445	1678	1681	1685	rBV6	1821	1525	0.15%	0.021%
41	6.860	1809	1810	1813	rVB3	1762	583	0.06%	0.008%
42	6.918	1813	1828	1845	rBV	112093	214962	21.72%	2.971%
43	7.066	1872	1874	1879	rBV5	1758	1559	0.16%	0.022%
44	7.146	1897	1899	1900	rBV	1745	615	0.06%	0.009%
45	7.249	1920	1931	1950	rBV	401321	706803	71.40%	9.770%
46	7.558	2019	2027	2043	rBV	71703	127894	12.92%	1.768%
47	8.034	2166	2175	2206	rBV	166599	351207	35.48%	4.854%
48	8.789	2400	2410	2431	rBV	397732	653202	65.99%	9.029%
49	9.419	2604	2606	2611	rVB6	1748	1563	0.16%	0.022%
50	9.452	2611	2616	2617	rBV5	1335	1185	0.12%	0.016%
51	9.461	2617	2619	2621	rBV3	1541	949	0.10%	0.013%
52	9.519	2634	2637	2639	rBV4	1551	1231	0.12%	0.017%
53	9.628	2669	2671	2674	rVB4	1596	909	0.09%	0.013%
54	9.648	2674	2677	2679	rVB4	1539	818	0.08%	0.011%
55	9.712	2695	2697	2700	rBV4	1967	1188	0.12%	0.016%
56	9.728	2700	2702	2703	rVV2	1589	620	0.06%	0.009%
57	9.747	2706	2708	2713	rVB6	1294	805	0.08%	0.011%
58	10.101	2816	2818	2822	rVB5	1813	1315	0.13%	0.018%
59	10.159	2822	2836	2854	rBV	295385	468383	47.32%	6.474%
60	10.310	2881	2883	2887	rBV5	1965	1313	0.13%	0.018%
61	10.336	2888	2891	2896	rVV6	1738	1401	0.14%	0.019%
62	10.400	2907	2911	2913	rBV5	1615	838	0.08%	0.012%
63	10.432	2917	2921	2923	rBV5	2085	1284	0.13%	0.018%
64	10.487	2935	2938	2942	rBV6	1793	1322	0.13%	0.018%
65	10.532	2947	2952	2962	rBV6	2008	3070	0.31%	0.042%
66	10.570	2962	2964	2968	rVB4	1465	916	0.09%	0.013%
67	10.619	2975	2979	2983	rBV7	1432	1436	0.15%	0.020%
68	10.783	3028	3030	3031	rBV2	1794	815	0.08%	0.011%
69	10.953	3079	3083	3084	rBV4	1007	777	0.08%	0.011%
70	11.191	3147	3157	3174	rBV	423665	662711	66.95%	9.160%
71	11.448	3235	3237	3239	rVB3	1388	591	0.06%	0.008%
72	11.464	3239	3242	3244	rBV4	2006	1277	0.13%	0.018%
73	11.567	3262	3274	3291	rBV	435223	695423	70.25%	9.612%
74	11.828	3352	3355	3358	rBV4	2704	1750	0.18%	0.024%
75	11.889	3371	3374	3377	rBV4	1532	979	0.10%	0.014%
76	11.931	3383	3387	3390	rBV5	1012	1055	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031183.D
 Acq On : 23 May 2023 12:33
 Operator : SY/MD
 Sample : 02861-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.136	3449	3451	3452	rBV2	1495	722	0.07%	0.010%
78	12.287	3495	3498	3500	rBV4	1383	776	0.08%	0.011%
79	12.345	3514	3516	3518	rBV3	1965	780	0.08%	0.011%
80	12.503	3562	3565	3569	rVB6	1707	1234	0.12%	0.017%
81	12.529	3569	3573	3574	rBV4	1881	1249	0.13%	0.017%
82	12.558	3577	3582	3584	rBV5	1621	1441	0.15%	0.020%
83	12.590	3590	3592	3594	rBV3	1366	587	0.06%	0.008%
84	12.657	3611	3613	3614	rBV2	1098	600	0.06%	0.008%
85	12.750	3638	3642	3644	rBV6	1625	1119	0.11%	0.015%
86	12.818	3660	3663	3667	rVB4	2107	1213	0.12%	0.017%
87	13.127	3756	3759	3761	rBV4	2038	1425	0.14%	0.020%
88	13.239	3791	3794	3795	rBV3	1904	1051	0.11%	0.015%
89	13.310	3814	3816	3819	rVB3	2077	1063	0.11%	0.015%
90	13.332	3821	3823	3826	rBV4	1145	696	0.07%	0.010%
91	13.390	3839	3841	3844	rVB3	1295	656	0.07%	0.009%
92	13.429	3849	3853	3855	rBV5	1436	839	0.08%	0.012%
93	13.467	3863	3865	3867	rBV3	1250	649	0.07%	0.009%
94	13.676	3926	3930	3931	rBV3	1312	1013	0.10%	0.014%
95	13.866	3987	3989	3992	rBV4	1077	594	0.06%	0.008%
96	13.950	4013	4015	4018	rBV5	1770	1006	0.10%	0.014%
97	14.072	4051	4053	4054	rBV2	1862	742	0.07%	0.010%
98	14.291	4118	4121	4123	rBV4	2130	1500	0.15%	0.021%
99	14.731	4256	4258	4259	rBV2	1933	752	0.08%	0.010%
100	15.541	4508	4510	4512	rBV3	2411	1211	0.12%	0.017%




Sum of corrected areas: 7234691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031183.D
Acq On : 23 May 2023 12:33
Operator : SY/MD
Sample : 02861-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

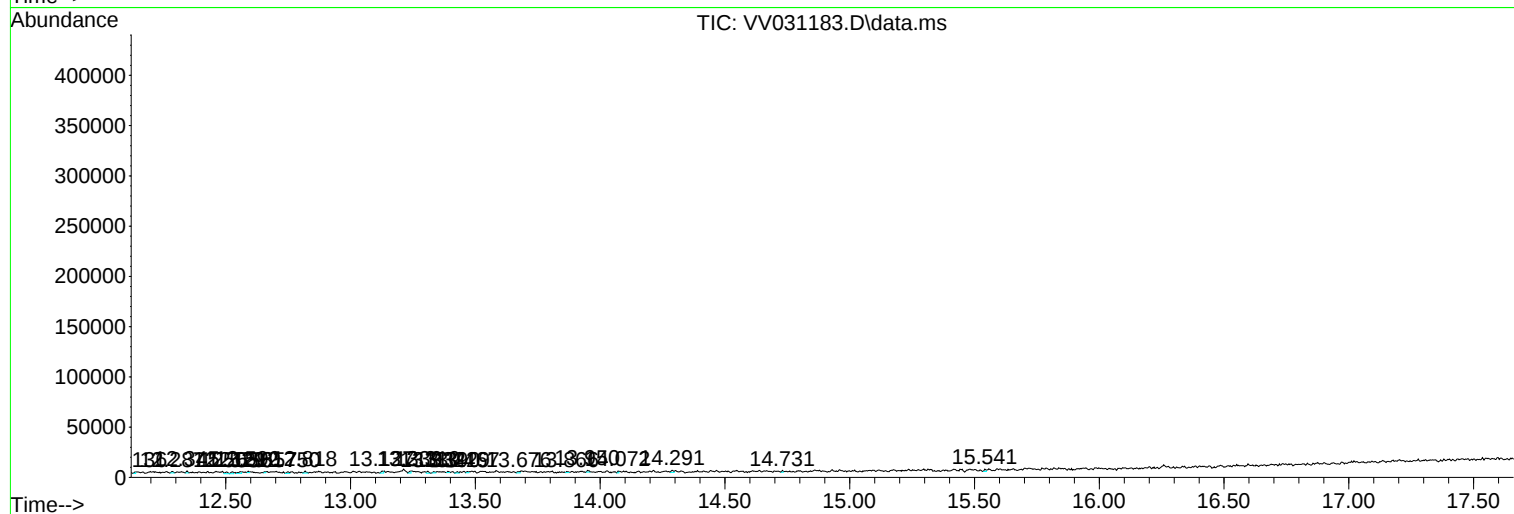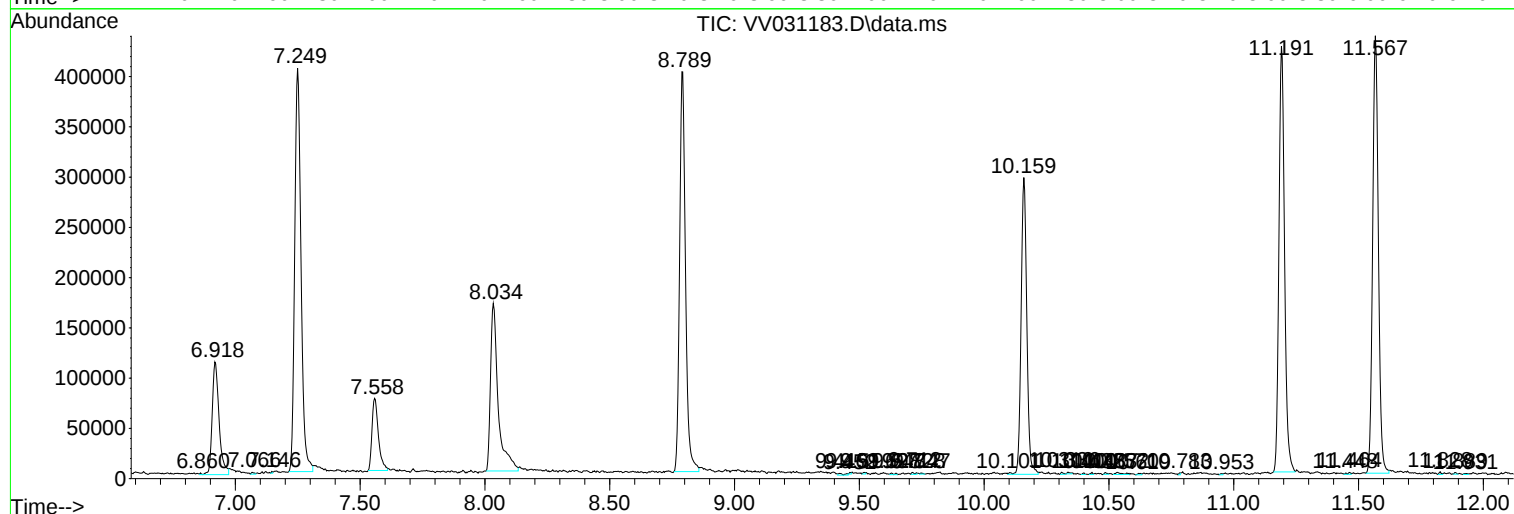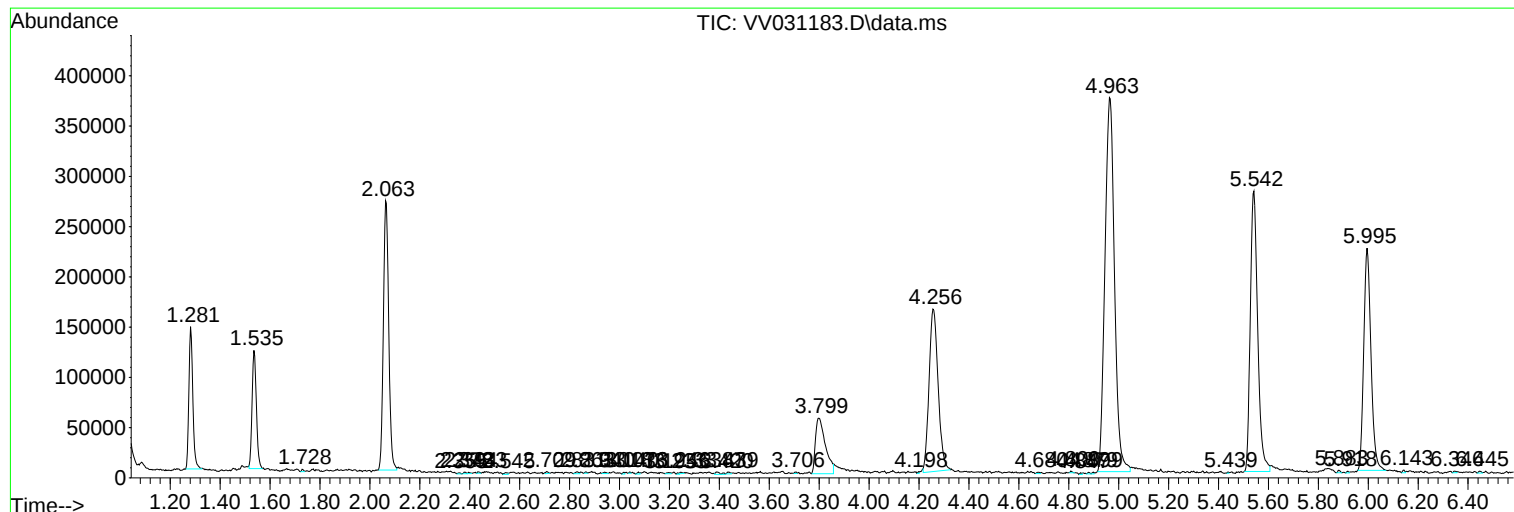

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031183.D
Acq On : 23 May 2023 12:33
Operator : SY/MD
Sample : 02861-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031183.D
Acq On : 23 May 2023 12:33
Operator : SY/MD
Sample : 02861-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------