

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031184.D
 Acq On : 23 May 2023 12:56
 Operator : SY/MD
 Sample : 02861-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	138605	154149	15.41%	2.340%
2	1.536	148	154	170	rVB	117677	147257	14.72%	2.236%
3	2.063	310	318	333	rVB	246356	354441	35.44%	5.381%
4	2.240	369	373	380	rBV10	2513	2981	0.30%	0.045%
5	2.407	423	425	428	rBV4	609	320	0.03%	0.005%
6	2.423	428	430	431	rVB2	1285	391	0.04%	0.006%
7	2.445	435	437	439	rBV2	1565	924	0.09%	0.014%
8	2.519	459	460	461	rBV	1138	388	0.04%	0.006%
9	2.590	480	482	486	rBV5	1207	617	0.06%	0.009%
10	2.744	528	530	534	rBV5	1533	1184	0.12%	0.018%
11	2.764	534	536	540	rVV3	1216	845	0.08%	0.013%
12	2.857	564	565	567	rBV2	1088	516	0.05%	0.008%
13	3.005	609	611	613	rBV3	1551	784	0.08%	0.012%
14	3.043	620	623	626	rVB5	2002	1241	0.12%	0.019%
15	3.060	626	628	632	rBV4	1232	982	0.10%	0.015%
16	3.111	641	644	646	rBV4	2055	1259	0.13%	0.019%
17	3.150	653	656	661	rVB6	2732	1950	0.19%	0.030%
18	3.172	661	663	665	rBV3	1530	757	0.08%	0.011%
19	3.195	665	670	672	rBV6	1261	1090	0.11%	0.017%
20	3.211	674	675	678	rVB3	1645	640	0.06%	0.010%
21	3.230	678	681	684	rBV4	1666	1281	0.13%	0.019%
22	3.278	694	696	698	rVB3	1991	747	0.07%	0.011%
23	3.346	715	717	722	rVB6	1773	1059	0.11%	0.016%
24	3.368	722	724	726	rBV3	981	399	0.04%	0.006%
25	3.394	730	732	734	rBV3	1071	466	0.05%	0.007%
26	3.445	746	748	750	rBV3	1005	506	0.05%	0.008%
27	3.497	761	764	765	rBV3	1507	878	0.09%	0.013%
28	3.526	769	773	775	rBV5	1829	1451	0.15%	0.022%
29	3.597	793	795	797	rBV3	1763	818	0.08%	0.012%
30	3.687	821	823	824	rBV2	1183	571	0.06%	0.009%
31	3.767	843	848	849	rBV4	1765	1581	0.16%	0.024%
32	3.802	849	859	886	rVV	56246	162681	16.26%	2.470%
33	4.259	987	1001	1026	rVB2	162430	405531	40.54%	6.156%
34	4.580	1099	1101	1103	rBV3	1078	513	0.05%	0.008%
35	4.632	1115	1117	1121	rVB4	2208	1333	0.13%	0.020%
36	4.693	1133	1136	1139	rBV5	1174	918	0.09%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031184.D
 Acq On : 23 May 2023 12:56
 Operator : SY/MD
 Sample : 02861-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.748	1150	1153	1156	rBV4	1095	684	0.07%	0.010%
38	4.812	1170	1173	1176	rVB4	942	627	0.06%	0.010%
39	4.825	1176	1177	1178	rBV	1038	266	0.03%	0.004%
40	4.841	1178	1182	1184	rVV5	1087	625	0.06%	0.009%
41	4.879	1192	1194	1197	rBV4	948	445	0.04%	0.007%
42	4.966	1203	1221	1246	rBV2	373423	1000247	100.00%	15.185%
43	5.336	1331	1336	1339	rBV5	1990	2129	0.21%	0.032%
44	5.542	1386	1400	1425	rBV	285737	601436	60.13%	9.130%
45	5.995	1530	1541	1561	rBV2	212840	433956	43.38%	6.588%
46	6.555	1712	1715	1716	rBV3	2066	1425	0.14%	0.022%
47	6.921	1819	1829	1850	rBV	101172	185261	18.52%	2.812%
48	7.249	1921	1931	1949	rBV	334493	585699	58.56%	8.891%
49	7.561	2019	2028	2042	rBV	62947	112195	11.22%	1.703%
50	8.034	2166	2175	2192	rBV	143607	289984	28.99%	4.402%
51	8.587	2345	2347	2348	rBV2	1819	808	0.08%	0.012%
52	8.792	2399	2411	2431	rBV	354553	606160	60.60%	9.202%
53	9.985	2781	2782	2784	rBV2	1757	539	0.05%	0.008%
54	10.159	2826	2836	2852	rBV2	235052	372116	37.20%	5.649%
55	10.583	2966	2968	2970	rVB3	2164	775	0.08%	0.012%
56	10.606	2970	2975	2978	rBV6	2264	2393	0.24%	0.036%
57	10.628	2981	2982	2984	rVB2	2244	596	0.06%	0.009%
58	11.191	3147	3157	3174	rBV	348950	562797	56.27%	8.544%
59	11.567	3263	3274	3289	rBV	356935	569843	56.97%	8.651%
60	12.709	3627	3629	3630	rBV	1564	516	0.05%	0.008%
61	13.603	3904	3907	3909	rBV3	1993	1299	0.13%	0.020%
62	14.397	4152	4154	4155	rBV2	2249	924	0.09%	0.014%




Sum of corrected areas: 6587194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031184.D
Acq On : 23 May 2023 12:56
Operator : SY/MD
Sample : 02861-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

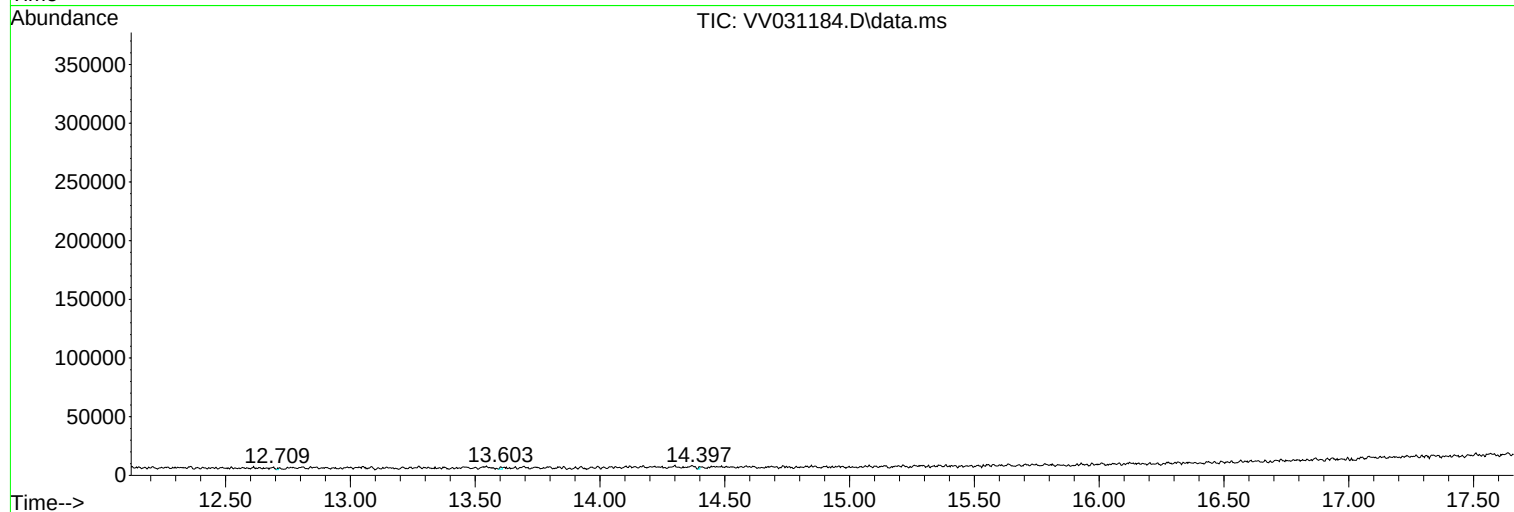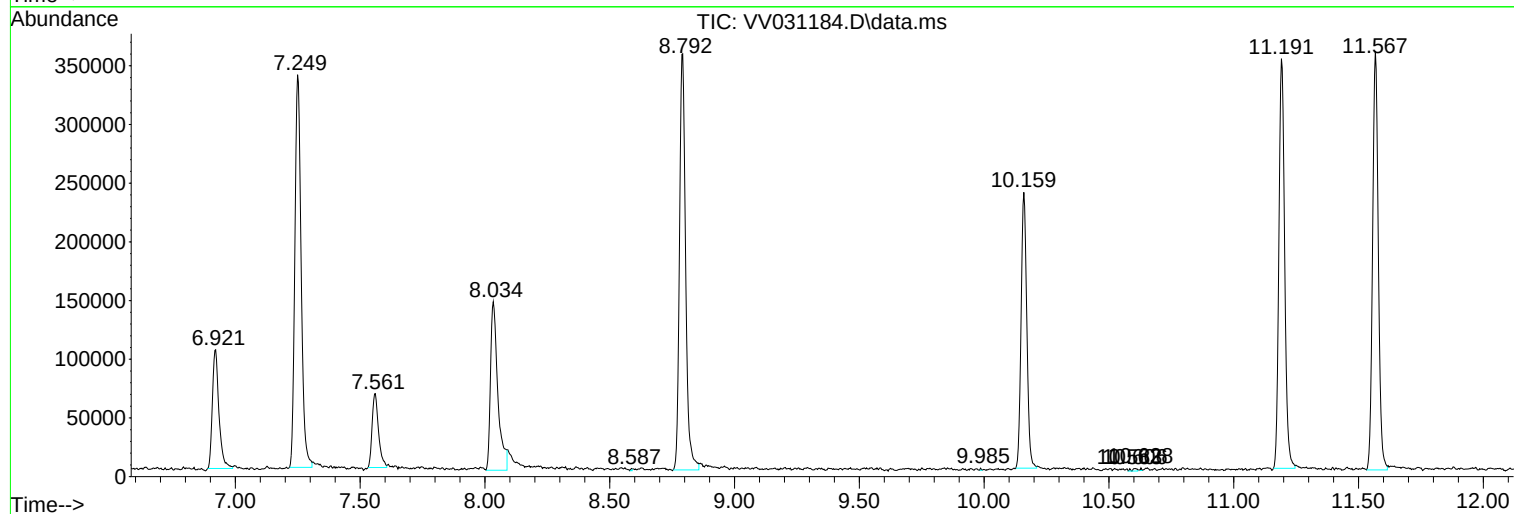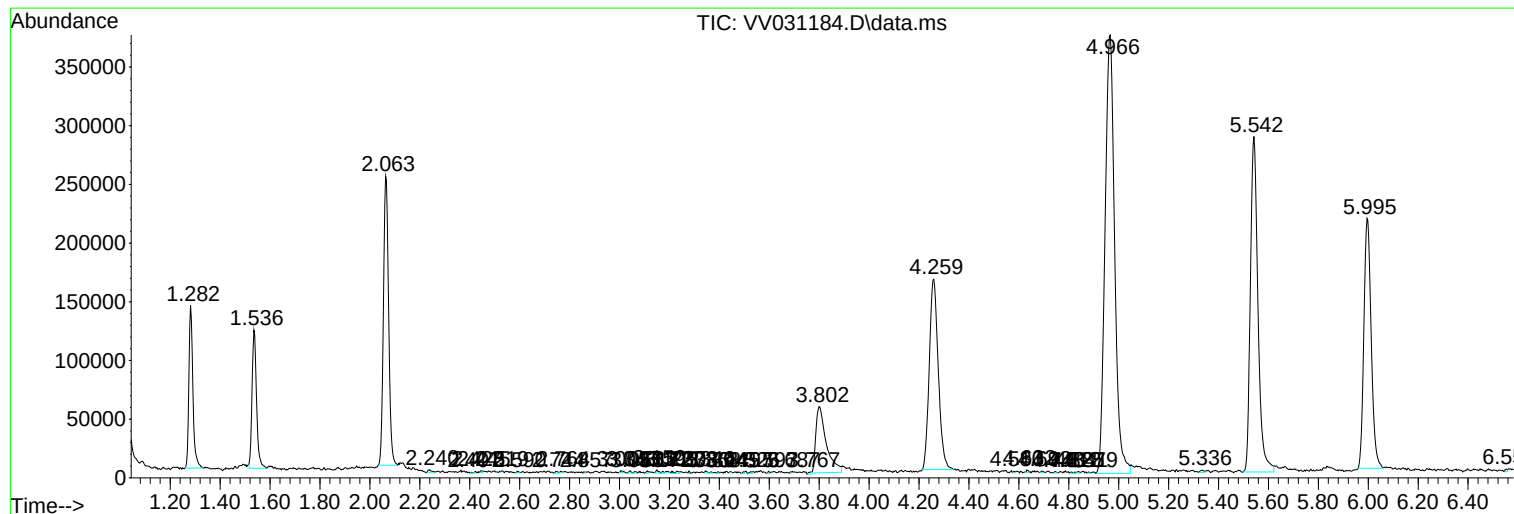

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031184.D
Acq On : 23 May 2023 12:56
Operator : SY/MD
Sample : 02861-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031184.D
Acq On : 23 May 2023 12:56
Operator : SY/MD
Sample : 02861-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------