

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031186.D
 Acq On : 23 May 2023 13:44
 Operator : SY/MD
 Sample : 02861-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rBV	110859	124222	15.59%	2.071%
2	1.535	148	154	169	rVB	109321	129357	16.23%	2.157%
3	2.066	309	319	333	rBV	213124	318808	40.00%	5.316%
4	2.220	364	367	368	rBV3	1554	972	0.12%	0.016%
5	2.494	450	452	454	rBV2	1624	977	0.12%	0.016%
6	2.577	477	478	482	rBV5	1219	822	0.10%	0.014%
7	2.760	532	535	538	rBV4	1583	1119	0.14%	0.019%
8	2.776	538	540	543	rBV4	1500	811	0.10%	0.014%
9	3.137	648	652	654	rBV5	2305	1497	0.19%	0.025%
10	3.252	685	688	690	rBV3	1270	705	0.09%	0.012%
11	3.284	695	698	699	rBV3	2206	1412	0.18%	0.024%
12	3.362	720	722	725	rVB5	2117	914	0.11%	0.015%
13	3.378	725	727	730	rVB4	2262	1070	0.13%	0.018%
14	3.397	730	733	737	rBV6	2235	1893	0.24%	0.032%
15	3.429	742	743	745	rVV2	1546	563	0.07%	0.009%
16	3.487	756	761	764	rBV6	2515	1847	0.23%	0.031%
17	3.503	764	766	768	rBV3	1429	833	0.10%	0.014%
18	3.545	778	779	781	rBV2	1949	1032	0.13%	0.017%
19	3.661	813	815	818	rBV4	1500	858	0.11%	0.014%
20	3.696	824	826	827	rBV2	1821	793	0.10%	0.013%
21	3.767	843	848	849	rBV5	1375	1356	0.17%	0.023%
22	3.799	849	858	877	rVV2	44915	122900	15.42%	2.049%
23	4.149	965	967	972	rBV5	1882	1412	0.18%	0.024%
24	4.198	978	982	983	rBV3	1158	770	0.10%	0.013%
25	4.259	988	1001	1024	rVB	131042	334200	41.93%	5.572%
26	4.747	1151	1153	1156	rBV4	2142	1337	0.17%	0.022%
27	4.966	1202	1221	1244	rBV2	296853	797037	100.00%	13.290%
28	5.236	1303	1305	1307	rBV2	1563	881	0.11%	0.015%
29	5.387	1350	1352	1356	rBV4	1640	989	0.12%	0.016%
30	5.426	1362	1364	1367	rBV4	1851	1074	0.13%	0.018%
31	5.542	1387	1400	1421	rBV	228365	489057	61.36%	8.155%
32	5.995	1531	1541	1563	rVB	174600	352004	44.16%	5.869%
33	6.307	1636	1638	1641	rBV4	2295	1431	0.18%	0.024%
34	6.529	1704	1707	1709	rBV4	1756	1171	0.15%	0.020%
35	6.596	1725	1728	1732	rVB4	2260	1430	0.18%	0.024%
36	6.667	1748	1750	1753	rBV4	1764	901	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031186.D
 Acq On : 23 May 2023 13:44
 Operator : SY/MD
 Sample : 02861-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.918	1818	1828	1843	rBV2	89043	164608	20.65%	2.745%
38	7.104	1884	1886	1889	rBV5	2850	2138	0.27%	0.036%
39	7.249	1921	1931	1946	rBV	332532	586639	73.60%	9.782%
40	7.561	2019	2028	2039	rBV	64649	110605	13.88%	1.844%
41	7.982	2155	2159	2162	rBV5	1570	1184	0.15%	0.020%
42	8.033	2167	2175	2206	rVV	137008	287616	36.09%	4.796%
43	8.368	2275	2279	2282	rBV6	1936	1612	0.20%	0.027%
44	8.439	2297	2301	2306	rBV7	1943	2214	0.28%	0.037%
45	8.493	2315	2318	2319	rBV3	1580	908	0.11%	0.015%
46	8.599	2349	2351	2353	rVB3	1498	708	0.09%	0.012%
47	8.632	2358	2361	2365	rVB5	1796	1129	0.14%	0.019%
48	8.664	2369	2371	2374	rBV4	1334	923	0.12%	0.015%
49	8.683	2374	2377	2379	rBV4	1197	840	0.11%	0.014%
50	8.792	2399	2411	2434	rBV	350540	589526	73.96%	9.830%
51	8.998	2473	2475	2478	rVB4	2497	1120	0.14%	0.019%
52	9.017	2478	2481	2483	rBV4	2047	1304	0.16%	0.022%
53	9.040	2487	2488	2491	rVB2	1089	515	0.06%	0.009%
54	9.056	2491	2493	2494	rBV2	1176	523	0.07%	0.009%
55	9.233	2544	2548	2550	rVV4	1188	856	0.11%	0.014%
56	9.249	2550	2553	2556	rVB5	831	606	0.08%	0.010%
57	9.307	2568	2571	2575	rVB7	1500	1003	0.13%	0.017%
58	9.374	2589	2592	2594	rBV4	2028	1079	0.14%	0.018%
59	9.439	2609	2612	2615	rBV6	2130	1516	0.19%	0.025%
60	9.503	2629	2632	2635	rBV5	1966	1407	0.18%	0.023%
61	9.615	2664	2667	2668	rBV2	1366	860	0.11%	0.014%
62	9.680	2681	2687	2689	rBV7	2096	1652	0.21%	0.028%
63	9.741	2705	2706	2709	rBV3	1354	758	0.10%	0.013%
64	9.776	2716	2717	2721	rBV4	1153	702	0.09%	0.012%
65	9.869	2743	2746	2748	rBV3	2596	1500	0.19%	0.025%
66	9.963	2772	2775	2777	rBV4	2228	1304	0.16%	0.022%
67	10.159	2826	2836	2849	rBV	231397	366901	46.03%	6.118%
68	10.394	2906	2909	2910	rBV3	2072	1003	0.13%	0.017%
69	10.519	2945	2948	2950	rBV4	1942	1123	0.14%	0.019%
70	10.638	2984	2985	2988	rVB3	2004	652	0.08%	0.011%
71	10.660	2990	2992	2996	rVB4	1559	818	0.10%	0.014%
72	10.709	3006	3007	3009	rBV2	1517	510	0.06%	0.009%
73	10.725	3009	3012	3013	rBV2	1348	764	0.10%	0.013%
74	10.754	3019	3021	3023	rBV3	1949	835	0.10%	0.014%
75	10.930	3072	3076	3077	rBV3	1918	1325	0.17%	0.022%
76	11.033	3105	3108	3115	rVB8	1983	1759	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031186.D
 Acq On : 23 May 2023 13:44
 Operator : SY/MD
 Sample : 02861-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.066	3115	3118	3122	rBV6	2541	2190	0.27%	0.037%
78	11.191	3146	3157	3176	rBV	352249	558864	70.12%	9.319%
79	11.397	3219	3221	3222	rBV2	1644	538	0.07%	0.009%
80	11.567	3262	3274	3293	rBV	348969	569807	71.49%	9.501%
81	11.783	3337	3341	3344	rBV6	1533	1494	0.19%	0.025%
82	11.956	3394	3395	3397	rBV2	1618	735	0.09%	0.012%
83	12.014	3410	3413	3416	rBV5	1572	1492	0.19%	0.025%
84	12.397	3530	3532	3537	rVB5	2539	2122	0.27%	0.035%
85	12.422	3537	3540	3542	rBV4	1484	907	0.11%	0.015%
86	12.435	3542	3544	3546	rBV3	1842	835	0.10%	0.014%
87	12.500	3560	3564	3565	rBV3	1734	1036	0.13%	0.017%
88	12.901	3687	3689	3691	rBV3	1531	785	0.10%	0.013%
89	13.053	3734	3736	3737	rBV2	1630	573	0.07%	0.010%
90	13.429	3850	3853	3856	rBV4	1915	1419	0.18%	0.024%
91	13.451	3858	3860	3861	rBV2	1654	695	0.09%	0.012%
92	13.500	3873	3875	3877	rBV3	2021	842	0.11%	0.014%
93	13.612	3908	3910	3913	rBV3	2097	987	0.12%	0.016%
94	13.699	3933	3937	3941	rBV5	2591	2634	0.33%	0.044%
95	13.795	3965	3967	3968	rBV2	1249	568	0.07%	0.009%
96	13.815	3972	3973	3975	rBV2	1445	736	0.09%	0.012%
97	13.963	4016	4019	4022	rBV5	1929	1591	0.20%	0.027%
98	14.098	4057	4061	4064	rBV6	2069	1723	0.22%	0.029%
99	14.155	4075	4079	4086	rBV10	2715	2578	0.32%	0.043%
100	15.062	4359	4361	4362	rBV2	1816	677	0.08%	0.011%




Sum of corrected areas: 5997328

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031186.D
Acq On : 23 May 2023 13:44
Operator : SY/MD
Sample : 02861-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

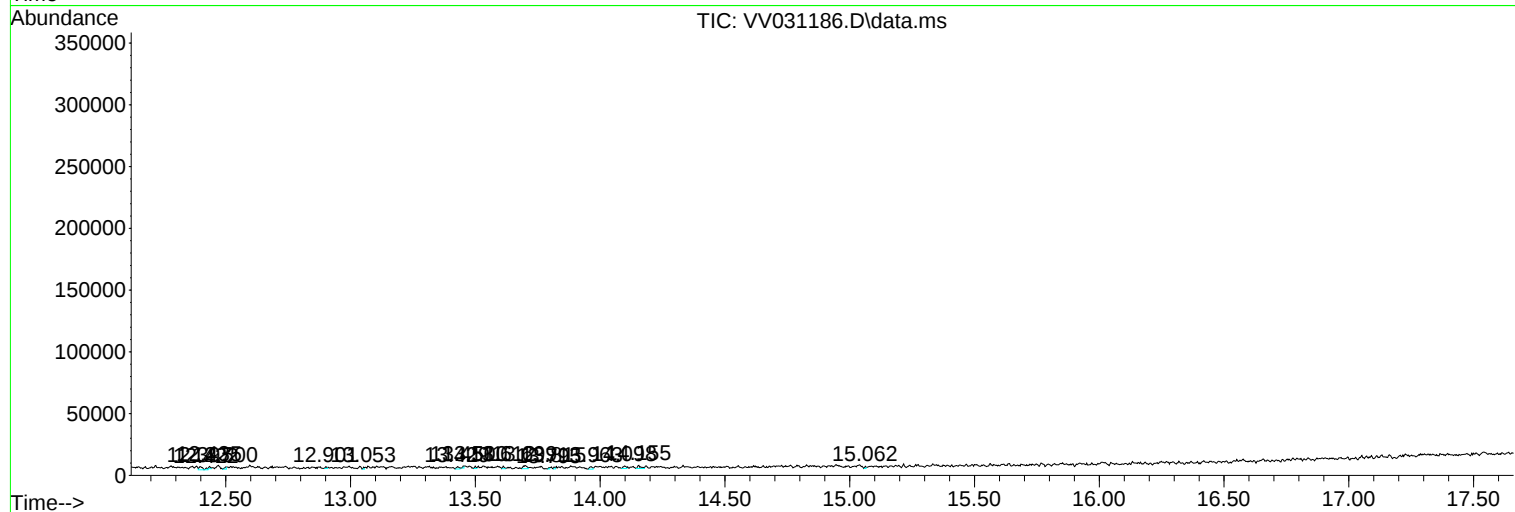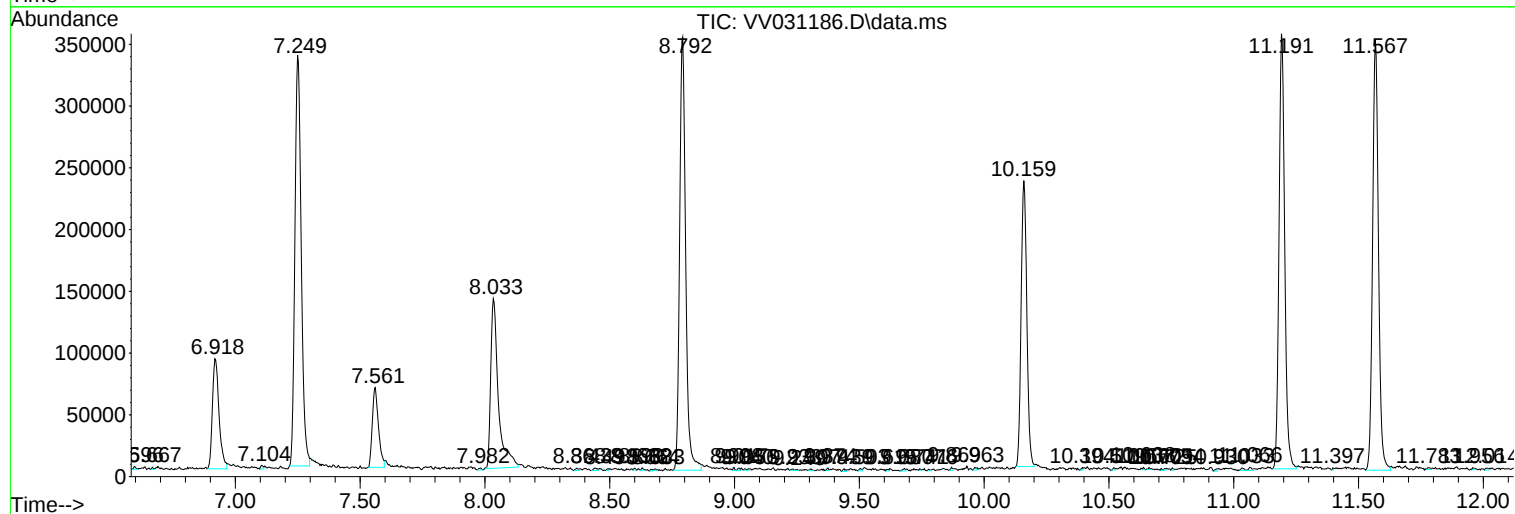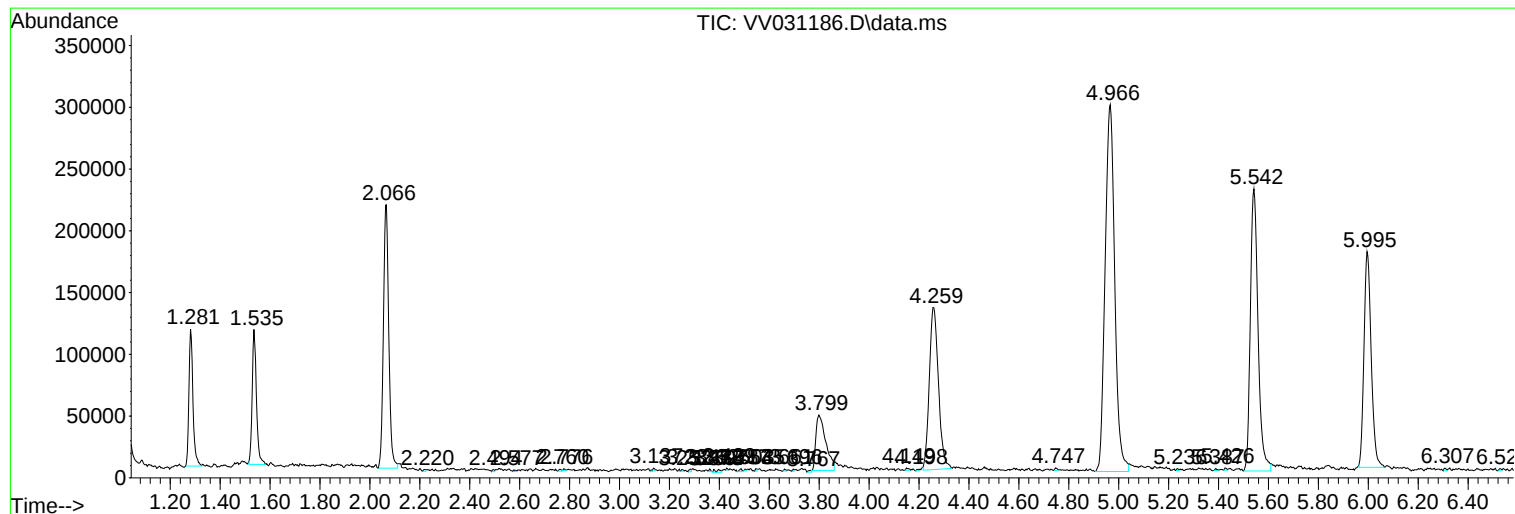

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031186.D
Acq On : 23 May 2023 13:44
Operator : SY/MD
Sample : 02861-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031186.D
Acq On : 23 May 2023 13:44
Operator : SY/MD
Sample : 02861-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------