

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031187.D
 Acq On : 23 May 2023 14:08
 Operator : SY/MD
 Sample : 02861-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	94	rVB	110716	122787	16.54%	2.095%
2	1.536	148	154	168	rVB	110078	129105	17.39%	2.202%
3	2.063	310	318	334	rVB	209563	304600	41.02%	5.196%
4	2.349	405	407	409	rBV3	2245	1009	0.14%	0.017%
5	2.391	415	420	423	rBV6	2182	2329	0.31%	0.040%
6	2.764	535	536	537	rBV	1959	718	0.10%	0.012%
7	2.953	592	595	596	rBV3	1055	740	0.10%	0.013%
8	3.114	643	645	647	rBV3	2285	1158	0.16%	0.020%
9	3.169	657	662	666	rBV7	2360	2490	0.34%	0.042%
10	3.188	666	668	673	rVV6	1528	1006	0.14%	0.017%
11	3.384	727	729	731	rBV3	1206	563	0.08%	0.010%
12	3.397	731	733	735	rVB3	1223	510	0.07%	0.009%
13	3.413	735	738	739	rBV3	1167	623	0.08%	0.011%
14	3.433	742	744	746	rBV3	1861	1188	0.16%	0.020%
15	3.574	785	788	790	rBV4	1353	866	0.12%	0.015%
16	3.645	808	810	814	rBV5	1754	916	0.12%	0.016%
17	3.690	822	824	825	rBV2	1652	593	0.08%	0.010%
18	3.799	850	858	886	rBV	43853	130156	17.53%	2.220%
19	4.259	987	1001	1025	rBV	129446	332506	44.78%	5.672%
20	4.577	1098	1100	1101	rBV2	1922	1057	0.14%	0.018%
21	4.609	1108	1110	1115	rBV5	1665	1554	0.21%	0.027%
22	4.674	1128	1130	1134	rBV5	2185	1381	0.19%	0.024%
23	4.751	1152	1154	1155	rBV2	1938	677	0.09%	0.012%
24	4.963	1207	1220	1242	rVB2	288520	742576	100.00%	12.667%
25	5.468	1374	1377	1385	rVB9	2647	2412	0.32%	0.041%
26	5.542	1388	1400	1421	rBV	212136	442026	59.53%	7.540%
27	5.998	1530	1542	1561	rBV	178402	359750	48.45%	6.137%
28	6.185	1598	1600	1603	rVB4	2248	989	0.13%	0.017%
29	6.542	1709	1711	1714	rBV4	2157	1370	0.18%	0.023%
30	6.767	1777	1781	1784	rBV6	2470	2208	0.30%	0.038%
31	6.918	1819	1828	1846	rBV	87121	161529	21.75%	2.755%
32	7.101	1883	1885	1887	rBV3	2159	910	0.12%	0.016%
33	7.249	1921	1931	1958	rBV	334836	602059	81.08%	10.270%
34	7.558	2020	2027	2046	rVB2	63593	112019	15.09%	1.911%
35	8.034	2166	2175	2208	rBV	143545	308921	41.60%	5.270%
36	8.464	2306	2309	2311	rBV4	1684	1142	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031187.D
 Acq On : 23 May 2023 14:08
 Operator : SY/MD
 Sample : 02861-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	8.510	2321	2323	2326	rBV3	1746	1059	0.14%	0.018%
38	8.792	2400	2411	2432	rBV	329731	553322	74.51%	9.439%
39	9.091	2502	2504	2505	rBV2	1788	668	0.09%	0.011%
40	9.210	2537	2541	2547	rBV8	2108	2054	0.28%	0.035%
41	9.233	2547	2548	2551	rBV3	1768	937	0.13%	0.016%
42	9.744	2705	2707	2711	rBB4	1678	1054	0.14%	0.018%
43	9.767	2711	2714	2717	rBV4	1924	1493	0.20%	0.025%
44	9.854	2739	2741	2745	rBV5	2261	1655	0.22%	0.028%
45	10.098	2815	2817	2820	rBV4	1811	1088	0.15%	0.019%
46	10.114	2820	2822	2823	rVV3	1562	460	0.06%	0.008%
47	10.159	2825	2836	2849	rVV	237666	374219	50.39%	6.384%
48	10.667	2989	2994	2997	rBV6	1666	1570	0.21%	0.027%
49	10.725	3010	3012	3015	rBV3	1300	663	0.09%	0.011%
50	10.834	3044	3046	3048	rBV2	1185	490	0.07%	0.008%
51	11.011	3098	3101	3102	rBV3	986	672	0.09%	0.011%
52	11.043	3109	3111	3117	rVB6	2045	1766	0.24%	0.030%
53	11.194	3147	3158	3178	rBV	329703	522122	70.31%	8.907%
54	11.464	3240	3242	3246	rBV5	1958	1471	0.20%	0.025%
55	11.567	3263	3274	3291	rBV	357586	568700	76.58%	9.701%
56	12.069	3428	3430	3432	rBV3	1229	535	0.07%	0.009%
57	12.143	3451	3453	3456	rBV4	2170	1609	0.22%	0.027%
58	12.252	3484	3487	3489	rBV4	931	624	0.08%	0.011%
59	12.291	3497	3499	3500	rBV2	1248	576	0.08%	0.010%
60	12.339	3511	3514	3519	rBV6	1725	1789	0.24%	0.031%
61	12.468	3551	3554	3556	rBV5	1850	1279	0.17%	0.022%
62	12.480	3556	3558	3560	rVV3	1219	551	0.07%	0.009%
63	12.519	3568	3570	3574	rVB4	1287	731	0.10%	0.012%
64	12.541	3574	3577	3578	rBV2	1815	891	0.12%	0.015%
65	12.593	3589	3593	3597	rBV6	2335	1892	0.25%	0.032%
66	12.632	3602	3605	3607	rBV5	1196	907	0.12%	0.015%
67	12.689	3619	3623	3624	rBV3	1236	823	0.11%	0.014%
68	12.728	3632	3635	3637	rBV4	1836	1111	0.15%	0.019%
69	12.757	3641	3644	3647	rBV4	1166	626	0.08%	0.011%
70	12.786	3652	3653	3657	rVB4	1502	764	0.10%	0.013%
71	12.976	3709	3712	3715	rBV5	1933	1689	0.23%	0.029%
72	13.040	3730	3732	3735	rVB3	1912	955	0.13%	0.016%
73	13.075	3741	3743	3745	rBV2	1535	843	0.11%	0.014%
74	13.098	3748	3750	3752	rBV4	1278	708	0.10%	0.012%
75	13.191	3777	3779	3783	rBV5	1892	1646	0.22%	0.028%
76	13.252	3795	3798	3800	rBV3	1335	579	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031187.D
 Acq On : 23 May 2023 14:08
 Operator : SY/MD
 Sample : 02861-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	13.268	3800	3803	3805	rVV3	880	448	0.06%	0.008%
78	13.339	3823	3825	3828	rVB3	1681	609	0.08%	0.010%
79	13.371	3833	3835	3840	rBV5	1834	1395	0.19%	0.024%
80	13.455	3859	3861	3866	rBV5	1586	1429	0.19%	0.024%
81	13.490	3870	3872	3875	rVB3	1899	971	0.13%	0.017%
82	13.506	3875	3877	3880	rBV4	2081	1465	0.20%	0.025%
83	13.574	3894	3898	3899	rBV3	1873	1387	0.19%	0.024%
84	13.638	3915	3918	3921	rVB5	1917	1337	0.18%	0.023%
85	13.657	3921	3924	3926	rBV4	1484	868	0.12%	0.015%
86	13.670	3926	3928	3929	rBV2	1374	502	0.07%	0.009%
87	13.747	3950	3952	3955	rVB4	2368	1078	0.15%	0.018%
88	13.767	3955	3958	3959	rBV3	741	431	0.06%	0.007%
89	13.792	3964	3966	3968	rVV3	2124	1076	0.14%	0.018%
90	13.818	3972	3974	3975	rBV2	1323	478	0.06%	0.008%
91	13.850	3981	3984	3987	rVB4	2097	1085	0.15%	0.019%
92	13.911	4000	4003	4008	rBV6	1980	1977	0.27%	0.034%
93	13.998	4028	4030	4034	rBV5	1676	1378	0.19%	0.024%
94	14.049	4041	4046	4047	rBV5	1953	1652	0.22%	0.028%
95	14.107	4060	4064	4067	rBV6	2292	1843	0.25%	0.031%
96	14.143	4073	4075	4079	rVB4	2039	1251	0.17%	0.021%
97	14.210	4094	4096	4099	rBV4	1570	678	0.09%	0.012%
98	14.493	4180	4184	4188	rBV6	2678	2541	0.34%	0.043%
99	14.593	4213	4215	4217	rBV3	1533	733	0.10%	0.013%
100	15.242	4413	4417	4420	rBV6	2935	2566	0.35%	0.044%




Sum of corrected areas: 5862212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031187.D
Acq On : 23 May 2023 14:08
Operator : SY/MD
Sample : 02861-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

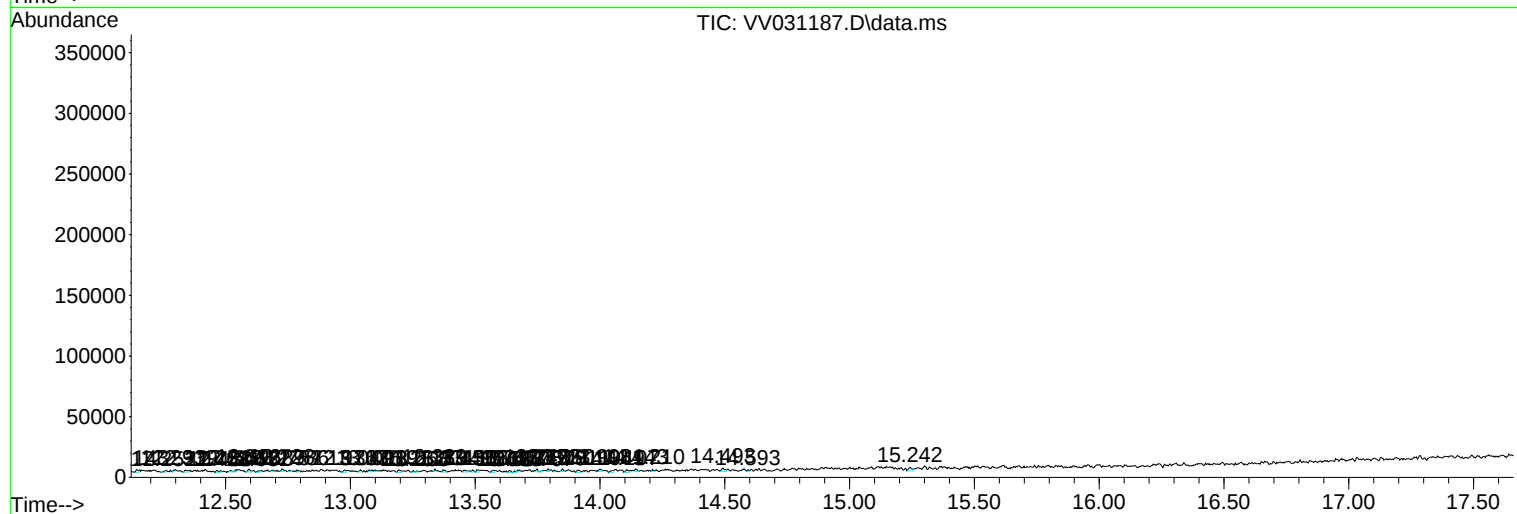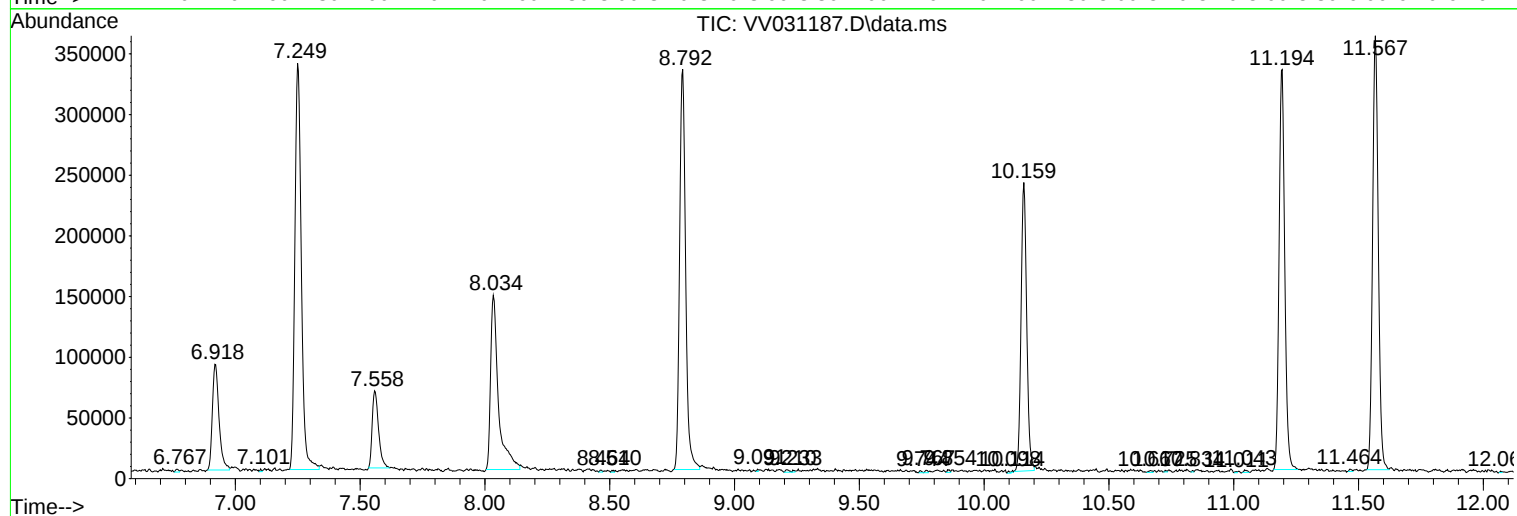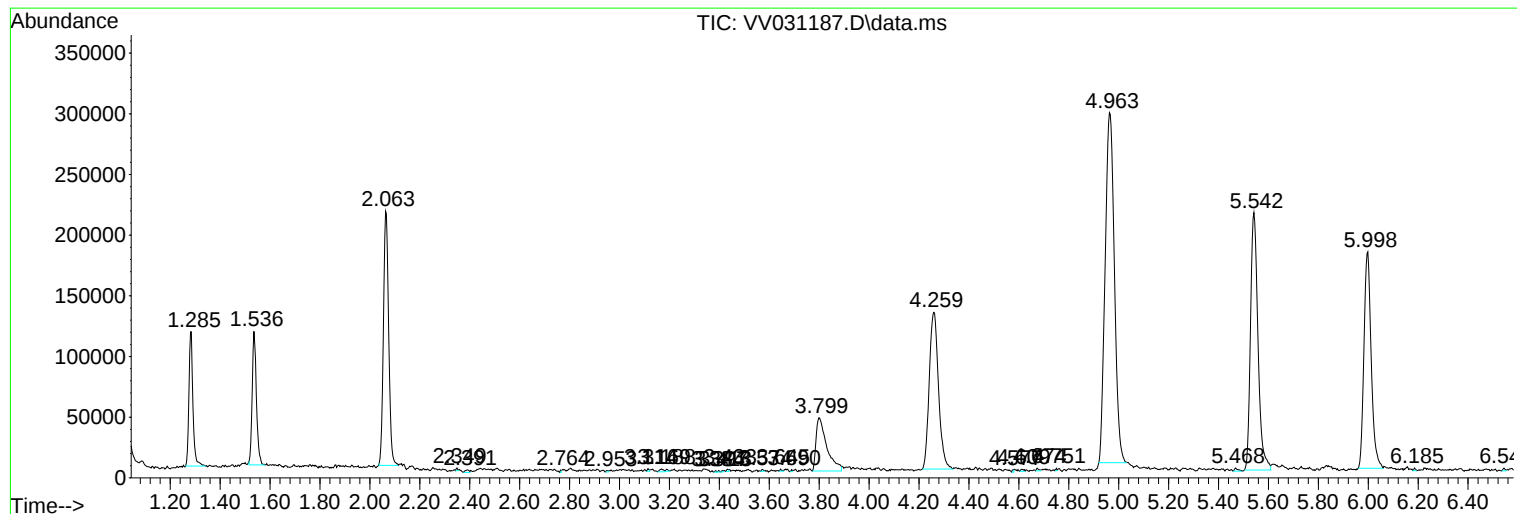

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031187.D
Acq On : 23 May 2023 14:08
Operator : SY/MD
Sample : 02861-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031187.D
Acq On : 23 May 2023 14:08
Operator : SY/MD
Sample : 02861-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc