

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031188.D
 Acq On : 23 May 2023 14:32
 Operator : SY/MD
 Sample : 02861-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	109889	117312	15.02%	1.899%
2	1.536	148	154	166	rVB	111018	126752	16.23%	2.052%
3	2.063	309	318	332	rBV	211025	305669	39.15%	4.948%
4	2.191	357	358	361	rBV3	1551	678	0.09%	0.011%
5	2.420	427	429	431	rBV3	1144	613	0.08%	0.010%
6	2.510	455	457	458	rBV2	1639	675	0.09%	0.011%
7	2.622	489	492	494	rBV3	2083	1772	0.23%	0.029%
8	2.648	497	500	506	rVV8	1338	1543	0.20%	0.025%
9	2.899	575	578	582	rBV6	1639	1288	0.16%	0.021%
10	3.346	715	717	719	rBV3	1808	819	0.10%	0.013%
11	3.465	752	754	760	rVB6	2827	1580	0.20%	0.026%
12	3.584	789	791	793	rBV3	1946	1014	0.13%	0.016%
13	3.770	847	849	850	rBV2	1593	714	0.09%	0.012%
14	3.799	850	858	887	rVV	44715	130582	16.72%	2.114%
15	4.256	989	1000	1023	rVB	131654	326799	41.85%	5.290%
16	4.825	1173	1177	1178	rBV4	1761	1421	0.18%	0.023%
17	4.966	1205	1221	1241	rBV3	296951	780826	100.00%	12.641%
18	5.330	1333	1334	1335	rBV	1811	626	0.08%	0.010%
19	5.420	1359	1362	1364	rBV4	1665	821	0.11%	0.013%
20	5.542	1388	1400	1417	rBV	267202	547035	70.06%	8.856%
21	5.995	1531	1541	1558	rVB	172509	343234	43.96%	5.557%
22	6.288	1630	1632	1633	rBV2	1613	659	0.08%	0.011%
23	6.860	1808	1810	1812	rBV3	1659	653	0.08%	0.011%
24	6.921	1818	1829	1849	rBV2	88175	167314	21.43%	2.709%
25	7.249	1920	1931	1949	rBV	339387	599660	76.80%	9.708%
26	7.558	2018	2027	2047	rBV	67158	126461	16.20%	2.047%
27	8.034	2166	2175	2189	rBV	146602	281981	36.11%	4.565%
28	8.792	2400	2411	2427	rBV	414996	681073	87.22%	11.026%
29	9.458	2616	2618	2620	rBV3	1569	774	0.10%	0.013%
30	9.593	2657	2660	2664	rBV6	1910	1589	0.20%	0.026%
31	9.850	2739	2740	2742	rBV2	1169	639	0.08%	0.010%
32	9.927	2760	2764	2765	rBV4	1779	1108	0.14%	0.018%
33	10.159	2823	2836	2851	rBV	240655	390266	49.98%	6.318%
34	10.484	2933	2937	2940	rBV5	3951	3361	0.43%	0.054%
35	10.683	2996	2999	3000	rBV3	1620	864	0.11%	0.014%
36	10.937	3075	3078	3079	rBV3	1274	737	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031188.D
 Acq On : 23 May 2023 14:32
 Operator : SY/MD
 Sample : 02861-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	10.992	3092	3095	3098	rBV5	3197	2274	0.29%	0.037%
38	11.098	3124	3128	3133	rVB8	1765	1297	0.17%	0.021%
39	11.124	3133	3136	3137	rBV3	1905	981	0.13%	0.016%
40	11.191	3146	3157	3178	rBV	399385	639238	81.87%	10.348%
41	11.313	3192	3195	3196	rBV3	1504	1020	0.13%	0.017%
42	11.397	3219	3221	3222	rBV2	1109	311	0.04%	0.005%
43	11.426	3228	3230	3236	rVB6	1147	656	0.08%	0.011%
44	11.567	3262	3274	3289	rBV	357702	563027	72.11%	9.115%
45	12.011	3409	3412	3413	rBV3	2449	1272	0.16%	0.021%
46	12.185	3464	3466	3469	rBV4	1525	909	0.12%	0.015%
47	12.223	3476	3478	3483	rBV5	1346	1326	0.17%	0.021%
48	12.291	3497	3499	3500	rBV2	1288	375	0.05%	0.006%
49	12.410	3533	3536	3539	rBV4	1303	906	0.12%	0.015%
50	12.429	3539	3542	3546	rBV6	1810	1546	0.20%	0.025%
51	12.815	3659	3662	3663	rBV3	1541	902	0.12%	0.015%
52	12.998	3717	3719	3720	rBV2	1142	337	0.04%	0.005%
53	13.156	3766	3768	3771	rBV4	1715	1229	0.16%	0.020%
54	13.236	3791	3793	3796	rBV3	1550	948	0.12%	0.015%
55	13.287	3805	3809	3812	rBV6	2284	1836	0.24%	0.030%
56	13.773	3958	3960	3963	rBV4	1754	893	0.11%	0.014%
57	13.840	3978	3981	3982	rBV3	2107	1371	0.18%	0.022%
58	14.638	4227	4229	4230	rBV2	2012	901	0.12%	0.015%
59	14.975	4332	4334	4335	rBV2	1251	481	0.06%	0.008%
60	15.130	4377	4382	4387	rBV7	3004	3230	0.41%	0.052%
61	15.233	4413	4414	4416	rBV2	2052	975	0.12%	0.016%




Sum of corrected areas: 6177153

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031188.D
Acq On : 23 May 2023 14:32
Operator : SY/MD
Sample : 02861-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

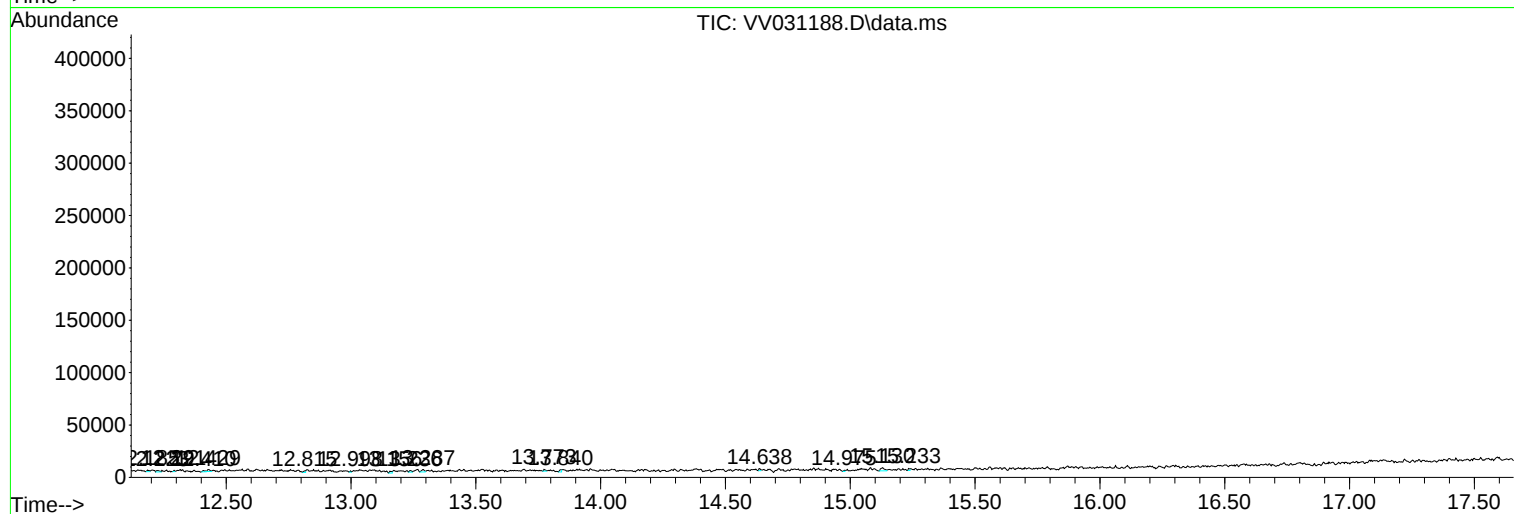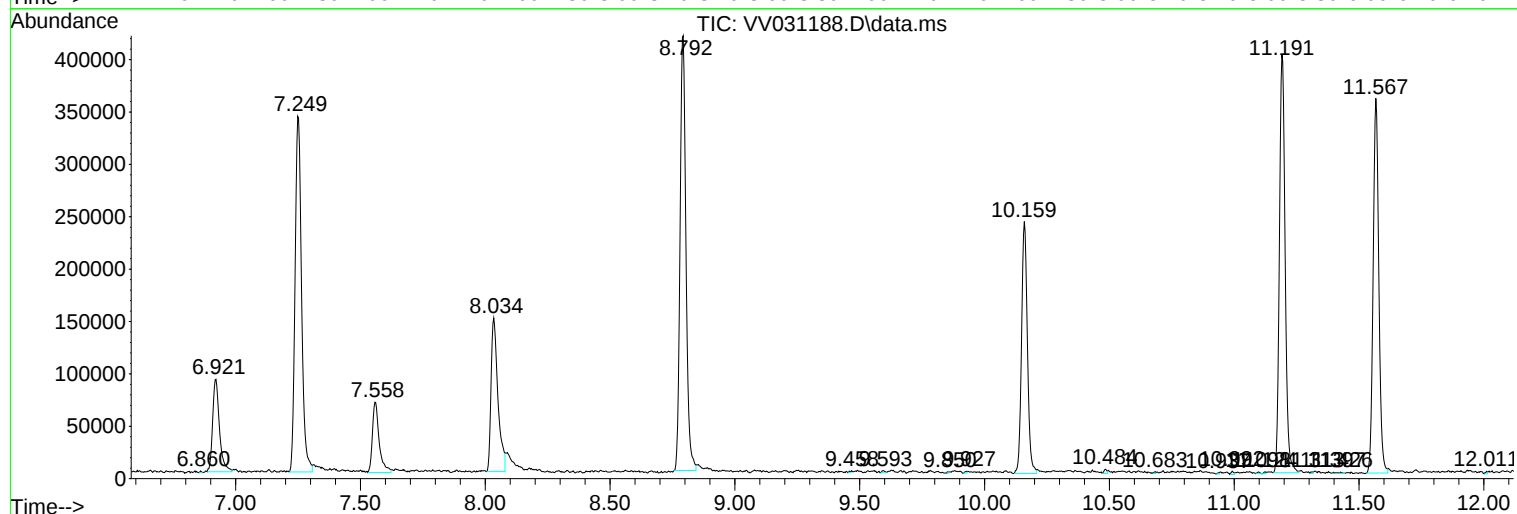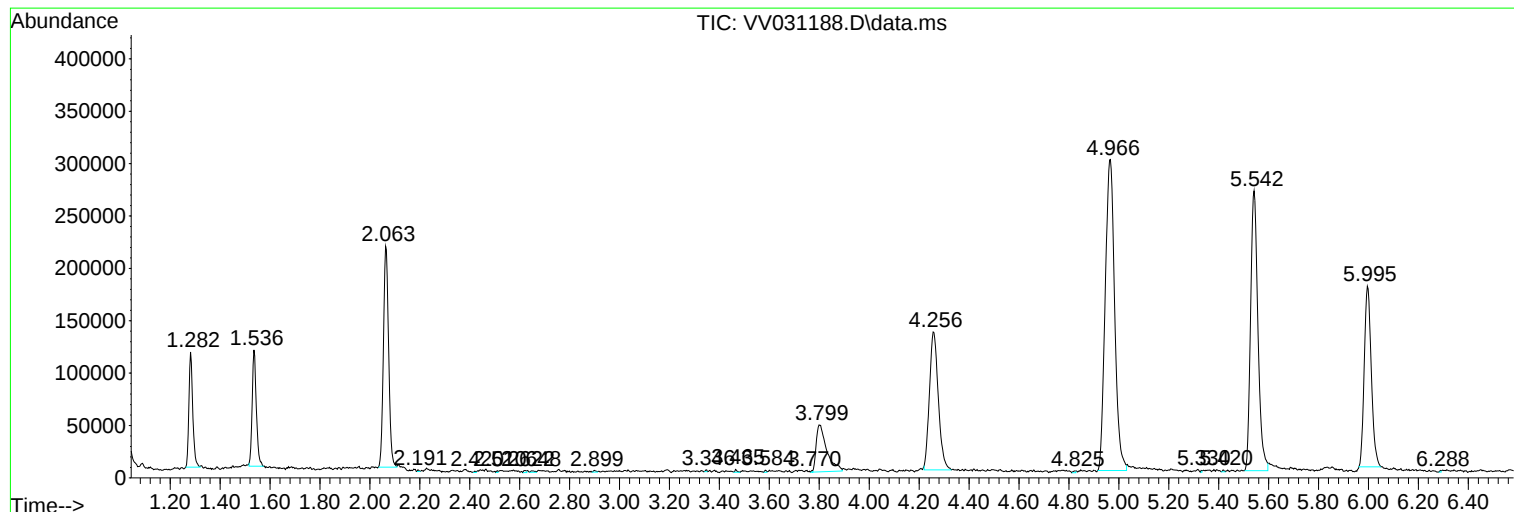

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031188.D
Acq On : 23 May 2023 14:32
Operator : SY/MD
Sample : 02861-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031188.D
Acq On : 23 May 2023 14:32
Operator : SY/MD
Sample : 02861-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------