

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031189.D
 Acq On : 23 May 2023 14:56
 Operator : SY/MD
 Sample : 02861-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	108088	117309	15.28%	2.014%
2	1.536	148	154	165	rVB	100760	120826	15.74%	2.074%
3	2.063	309	318	333	rBV	205536	300092	39.09%	5.152%
4	2.217	364	366	367	rBV2	1469	506	0.07%	0.009%
5	2.433	431	433	436	rBV4	1836	821	0.11%	0.014%
6	2.462	439	442	443	rBV3	1247	615	0.08%	0.011%
7	2.561	471	473	477	rBV4	961	532	0.07%	0.009%
8	2.600	480	485	486	rBV4	1284	804	0.10%	0.014%
9	2.664	503	505	507	rBV3	2189	1298	0.17%	0.022%
10	2.690	510	513	514	rBV3	1466	940	0.12%	0.016%
11	2.876	567	571	574	rBV6	3026	1970	0.26%	0.034%
12	3.044	620	623	625	rBV4	1148	706	0.09%	0.012%
13	3.114	642	645	647	rVV4	1854	995	0.13%	0.017%
14	3.162	657	660	663	rBV5	1720	1043	0.14%	0.018%
15	3.207	668	674	678	rBV8	1754	2353	0.31%	0.040%
16	3.252	686	688	689	rBV2	1547	695	0.09%	0.012%
17	3.333	710	713	717	rBV6	1954	1577	0.21%	0.027%
18	3.632	803	806	809	rBV5	1544	1032	0.13%	0.018%
19	3.744	840	841	845	rBV4	1477	837	0.11%	0.014%
20	3.802	849	859	877	rBV	44686	120435	15.69%	2.068%
21	4.130	959	961	964	rBV4	1484	720	0.09%	0.012%
22	4.256	980	1000	1028	rBV	126637	341845	44.53%	5.869%
23	4.609	1105	1110	1113	rVB7	1874	1875	0.24%	0.032%
24	4.822	1172	1176	1177	rBV4	1666	1347	0.18%	0.023%
25	4.896	1197	1199	1205	rBV6	2432	2879	0.38%	0.049%
26	4.966	1205	1221	1239	rBV2	291254	767700	100.00%	13.180%
27	5.220	1298	1300	1303	rVB4	2409	1268	0.17%	0.022%
28	5.449	1368	1371	1373	rBV3	1320	1033	0.13%	0.018%
29	5.542	1389	1400	1418	rBV	225160	453169	59.03%	7.780%
30	5.748	1462	1464	1467	rBV3	1972	1201	0.16%	0.021%
31	5.812	1479	1484	1485	rBV5	2718	2522	0.33%	0.043%
32	5.995	1531	1541	1566	rVB	171215	350251	45.62%	6.013%
33	6.378	1658	1660	1661	rBV3	1919	682	0.09%	0.012%
34	6.452	1681	1683	1686	rVB3	1498	861	0.11%	0.015%
35	6.497	1695	1697	1701	rBV5	1287	778	0.10%	0.013%
36	6.587	1723	1725	1727	rBV3	1048	533	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031189.D
 Acq On : 23 May 2023 14:56
 Operator : SY/MD
 Sample : 02861-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.719	1760	1766	1768	rBV6	2699	2494	0.32%	0.043%
38	6.783	1782	1786	1787	rBV4	2237	1734	0.23%	0.030%
39	6.921	1819	1829	1846	rBV	85498	159603	20.79%	2.740%
40	7.249	1921	1931	1951	rBV2	328447	576542	75.10%	9.898%
41	7.561	2020	2028	2039	rBV	60457	98232	12.80%	1.686%
42	8.034	2166	2175	2192	rBV	142076	279791	36.45%	4.803%
43	8.455	2304	2306	2310	rBV4	1718	1264	0.16%	0.022%
44	8.561	2336	2339	2340	rBV3	1161	640	0.08%	0.011%
45	8.792	2400	2411	2434	rBV	347414	580094	75.56%	9.959%
46	9.294	2563	2567	2570	rBV5	2582	2204	0.29%	0.038%
47	9.464	2619	2620	2624	rVB4	1932	988	0.13%	0.017%
48	9.661	2679	2681	2682	rBV2	1540	567	0.07%	0.010%
49	9.690	2686	2690	2691	rBV4	1398	921	0.12%	0.016%
50	9.802	2722	2725	2729	rVB6	2018	1300	0.17%	0.022%
51	9.821	2729	2731	2734	rVB4	1657	1065	0.14%	0.018%
52	9.837	2734	2736	2740	rBV4	1542	1348	0.18%	0.023%
53	9.927	2762	2764	2767	rVB4	1772	688	0.09%	0.012%
54	9.947	2767	2770	2772	rBV3	1116	622	0.08%	0.011%
55	10.018	2790	2792	2796	rVB5	2642	1545	0.20%	0.027%
56	10.040	2796	2799	2800	rBV3	1863	941	0.12%	0.016%
57	10.159	2825	2836	2848	rBV	228190	365906	47.66%	6.282%
58	10.326	2885	2888	2892	rBV6	2430	1834	0.24%	0.031%
59	10.448	2924	2926	2928	rBV3	1199	609	0.08%	0.010%
60	10.468	2928	2932	2933	rBV3	1065	721	0.09%	0.012%
61	10.509	2942	2945	2949	rBV6	1715	1379	0.18%	0.024%
62	10.567	2959	2963	2964	rBV4	1805	1263	0.16%	0.022%
63	10.702	3003	3005	3007	rBV3	1140	674	0.09%	0.012%
64	10.783	3027	3030	3031	rBV3	1617	896	0.12%	0.015%
65	10.815	3039	3040	3045	rVB5	1429	981	0.13%	0.017%
66	10.911	3067	3070	3076	rVB7	3359	2559	0.33%	0.044%
67	10.937	3076	3078	3081	rBV4	1232	985	0.13%	0.017%
68	10.966	3085	3087	3090	rVB3	1370	498	0.06%	0.009%
69	11.008	3097	3100	3101	rBV3	1798	765	0.10%	0.013%
70	11.107	3129	3131	3134	rBV4	1322	951	0.12%	0.016%
71	11.156	3144	3146	3147	rBV2	1998	866	0.11%	0.015%
72	11.191	3147	3157	3173	rVV	337895	542569	70.67%	9.315%
73	11.567	3263	3274	3292	rBV	348655	554963	72.29%	9.528%
74	11.734	3324	3326	3328	rBV3	1899	989	0.13%	0.017%
75	12.191	3465	3468	3469	rBV3	1111	618	0.08%	0.011%
76	12.204	3470	3472	3474	rVB3	1287	594	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031189.D
 Acq On : 23 May 2023 14:56
 Operator : SY/MD
 Sample : 02861-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.230	3477	3480	3483	rBV4	2628	1770	0.23%	0.030%
78	12.249	3484	3486	3489	rBV4	1360	901	0.12%	0.015%
79	12.320	3506	3508	3515	rVB7	1454	1123	0.15%	0.019%
80	12.352	3515	3518	3519	rBV3	1563	887	0.12%	0.015%
81	12.535	3573	3575	3578	rBV3	699	528	0.07%	0.009%
82	12.574	3585	3587	3590	rBV3	1321	952	0.12%	0.016%
83	12.590	3590	3592	3595	rBV4	1517	978	0.13%	0.017%
84	12.834	3666	3668	3674	rVB5	2258	1504	0.20%	0.026%
85	12.943	3695	3702	3707	rBV9	2640	3640	0.47%	0.062%
86	13.136	3758	3762	3764	rBV4	1832	1186	0.15%	0.020%
87	13.262	3799	3801	3803	rBV3	1481	540	0.07%	0.009%
88	13.294	3809	3811	3816	rBV4	1668	1271	0.17%	0.022%
89	13.329	3820	3822	3825	rBV4	1440	852	0.11%	0.015%
90	13.374	3833	3836	3838	rBV3	2314	1439	0.19%	0.025%
91	13.567	3894	3896	3897	rBV2	1332	536	0.07%	0.009%
92	13.738	3946	3949	3952	rVB5	2278	1507	0.20%	0.026%
93	13.754	3952	3954	3959	rBV6	783	632	0.08%	0.011%
94	13.834	3977	3979	3982	rBV4	1520	929	0.12%	0.016%
95	13.918	4002	4005	4007	rBV3	1556	980	0.13%	0.017%
96	14.152	4076	4078	4079	rBV2	1519	497	0.06%	0.009%
97	14.194	4089	4091	4095	rVB5	1615	825	0.11%	0.014%
98	14.387	4149	4151	4153	rBV3	1323	813	0.11%	0.014%
99	14.448	4166	4170	4172	rBV5	2235	1592	0.21%	0.027%
100	15.268	4421	4425	4428	rBV5	2278	1663	0.22%	0.029%




Sum of corrected areas: 5824798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031189.D
Acq On : 23 May 2023 14:56
Operator : SY/MD
Sample : 02861-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

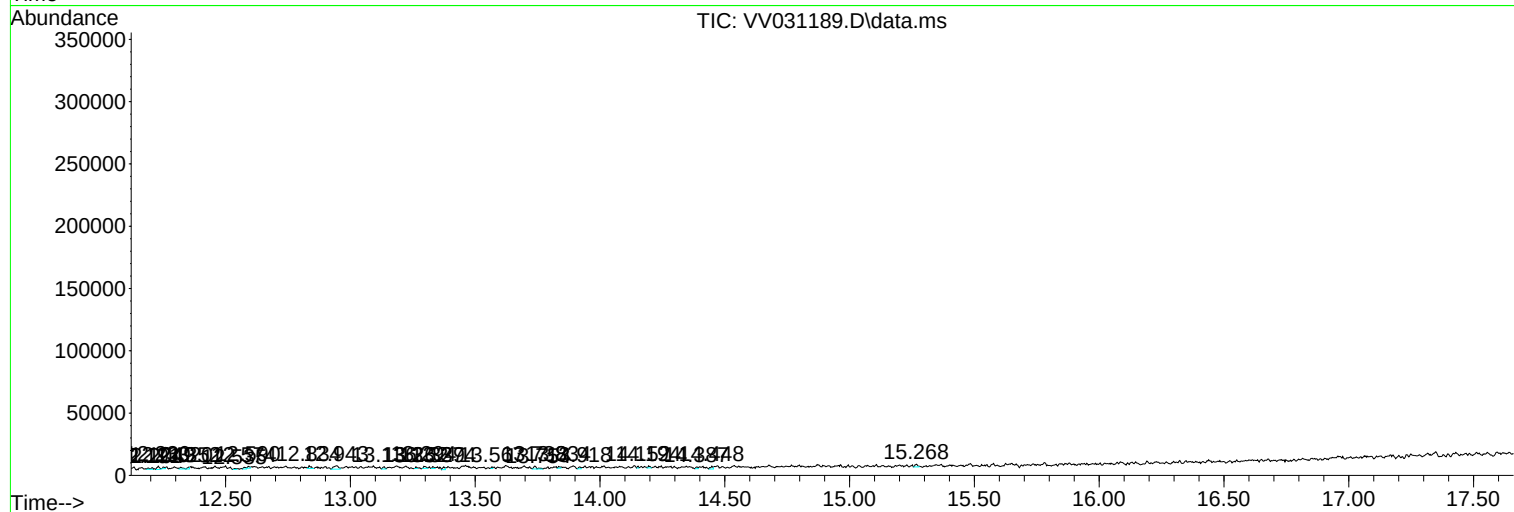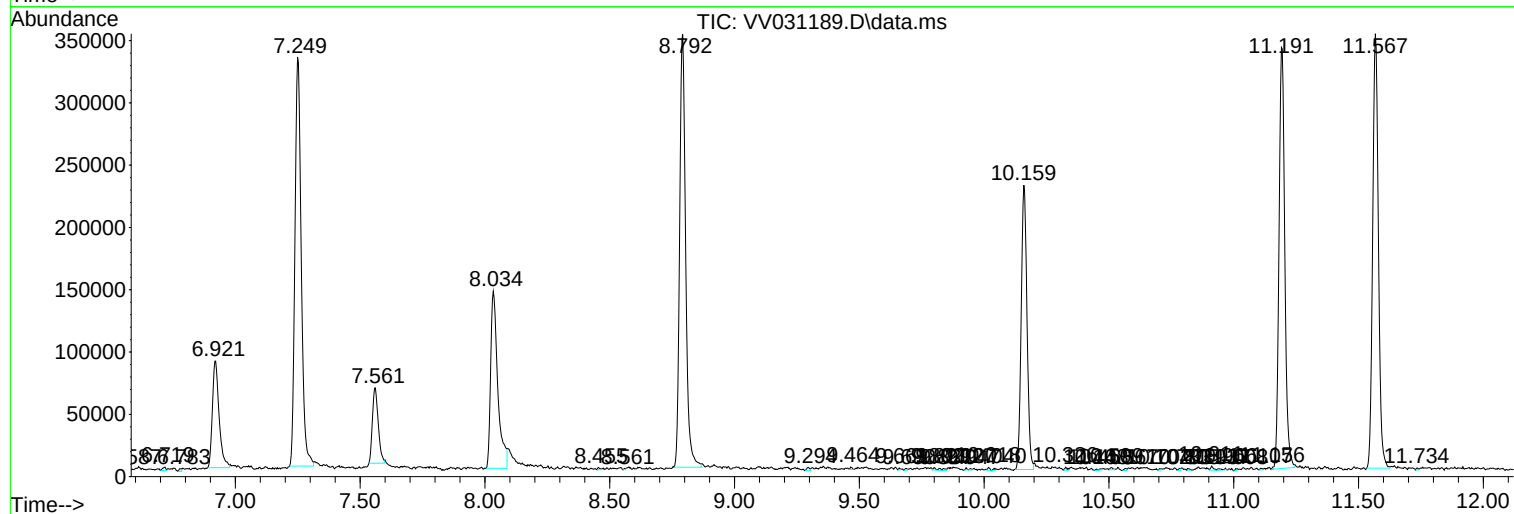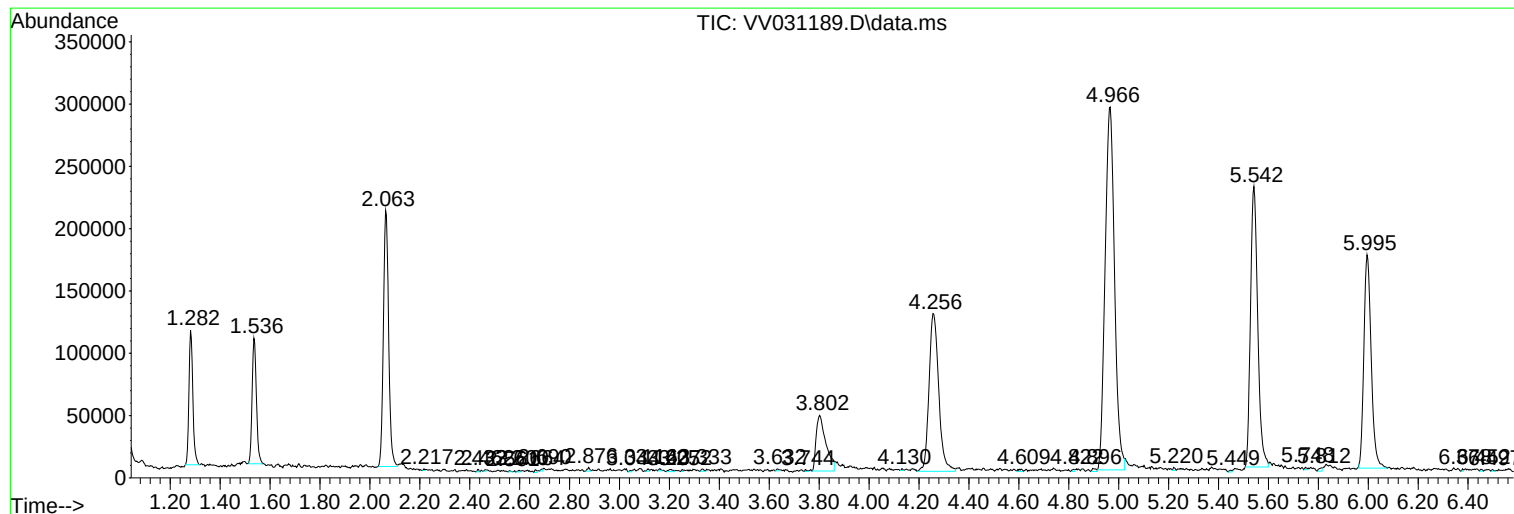

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031189.D
Acq On : 23 May 2023 14:56
Operator : SY/MD
Sample : 02861-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031189.D
Acq On : 23 May 2023 14:56
Operator : SY/MD
Sample : 02861-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------