

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031190.D
 Acq On : 23 May 2023 15:19
 Operator : SY/MD
 Sample : 02861-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	101465	109564	14.99%	1.971%
2	1.535	148	154	164	rVB	91552	108716	14.87%	1.956%
3	2.063	310	318	331	rVB	193835	284545	38.92%	5.119%
4	2.201	359	361	364	rBV4	1566	981	0.13%	0.018%
5	2.285	384	387	389	rBV4	1950	982	0.13%	0.018%
6	2.580	477	479	481	rBV2	2145	1070	0.15%	0.019%
7	2.905	578	580	587	rBV7	2115	2104	0.29%	0.038%
8	2.931	587	588	590	rBV2	1308	602	0.08%	0.011%
9	3.043	620	623	625	rBV4	2022	1516	0.21%	0.027%
10	3.323	709	710	713	rVB3	1728	603	0.08%	0.011%
11	3.416	736	739	744	rBV6	1983	2195	0.30%	0.039%
12	3.799	849	858	876	rBV	41604	110079	15.06%	1.980%
13	4.259	988	1001	1026	rVB	126664	319035	43.64%	5.739%
14	4.805	1167	1171	1173	rBV5	1895	1439	0.20%	0.026%
15	4.854	1184	1186	1189	rBV4	1603	1124	0.15%	0.020%
16	4.966	1206	1221	1245	rBV2	281885	731088	100.00%	13.151%
17	5.323	1330	1332	1334	rBV3	2305	1280	0.18%	0.023%
18	5.426	1362	1364	1365	rBV2	1858	659	0.09%	0.012%
19	5.542	1388	1400	1421	rBV	217141	444159	60.75%	7.990%
20	5.995	1531	1541	1559	rBV	163543	324735	44.42%	5.842%
21	6.571	1718	1720	1724	rBV4	2079	1241	0.17%	0.022%
22	6.722	1765	1767	1768	rBV2	1517	641	0.09%	0.012%
23	6.809	1789	1794	1797	rBV7	1834	1555	0.21%	0.028%
24	6.918	1819	1828	1842	rBV2	84914	157008	21.48%	2.824%
25	7.088	1879	1881	1885	rBV4	2035	929	0.13%	0.017%
26	7.249	1921	1931	1952	rBV	319969	562868	76.99%	10.125%
27	7.561	2019	2028	2047	rBV2	62837	118697	16.24%	2.135%
28	7.908	2134	2136	2141	rBV6	2159	1777	0.24%	0.032%
29	8.034	2166	2175	2211	rBV	135871	289728	39.63%	5.212%
30	8.693	2376	2380	2381	rBV4	1722	1236	0.17%	0.022%
31	8.792	2399	2411	2430	rVV	318669	536488	73.38%	9.651%
32	9.075	2497	2499	2502	rBV4	1278	767	0.10%	0.014%
33	9.091	2502	2504	2507	rBV4	1532	1074	0.15%	0.019%
34	9.172	2527	2529	2532	rBV4	1162	929	0.13%	0.017%
35	9.326	2575	2577	2580	rBV4	891	618	0.08%	0.011%
36	9.368	2588	2590	2592	rVB3	1566	734	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031190.D
 Acq On : 23 May 2023 15:19
 Operator : SY/MD
 Sample : 02861-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	9.381	2592	2594	2598	rBV5	1845	1581	0.22%	0.028%
38	9.599	2659	2662	2664	rBV4	2019	1401	0.19%	0.025%
39	9.628	2668	2671	2672	rBV3	1499	854	0.12%	0.015%
40	9.664	2680	2682	2684	rVB3	1705	711	0.10%	0.013%
41	9.699	2690	2693	2696	rBV5	1279	954	0.13%	0.017%
42	9.828	2731	2733	2736	rBV5	1482	710	0.10%	0.013%
43	10.159	2822	2836	2849	rBV	213305	346591	47.41%	6.235%
44	10.316	2883	2885	2887	rBV3	1490	751	0.10%	0.014%
45	10.374	2896	2903	2905	rBV7	1999	2108	0.29%	0.038%
46	10.429	2916	2920	2923	rBV6	1595	1385	0.19%	0.025%
47	10.535	2949	2953	2955	rVB5	1297	847	0.12%	0.015%
48	10.657	2990	2991	2994	rBV3	1104	677	0.09%	0.012%
49	10.673	2994	2996	2998	rVV3	1556	814	0.11%	0.015%
50	10.689	2998	3001	3003	rVB3	1343	683	0.09%	0.012%
51	10.751	3018	3020	3024	rVB5	1290	842	0.12%	0.015%
52	10.841	3045	3048	3049	rBV3	1793	883	0.12%	0.016%
53	10.898	3063	3066	3067	rBV3	1165	611	0.08%	0.011%
54	10.911	3067	3070	3074	rBV5	1171	1054	0.14%	0.019%
55	10.934	3074	3077	3079	rBV3	1137	822	0.11%	0.015%
56	11.021	3100	3104	3107	rBV6	1150	636	0.09%	0.011%
57	11.040	3107	3110	3111	rBV3	1410	682	0.09%	0.012%
58	11.088	3120	3125	3127	rBV7	1358	1229	0.17%	0.022%
59	11.191	3147	3157	3179	rVV	307182	501417	68.59%	9.020%
60	11.451	3235	3238	3240	rBV4	1231	800	0.11%	0.014%
61	11.474	3243	3245	3249	rVB4	1586	856	0.12%	0.015%
62	11.493	3249	3251	3254	rBV4	1440	843	0.12%	0.015%
63	11.567	3263	3274	3292	rBV	318264	524129	71.69%	9.428%
64	11.725	3321	3323	3326	rBV4	1579	821	0.11%	0.015%
65	11.796	3344	3345	3349	rVB4	2399	865	0.12%	0.016%
66	11.940	3389	3390	3396	rBV6	1372	1208	0.17%	0.022%
67	11.988	3403	3405	3408	rBV3	1204	614	0.08%	0.011%
68	12.181	3463	3465	3467	rBV3	1452	646	0.09%	0.012%
69	12.230	3476	3480	3484	rVB7	2100	1927	0.26%	0.035%
70	12.477	3553	3557	3560	rBV4	1236	917	0.13%	0.016%
71	12.554	3580	3581	3585	rVB3	1843	809	0.11%	0.015%
72	12.586	3585	3591	3592	rBV5	1562	1623	0.22%	0.029%
73	12.693	3621	3624	3628	rBV6	1924	1380	0.19%	0.025%
74	12.837	3667	3669	3670	rBV2	1270	609	0.08%	0.011%
75	12.895	3684	3687	3690	rBV5	2515	1685	0.23%	0.030%
76	12.959	3703	3707	3709	rBV5	1894	1536	0.21%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031190.D
 Acq On : 23 May 2023 15:19
 Operator : SY/MD
 Sample : 02861-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.992	3713	3717	3718	rBV4	1300	875	0.12%	0.016%
78	13.037	3729	3731	3733	rBV3	1999	1067	0.15%	0.019%
79	13.085	3744	3746	3748	rVV3	2010	916	0.13%	0.016%
80	13.133	3759	3761	3764	rVB4	1461	736	0.10%	0.013%
81	13.323	3818	3820	3822	rBV3	1540	781	0.11%	0.014%
82	13.448	3856	3859	3860	rBV3	1661	666	0.09%	0.012%
83	13.474	3864	3867	3868	rBV3	1195	704	0.10%	0.013%
84	13.628	3911	3915	3917	rBV4	2776	1933	0.26%	0.035%
85	13.680	3926	3931	3935	rVB6	2061	1660	0.23%	0.030%
86	13.699	3935	3937	3939	rBV2	2388	1067	0.15%	0.019%
87	13.744	3948	3951	3954	rBV5	1712	998	0.14%	0.018%
88	13.828	3973	3977	3981	rBV7	1918	1993	0.27%	0.036%
89	14.072	4050	4053	4056	rBV5	994	663	0.09%	0.012%
90	14.201	4091	4093	4095	rBV2	1122	591	0.08%	0.011%
91	14.310	4125	4127	4129	rVB3	1688	684	0.09%	0.012%
92	14.332	4129	4134	4136	rBV6	2045	2139	0.29%	0.038%
93	14.371	4144	4146	4150	rVB5	2031	1156	0.16%	0.021%
94	14.397	4150	4154	4155	rBV4	1562	1336	0.18%	0.024%
95	14.551	4199	4202	4205	rVB4	2973	2071	0.28%	0.037%
96	14.574	4205	4209	4210	rBV4	965	693	0.09%	0.012%
97	14.654	4232	4234	4237	rBV4	1753	1195	0.16%	0.021%
98	14.783	4271	4274	4275	rBV3	1230	725	0.10%	0.013%
99	15.262	4422	4423	4427	rBV4	1356	865	0.12%	0.016%
100	15.326	4441	4443	4445	rBV3	1931	1215	0.17%	0.022%




Sum of corrected areas: 5559006

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031190.D
Acq On : 23 May 2023 15:19
Operator : SY/MD
Sample : 02861-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

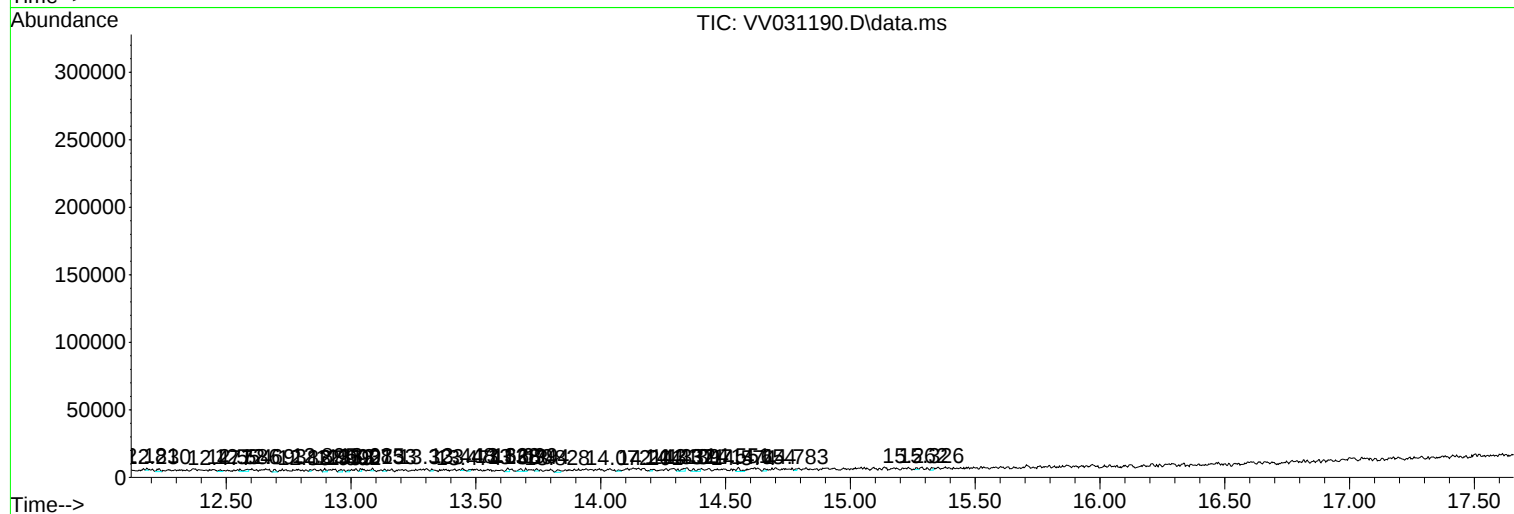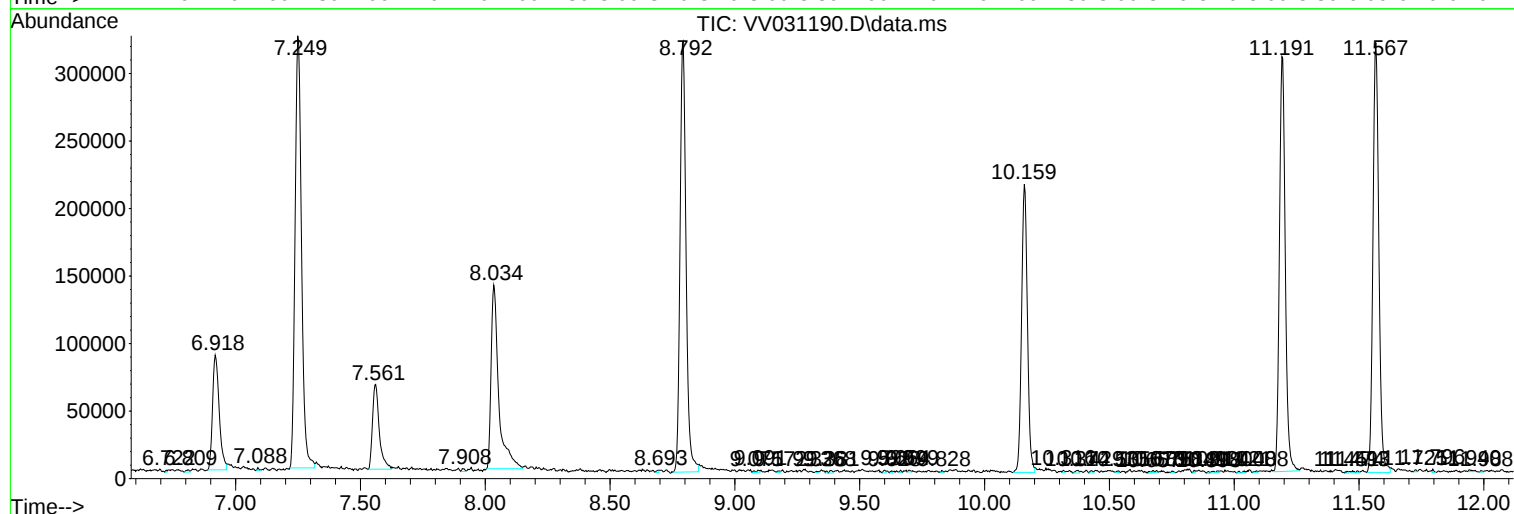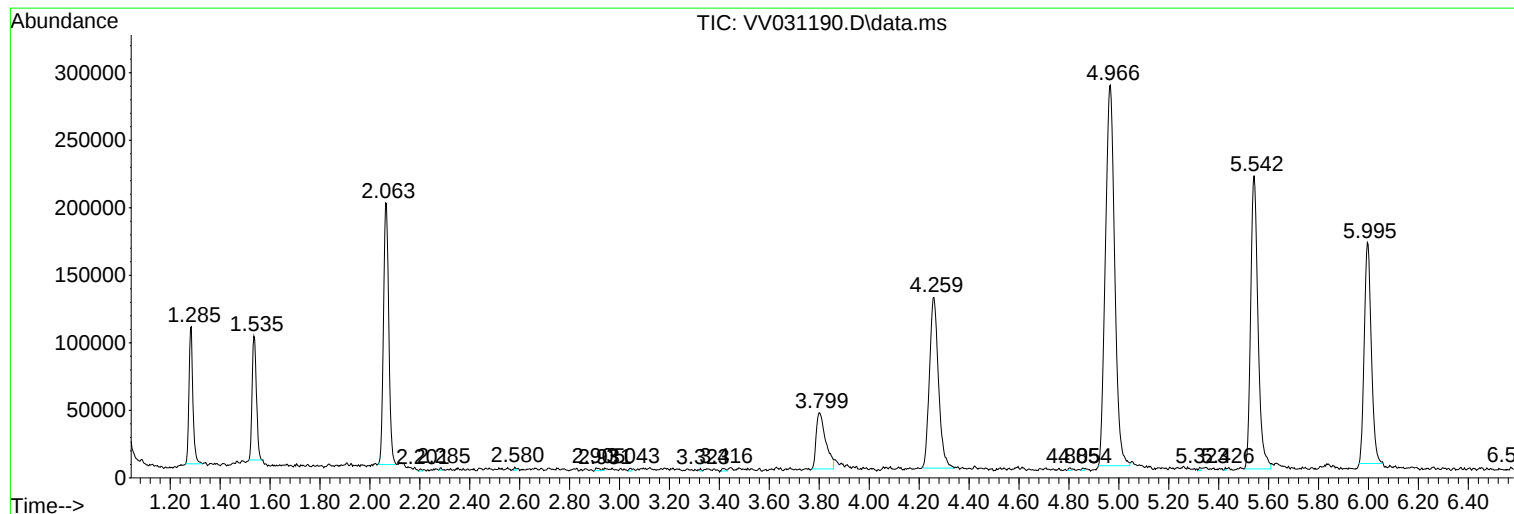

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031190.D
Acq On : 23 May 2023 15:19
Operator : SY/MD
Sample : 02861-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031190.D
Acq On : 23 May 2023 15:19
Operator : SY/MD
Sample : 02861-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------