

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031191.D
 Acq On : 23 May 2023 15:42
 Operator : SY/MD
 Sample : 02861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	84	rBV	104420	111575	14.64%	1.928%
2	1.535	148	154	168	rVB	107170	126302	16.57%	2.183%
3	2.063	310	318	333	rVB	203537	295114	38.72%	5.101%
4	2.407	422	425	427	rBV4	1987	1081	0.14%	0.019%
5	2.658	501	503	504	rBV2	2526	1187	0.16%	0.021%
6	2.703	515	517	519	rVB3	1644	543	0.07%	0.009%
7	2.748	530	531	535	rBV3	1543	973	0.13%	0.017%
8	3.024	615	617	620	rBV4	2490	1209	0.16%	0.021%
9	3.236	680	683	685	rBV4	1211	637	0.08%	0.011%
10	3.249	685	687	689	rBV3	1202	526	0.07%	0.009%
11	3.288	697	699	705	rVB5	2284	2155	0.28%	0.037%
12	3.314	705	707	709	rBV3	1979	1307	0.17%	0.023%
13	3.494	760	763	764	rBV3	1780	985	0.13%	0.017%
14	3.600	793	796	797	rBV3	2031	1322	0.17%	0.023%
15	3.645	808	810	813	rVB4	1864	871	0.11%	0.015%
16	3.664	813	816	818	rBV4	2110	1286	0.17%	0.022%
17	3.744	837	841	845	rBV6	2200	2164	0.28%	0.037%
18	3.802	850	859	882	rVV2	43883	122115	16.02%	2.111%
19	4.191	976	980	981	rBV4	1188	792	0.10%	0.014%
20	4.259	990	1001	1020	rVB	127534	305106	40.03%	5.273%
21	4.375	1035	1037	1040	rVB4	2398	1122	0.15%	0.019%
22	4.706	1136	1140	1142	rBV4	1285	877	0.12%	0.015%
23	4.735	1147	1149	1151	rBV3	1833	766	0.10%	0.013%
24	4.789	1164	1166	1168	rVB3	1571	663	0.09%	0.011%
25	4.805	1168	1171	1173	rBV4	2297	1394	0.18%	0.024%
26	4.857	1183	1187	1191	rBV6	1262	1411	0.19%	0.024%
27	4.966	1205	1221	1240	rBV3	288104	762183	100.00%	13.173%
28	5.432	1363	1366	1367	rBV3	1142	581	0.08%	0.010%
29	5.542	1389	1400	1423	rBV	213341	448965	58.91%	7.760%
30	5.995	1531	1541	1562	rVB	168183	344024	45.14%	5.946%
31	6.297	1633	1635	1639	rVB4	1738	1112	0.15%	0.019%
32	6.336	1645	1647	1649	rBV3	1644	511	0.07%	0.009%
33	6.670	1748	1751	1752	rBV3	2087	1013	0.13%	0.018%
34	6.809	1791	1794	1795	rBV3	1624	797	0.10%	0.014%
35	6.921	1818	1829	1844	rBV	86477	163216	21.41%	2.821%
36	7.249	1920	1931	1949	rBV	325424	575467	75.50%	9.946%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031191.D
 Acq On : 23 May 2023 15:42
 Operator : SY/MD
 Sample : 02861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.497	2004	2008	2013	rBV7	1396	1492	0.20%	0.026%
38	7.561	2017	2028	2047	rBV2	62297	121193	15.90%	2.095%
39	7.989	2158	2161	2163	rVB4	2289	1210	0.16%	0.021%
40	8.034	2165	2175	2192	rBV	141162	286307	37.56%	4.948%
41	8.645	2364	2365	2366	rBV	1425	433	0.06%	0.007%
42	8.792	2399	2411	2428	rBV	343035	568766	74.62%	9.830%
43	9.063	2491	2495	2499	rBV7	1366	1392	0.18%	0.024%
44	9.120	2511	2513	2515	rBV3	1068	446	0.06%	0.008%
45	9.194	2534	2536	2539	rBV4	1355	782	0.10%	0.014%
46	9.307	2569	2571	2574	rBV4	1857	939	0.12%	0.016%
47	9.426	2606	2608	2609	rBV2	1388	625	0.08%	0.011%
48	9.477	2621	2624	2626	rBV4	2657	1642	0.22%	0.028%
49	9.516	2632	2636	2639	rBV6	1805	1750	0.23%	0.030%
50	9.635	2671	2673	2676	rBV4	1645	833	0.11%	0.014%
51	9.728	2700	2702	2703	rBV2	1098	506	0.07%	0.009%
52	9.747	2706	2708	2710	rBV4	1714	764	0.10%	0.013%
53	10.034	2795	2797	2798	rBV2	1762	810	0.11%	0.014%
54	10.095	2814	2816	2819	rVB4	1997	1016	0.13%	0.018%
55	10.159	2825	2836	2852	rBV	228966	360354	47.28%	6.228%
56	10.387	2904	2907	2912	rVB6	2634	2784	0.37%	0.048%
57	10.413	2912	2915	2918	rBV5	2140	1657	0.22%	0.029%
58	10.558	2957	2960	2964	rBV6	1657	1312	0.17%	0.023%
59	10.641	2983	2986	2990	rBV6	1912	1410	0.18%	0.024%
60	10.664	2990	2993	2994	rBV3	1191	776	0.10%	0.013%
61	10.696	3001	3003	3004	rBV2	1186	504	0.07%	0.009%
62	10.818	3039	3041	3044	rBV3	1037	680	0.09%	0.012%
63	10.937	3074	3078	3081	rBV5	1667	1531	0.20%	0.026%
64	10.985	3091	3093	3094	rVB2	1656	457	0.06%	0.008%
65	11.075	3119	3121	3123	rBV3	1074	574	0.08%	0.010%
66	11.191	3145	3157	3179	rBV	334004	544394	71.43%	9.409%
67	11.458	3237	3240	3242	rBV4	1273	847	0.11%	0.015%
68	11.522	3257	3260	3262	rVB4	1282	726	0.10%	0.013%
69	11.567	3262	3274	3290	rBV	348655	558301	73.25%	9.649%
70	11.959	3392	3396	3397	rBV3	1621	1183	0.16%	0.020%
71	12.021	3411	3415	3416	rBV4	1113	739	0.10%	0.013%
72	12.220	3474	3477	3480	rVB5	1578	1006	0.13%	0.017%
73	12.236	3480	3482	3484	rBV3	1831	1128	0.15%	0.019%
74	12.422	3537	3540	3541	rBV3	1272	593	0.08%	0.010%
75	12.503	3562	3565	3567	rBV5	2394	1605	0.21%	0.028%
76	12.538	3574	3576	3577	rBV2	1183	623	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031191.D
 Acq On : 23 May 2023 15:42
 Operator : SY/MD
 Sample : 02861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.628	3598	3604	3608	rBV9	2934	3487	0.46%	0.060%
78	12.686	3620	3622	3625	rBV3	1957	1032	0.14%	0.018%
79	12.840	3666	3670	3677	rVB9	1988	2172	0.28%	0.038%
80	12.876	3677	3681	3682	rBV4	1414	923	0.12%	0.016%
81	12.950	3700	3704	3707	rVV5	1973	1503	0.20%	0.026%
82	13.017	3721	3725	3729	rBV6	1471	1473	0.19%	0.025%
83	13.037	3729	3731	3734	rBV3	1255	521	0.07%	0.009%
84	13.085	3743	3746	3748	rBV4	1722	1293	0.17%	0.022%
85	13.246	3794	3796	3801	rVB5	1445	785	0.10%	0.014%
86	13.509	3877	3878	3879	rBV	1345	500	0.07%	0.009%
87	13.551	3889	3891	3893	rBV3	1858	898	0.12%	0.016%
88	13.564	3893	3895	3897	rVB3	1410	581	0.08%	0.010%
89	13.612	3909	3910	3913	rBV3	1744	649	0.09%	0.011%
90	13.696	3930	3936	3937	rBV6	3362	3500	0.46%	0.060%
91	13.908	4000	4002	4005	rBV4	1343	708	0.09%	0.012%
92	13.924	4005	4007	4011	rBV5	2262	1878	0.25%	0.032%
93	14.165	4080	4082	4083	rBV2	1321	505	0.07%	0.009%
94	14.342	4135	4137	4140	rBV4	2284	1372	0.18%	0.024%
95	14.397	4152	4154	4155	rBV2	2048	729	0.10%	0.013%
96	14.490	4181	4183	4184	rBV2	1627	521	0.07%	0.009%
97	14.519	4189	4192	4197	rBV6	2507	1674	0.22%	0.029%
98	14.564	4203	4206	4208	rBV4	1510	1141	0.15%	0.020%
99	14.837	4289	4291	4294	rBV4	2638	1836	0.24%	0.032%
100	15.175	4394	4396	4397	rBV2	2035	704	0.09%	0.012%




Sum of corrected areas: 5785827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031191.D
Acq On : 23 May 2023 15:42
Operator : SY/MD
Sample : 02861-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

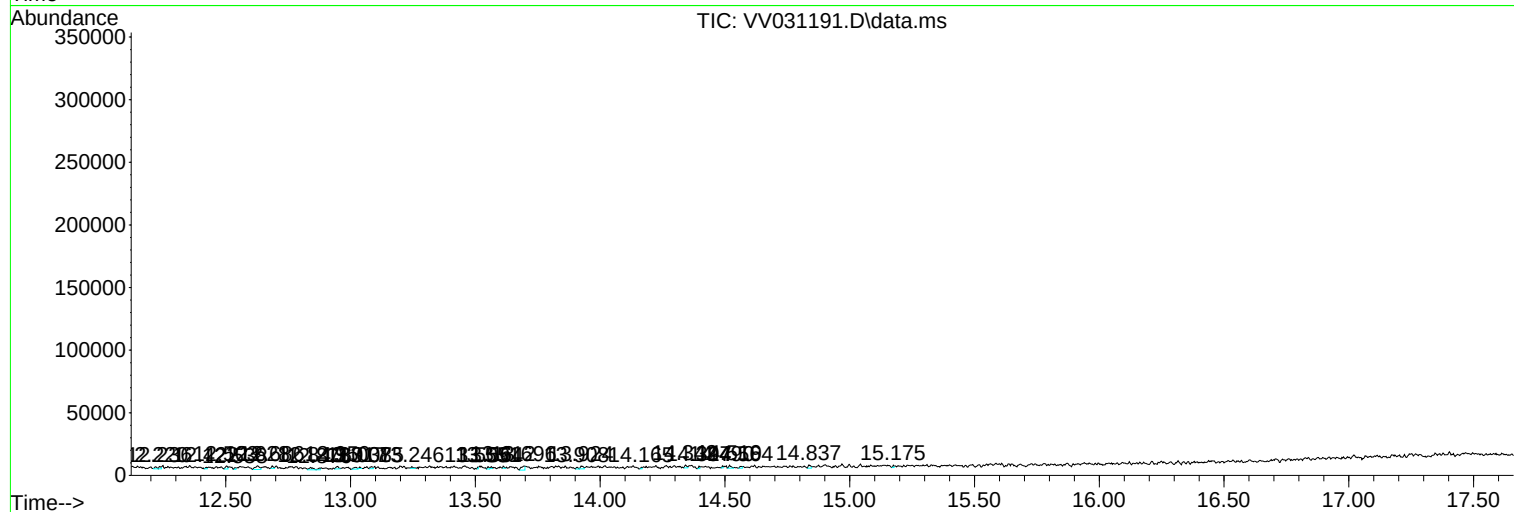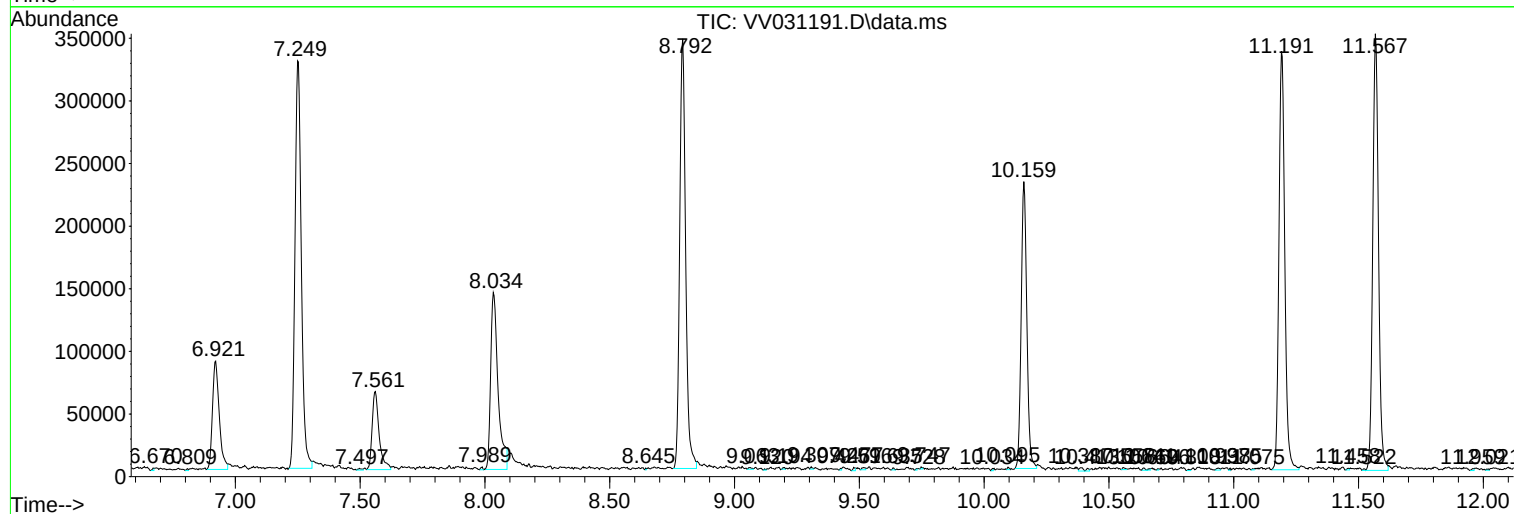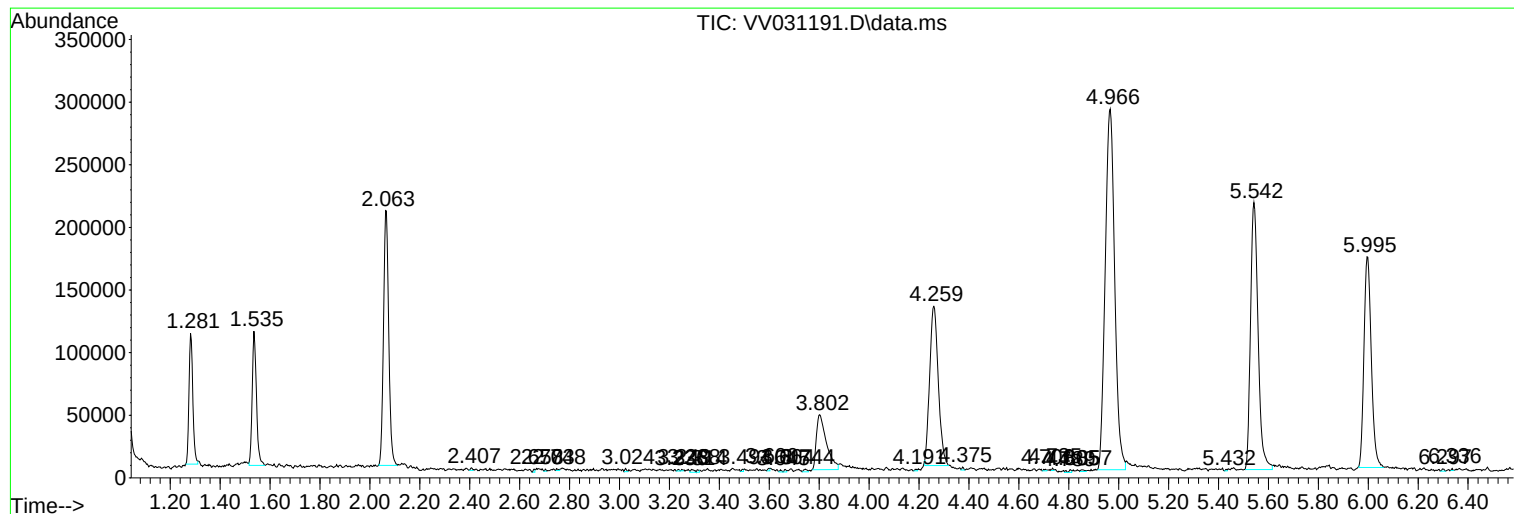

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031191.D
Acq On : 23 May 2023 15:42
Operator : SY/MD
Sample : 02861-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031191.D
Acq On : 23 May 2023 15:42
Operator : SY/MD
Sample : 02861-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc