

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031192.D
 Acq On : 23 May 2023 16:06
 Operator : SY/MD
 Sample : 02861-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	87	rBV	106738	115331	14.68%	1.939%
2	1.535	148	154	167	rVB	109579	130200	16.57%	2.189%
3	2.066	310	319	329	rBV	204383	293619	37.38%	4.936%
4	2.233	369	371	373	rBV3	1725	700	0.09%	0.012%
5	2.275	383	384	389	rVB5	1322	756	0.10%	0.013%
6	2.304	389	393	396	rBV5	2441	1940	0.25%	0.033%
7	2.378	414	416	418	rVB2	1595	577	0.07%	0.010%
8	2.391	418	420	422	rVB3	978	503	0.06%	0.008%
9	2.404	422	424	427	rBV5	1437	922	0.12%	0.015%
10	2.449	432	438	441	rBV7	2495	2699	0.34%	0.045%
11	2.799	545	547	549	rBV3	1392	882	0.11%	0.015%
12	2.854	561	564	567	rBV5	1602	1336	0.17%	0.022%
13	2.989	604	606	608	rBV3	1975	870	0.11%	0.015%
14	3.021	613	616	617	rBV3	2046	882	0.11%	0.015%
15	3.066	628	630	632	rBV3	1180	306	0.04%	0.005%
16	3.117	643	646	649	rBV5	1952	1591	0.20%	0.027%
17	3.239	682	684	685	rBV2	753	193	0.02%	0.003%
18	3.400	731	734	738	rBV6	2030	1501	0.19%	0.025%
19	3.799	850	858	880	rBV	47180	129870	16.53%	2.183%
20	4.256	986	1000	1021	rBV	132106	340261	43.31%	5.720%
21	4.625	1113	1115	1117	rBV3	1667	789	0.10%	0.013%
22	4.677	1129	1131	1133	rVB3	1364	489	0.06%	0.008%
23	4.741	1149	1151	1155	rBV5	1344	807	0.10%	0.014%
24	4.905	1198	1202	1204	rBV5	2877	2315	0.29%	0.039%
25	4.963	1205	1220	1240	rVV2	298523	785584	100.00%	13.206%
26	5.268	1313	1315	1316	rBV2	1345	395	0.05%	0.007%
27	5.542	1388	1400	1419	rBV	218696	449984	57.28%	7.565%
28	5.995	1530	1541	1562	rVB2	175004	358069	45.58%	6.019%
29	6.403	1666	1668	1671	rBV4	1332	598	0.08%	0.010%
30	6.532	1705	1708	1709	rBV3	1534	846	0.11%	0.014%
31	6.564	1714	1718	1719	rBV4	2144	1702	0.22%	0.029%
32	6.683	1753	1755	1760	rBV6	2020	1819	0.23%	0.031%
33	6.847	1803	1806	1807	rBV3	1895	990	0.13%	0.017%
34	6.870	1811	1813	1814	rBV2	994	327	0.04%	0.005%
35	6.921	1819	1829	1844	rBV	88717	163177	20.77%	2.743%
36	7.249	1920	1931	1952	rBV	337609	601563	76.58%	10.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031192.D
 Acq On : 23 May 2023 16:06
 Operator : SY/MD
 Sample : 02861-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.558	2020	2027	2046	rVB	63012	110552	14.07%	1.858%
38	7.689	2066	2068	2072	rVB5	2418	1348	0.17%	0.023%
39	7.898	2131	2133	2134	rBV2	1354	531	0.07%	0.009%
40	7.960	2150	2152	2153	rBV2	1834	651	0.08%	0.011%
41	8.034	2166	2175	2205	rBV	149599	319255	40.64%	5.367%
42	8.397	2286	2288	2290	rBV3	1794	755	0.10%	0.013%
43	8.702	2381	2383	2388	rBV5	1611	1070	0.14%	0.018%
44	8.792	2400	2411	2429	rBV	345008	572063	72.82%	9.617%
45	9.226	2543	2546	2548	rBV4	2253	1298	0.17%	0.022%
46	9.304	2567	2570	2573	rBV5	1186	782	0.10%	0.013%
47	9.445	2613	2614	2618	rVB3	2147	1273	0.16%	0.021%
48	9.474	2619	2623	2624	rBV4	1787	1126	0.14%	0.019%
49	9.509	2632	2634	2635	rBV3	1988	1017	0.13%	0.017%
50	9.619	2665	2668	2669	rBV3	1315	796	0.10%	0.013%
51	9.664	2680	2682	2688	rBV6	1582	1421	0.18%	0.024%
52	9.718	2693	2699	2702	rBV8	2370	2760	0.35%	0.046%
53	9.789	2720	2721	2723	rVB2	1806	583	0.07%	0.010%
54	9.924	2761	2763	2765	rBV3	1416	569	0.07%	0.010%
55	9.969	2775	2777	2782	rVB5	1941	963	0.12%	0.016%
56	10.027	2793	2795	2797	rBV3	895	340	0.04%	0.006%
57	10.111	2819	2821	2823	rBV3	1696	814	0.10%	0.014%
58	10.159	2825	2836	2852	rVV	240150	383799	48.86%	6.452%
59	10.265	2867	2869	2872	rBV4	1245	391	0.05%	0.007%
60	10.509	2943	2945	2946	rBV2	1002	320	0.04%	0.005%
61	10.631	2976	2983	2984	rBV6	2407	2362	0.30%	0.040%
62	10.676	2994	2997	3002	rVB6	1819	1711	0.22%	0.029%
63	10.699	3002	3004	3005	rBV2	1278	466	0.06%	0.008%
64	10.779	3027	3029	3030	rBV2	1397	482	0.06%	0.008%
65	10.812	3037	3039	3041	rBV3	1647	901	0.11%	0.015%
66	10.853	3046	3052	3054	rBV7	1723	1773	0.23%	0.030%
67	10.869	3054	3057	3058	rBV3	1228	735	0.09%	0.012%
68	11.040	3108	3110	3112	rBV3	1166	672	0.09%	0.011%
69	11.066	3116	3118	3121	rBV3	1299	1050	0.13%	0.018%
70	11.107	3129	3131	3132	rBV2	1065	324	0.04%	0.005%
71	11.191	3147	3157	3173	rBV	334685	536244	68.26%	9.015%
72	11.439	3231	3234	3240	rBV7	2935	2468	0.31%	0.041%
73	11.567	3263	3274	3290	rBV	356072	568734	72.40%	9.561%
74	11.927	3382	3386	3387	rBV4	1219	792	0.10%	0.013%
75	12.094	3436	3438	3441	rBV4	2066	1055	0.13%	0.018%
76	12.146	3451	3454	3455	rBV3	1650	963	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031192.D
 Acq On : 23 May 2023 16:06
 Operator : SY/MD
 Sample : 02861-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.188	3466	3467	3471	rBV4	1376	893	0.11%	0.015%
78	12.204	3471	3472	3475	rVV3	1166	565	0.07%	0.009%
79	12.348	3514	3517	3518	rBV3	1605	919	0.12%	0.015%
80	12.400	3532	3533	3535	rBV2	1068	390	0.05%	0.007%
81	12.532	3572	3574	3576	rBV3	1564	644	0.08%	0.011%
82	12.557	3579	3582	3584	rVB4	2131	1038	0.13%	0.017%
83	12.596	3591	3594	3596	rBV4	1830	1047	0.13%	0.018%
84	12.644	3606	3609	3611	rBV4	2101	1194	0.15%	0.020%
85	12.776	3646	3650	3654	rBV6	2214	2571	0.33%	0.043%
86	12.844	3668	3671	3673	rBV4	2462	1501	0.19%	0.025%
87	12.982	3711	3714	3718	rBV5	1388	1530	0.19%	0.026%
88	13.114	3753	3755	3758	rVB4	2024	924	0.12%	0.016%
89	13.136	3758	3762	3764	rBV5	1434	1118	0.14%	0.019%
90	13.172	3770	3773	3776	rBV5	3374	2443	0.31%	0.041%
91	13.307	3813	3815	3817	rBV3	1410	512	0.07%	0.009%
92	13.451	3857	3860	3864	rBV6	1757	1253	0.16%	0.021%
93	13.567	3893	3896	3899	rBV4	1720	1424	0.18%	0.024%
94	13.654	3921	3923	3925	rBV3	2076	1085	0.14%	0.018%
95	13.776	3958	3961	3963	rBV4	1331	814	0.10%	0.014%
96	13.789	3963	3965	3967	rBV3	2037	1098	0.14%	0.018%
97	13.937	4007	4011	4015	rBV6	2219	2608	0.33%	0.044%
98	14.049	4043	4046	4047	rBV3	1494	940	0.12%	0.016%
99	14.117	4065	4067	4068	rBV2	1291	611	0.08%	0.010%
100	14.191	4085	4090	4092	rBV6	1951	1781	0.23%	0.030%




Sum of corrected areas: 5948505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031192.D
Acq On : 23 May 2023 16:06
Operator : SY/MD
Sample : 02861-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

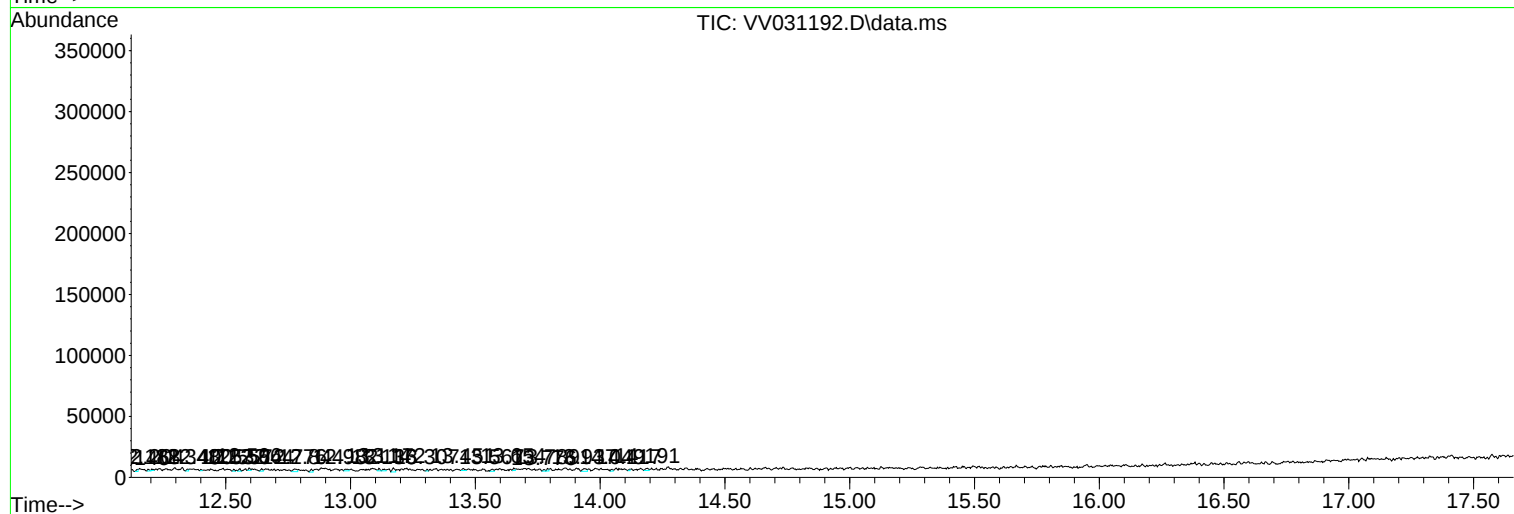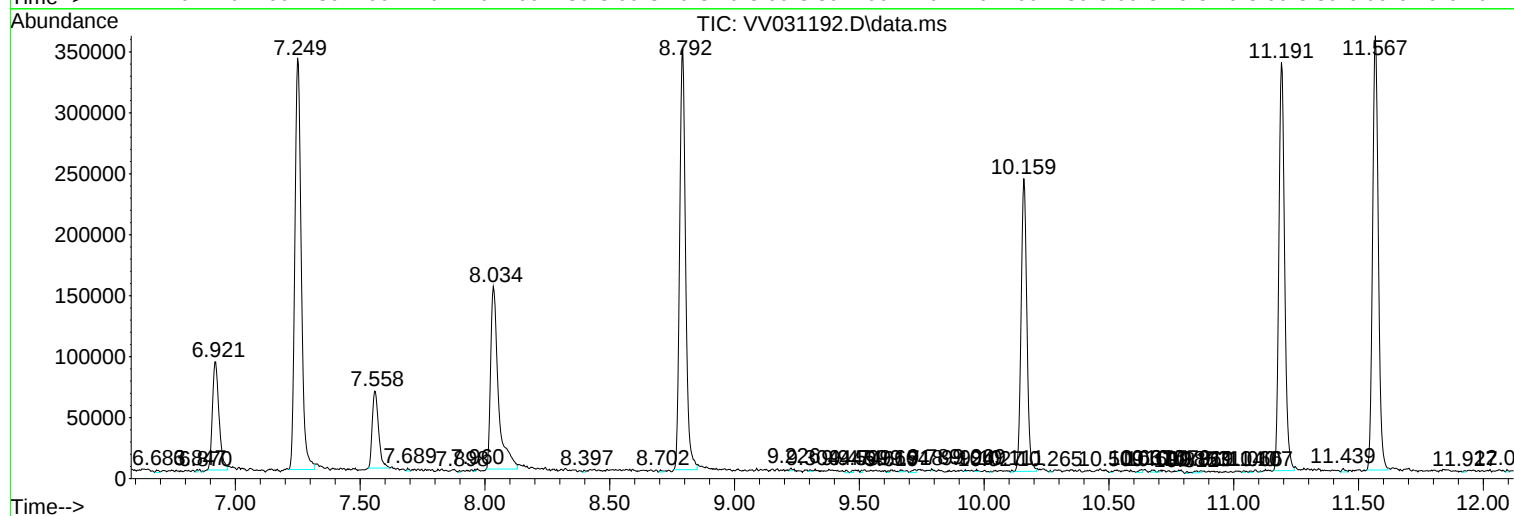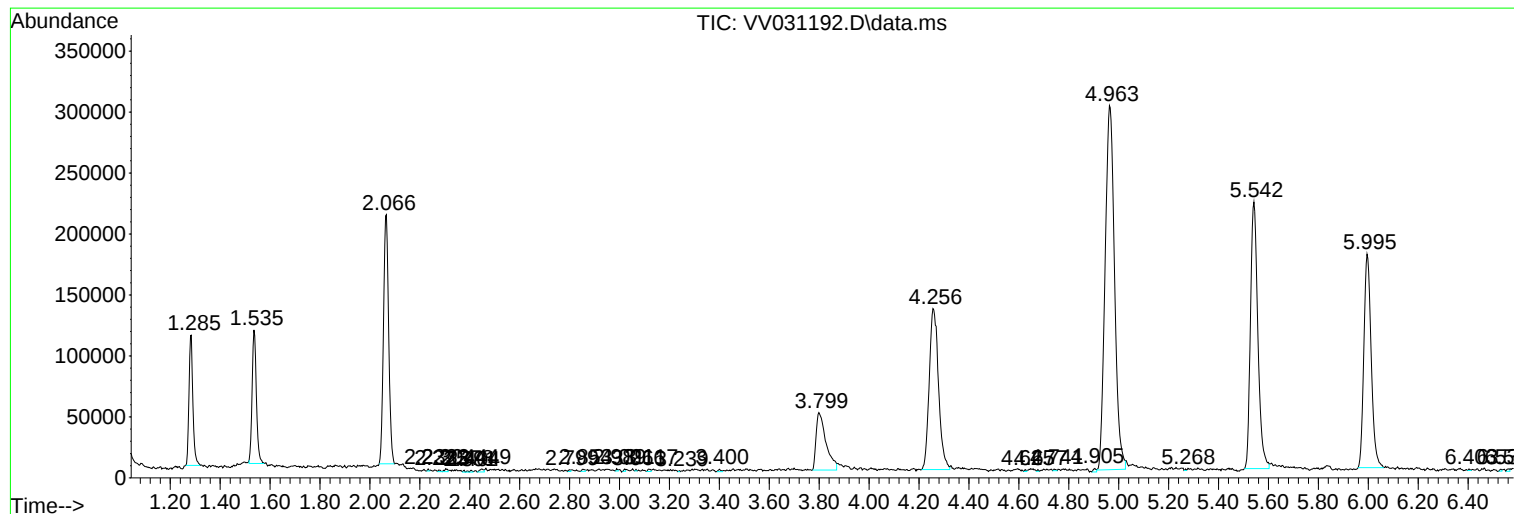

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031192.D
Acq On : 23 May 2023 16:06
Operator : SY/MD
Sample : 02861-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031192.D
Acq On : 23 May 2023 16:06
Operator : SY/MD
Sample : 02861-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------