

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031195.D
 Acq On : 23 May 2023 17:14
 Operator : SY/MD
 Sample : 02865-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	103484	117690	16.09%	1.945%
2	1.536	148	154	167	rVB	95717	117688	16.09%	1.945%
3	2.063	310	318	332	rVB	192847	281158	38.45%	4.646%
4	2.442	434	436	438	rBV3	1776	972	0.13%	0.016%
5	2.529	462	463	465	rBV2	1538	603	0.08%	0.010%
6	2.587	479	481	484	rBV4	2237	1031	0.14%	0.017%
7	2.683	504	511	513	rBV6	3692	2937	0.40%	0.049%
8	2.822	552	554	556	rBV3	1915	816	0.11%	0.013%
9	2.957	594	596	598	rBV3	1655	914	0.12%	0.015%
10	3.423	737	741	742	rBV4	1718	1229	0.17%	0.020%
11	3.516	768	770	771	rBV2	1174	489	0.07%	0.008%
12	3.529	771	774	776	rVV4	2709	1633	0.22%	0.027%
13	3.626	802	804	806	rBV3	1177	648	0.09%	0.011%
14	3.658	812	814	821	rVB6	3086	2698	0.37%	0.045%
15	3.703	821	828	830	rBV7	1721	2491	0.34%	0.041%
16	3.799	847	858	883	rBV2	54222	170879	23.37%	2.824%
17	4.024	926	928	930	rVB3	1820	618	0.08%	0.010%
18	4.095	948	950	952	rBV3	1964	797	0.11%	0.013%
19	4.114	955	956	960	rBV4	680	371	0.05%	0.006%
20	4.143	960	965	968	rBV7	1512	1557	0.21%	0.026%
21	4.172	972	974	976	rBV3	2167	857	0.12%	0.014%
22	4.188	976	979	981	rBV4	1023	620	0.08%	0.010%
23	4.259	988	1001	1021	rBV	117793	293949	40.20%	4.858%
24	4.391	1040	1042	1043	rBV2	1729	646	0.09%	0.011%
25	4.436	1054	1056	1059	rBV4	1897	1107	0.15%	0.018%
26	4.584	1099	1102	1106	rBV6	1591	1209	0.17%	0.020%
27	4.613	1109	1111	1114	rBV3	1200	572	0.08%	0.009%
28	4.699	1137	1138	1141	rBV3	1709	662	0.09%	0.011%
29	4.716	1141	1143	1144	rBV2	1383	576	0.08%	0.010%
30	4.725	1144	1146	1147	rVV2	1422	506	0.07%	0.008%
31	4.738	1149	1150	1154	rVV4	829	485	0.07%	0.008%
32	4.786	1163	1165	1168	rVB3	1024	559	0.08%	0.009%
33	4.806	1168	1171	1172	rBV3	1675	959	0.13%	0.016%
34	4.844	1181	1183	1184	rBV3	851	274	0.04%	0.005%
35	4.867	1188	1190	1191	rBV3	1092	529	0.07%	0.009%
36	4.896	1197	1199	1202	rBV4	1056	620	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031195.D
 Acq On : 23 May 2023 17:14
 Operator : SY/MD
 Sample : 02865-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.966	1203	1221	1249	rVV3	271503	731280	100.00%	12.085%
38	5.326	1331	1333	1334	rBV2	1967	944	0.13%	0.016%
39	5.359	1341	1343	1346	rBV4	1678	844	0.12%	0.014%
40	5.391	1351	1353	1357	rVB5	1969	1468	0.20%	0.024%
41	5.416	1359	1361	1362	rBV2	1217	552	0.08%	0.009%
42	5.474	1375	1379	1385	rVB9	2683	2874	0.39%	0.047%
43	5.542	1385	1400	1425	rBV	199226	423488	57.91%	6.998%
44	5.716	1452	1454	1458	rBV5	1787	1449	0.20%	0.024%
45	5.841	1482	1493	1514	rBV	146666	293627	40.15%	4.852%
46	5.995	1530	1541	1561	rBV	159872	327466	44.78%	5.412%
47	6.246	1617	1619	1622	rVB4	2704	1210	0.17%	0.020%
48	6.259	1622	1623	1625	rBV2	1230	672	0.09%	0.011%
49	6.275	1626	1628	1631	rVV4	1489	1012	0.14%	0.017%
50	6.365	1654	1656	1660	rVB5	1990	1216	0.17%	0.020%
51	6.526	1705	1706	1709	rVB3	1567	631	0.09%	0.010%
52	6.555	1713	1715	1716	rBV2	1305	498	0.07%	0.008%
53	6.638	1737	1741	1744	rBV6	1352	1418	0.19%	0.023%
54	6.680	1751	1754	1757	rBV5	1907	1226	0.17%	0.020%
55	6.921	1818	1829	1843	rBV	84158	161660	22.11%	2.672%
56	7.249	1920	1931	1949	rBV	320628	569545	77.88%	9.412%
57	7.561	2020	2028	2042	rBV	61552	106602	14.58%	1.762%
58	7.969	2152	2155	2156	rBV3	1617	681	0.09%	0.011%
59	8.034	2166	2175	2188	rBV	180799	339044	46.36%	5.603%
60	8.304	2257	2259	2261	rVB3	2061	654	0.09%	0.011%
61	8.793	2401	2411	2433	rVB	322877	527797	72.17%	8.722%
62	9.384	2592	2595	2596	rBV3	1278	658	0.09%	0.011%
63	9.793	2720	2722	2728	rBV7	1843	1564	0.21%	0.026%
64	10.082	2808	2812	2815	rBV5	2388	1955	0.27%	0.032%
65	10.159	2825	2836	2850	rBV	243311	378998	51.83%	6.263%
66	10.619	2974	2979	2981	rBV5	3707	2890	0.40%	0.048%
67	10.690	2999	3001	3004	rBV4	2221	1331	0.18%	0.022%
68	10.834	3043	3046	3049	rBV5	1833	1127	0.15%	0.019%
69	10.850	3049	3051	3052	rBV2	1389	520	0.07%	0.009%
70	10.892	3062	3064	3068	rBV5	1590	1416	0.19%	0.023%
71	10.911	3068	3070	3073	rVB4	2254	1059	0.14%	0.018%
72	10.928	3073	3075	3076	rBV2	1755	617	0.08%	0.010%
73	10.953	3082	3083	3084	rBV	1527	505	0.07%	0.008%
74	11.191	3145	3157	3177	rBV	313578	505762	69.16%	8.358%
75	11.493	3243	3251	3261	rBV3	35938	65849	9.00%	1.088%
76	11.567	3265	3274	3293	rVB	360903	566365	77.45%	9.360%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031195.D
 Acq On : 23 May 2023 17:14
 Operator : SY/MD
 Sample : 02865-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	11.860	3363	3365	3367	rBV3	1411	541	0.07%	0.009%
78	11.931	3385	3387	3390	rBV4	1678	825	0.11%	0.014%
79	12.522	3569	3571	3574	rBV4	1692	640	0.09%	0.011%
80	12.657	3611	3613	3614	rBV2	1169	415	0.06%	0.007%
81	12.667	3614	3616	3618	rVV3	1456	686	0.09%	0.011%
82	12.767	3645	3647	3650	rBV4	1527	889	0.12%	0.015%
83	13.172	3772	3773	3775	rVB2	1981	561	0.08%	0.009%
84	13.185	3775	3777	3778	rBV2	2138	861	0.12%	0.014%
85	13.342	3825	3826	3827	rBV	1165	340	0.05%	0.006%
86	13.783	3961	3963	3964	rBV2	1107	339	0.05%	0.006%
87	13.799	3967	3968	3970	rVV2	1687	582	0.08%	0.010%
88	13.853	3983	3985	3988	rBV3	1603	685	0.09%	0.011%
89	13.985	4025	4026	4027	rBV	1288	287	0.04%	0.005%
90	14.297	4121	4123	4124	rBV2	1782	719	0.10%	0.012%
91	14.963	4329	4330	4331	rBV	1594	383	0.05%	0.006%
92	15.011	4343	4345	4346	rBV2	1507	683	0.09%	0.011%
93	15.169	4392	4394	4398	rBV5	2202	1874	0.26%	0.031%




Sum of corrected areas: 6051133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031195.D
Acq On : 23 May 2023 17:14
Operator : SY/MD
Sample : 02865-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

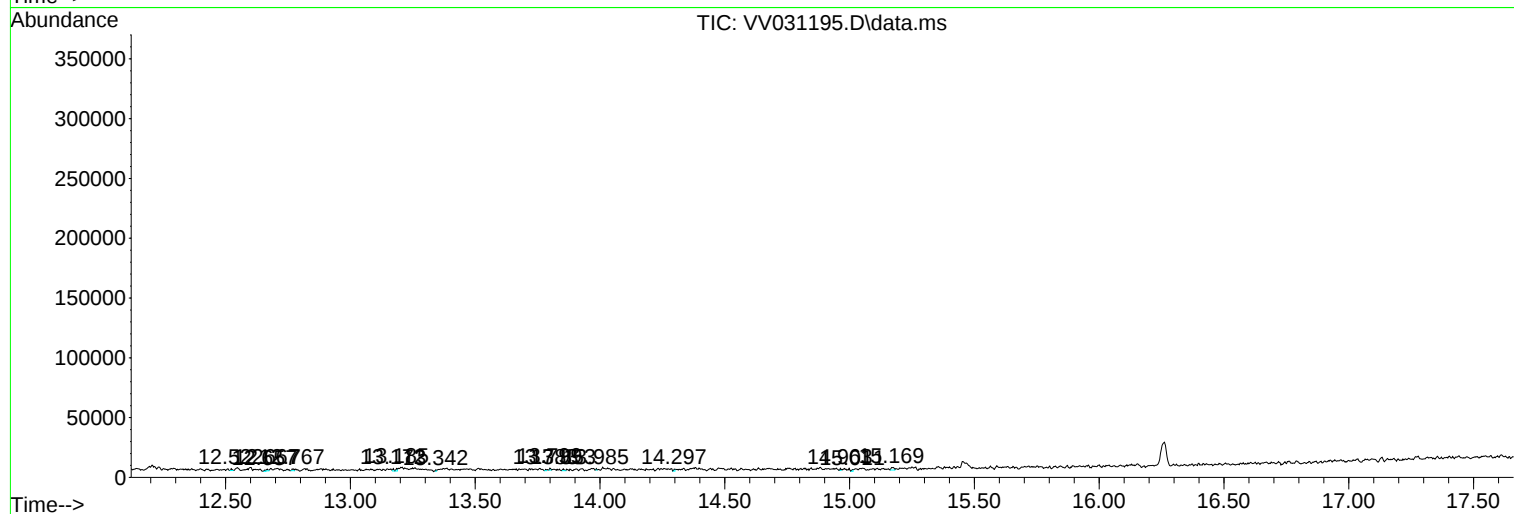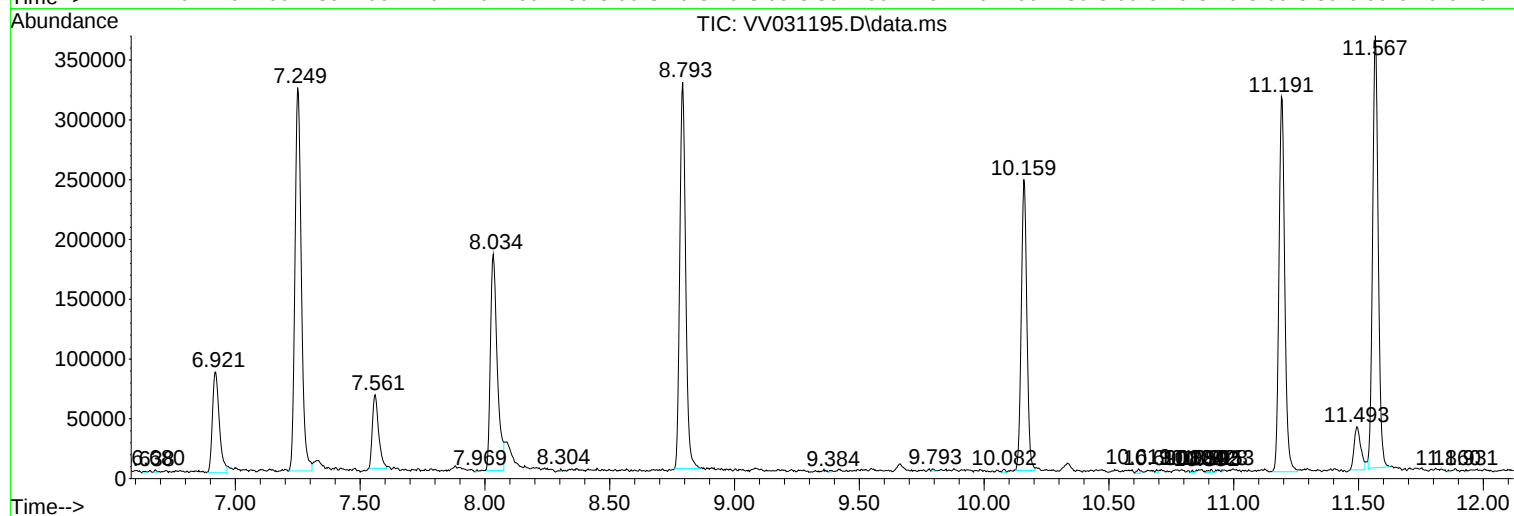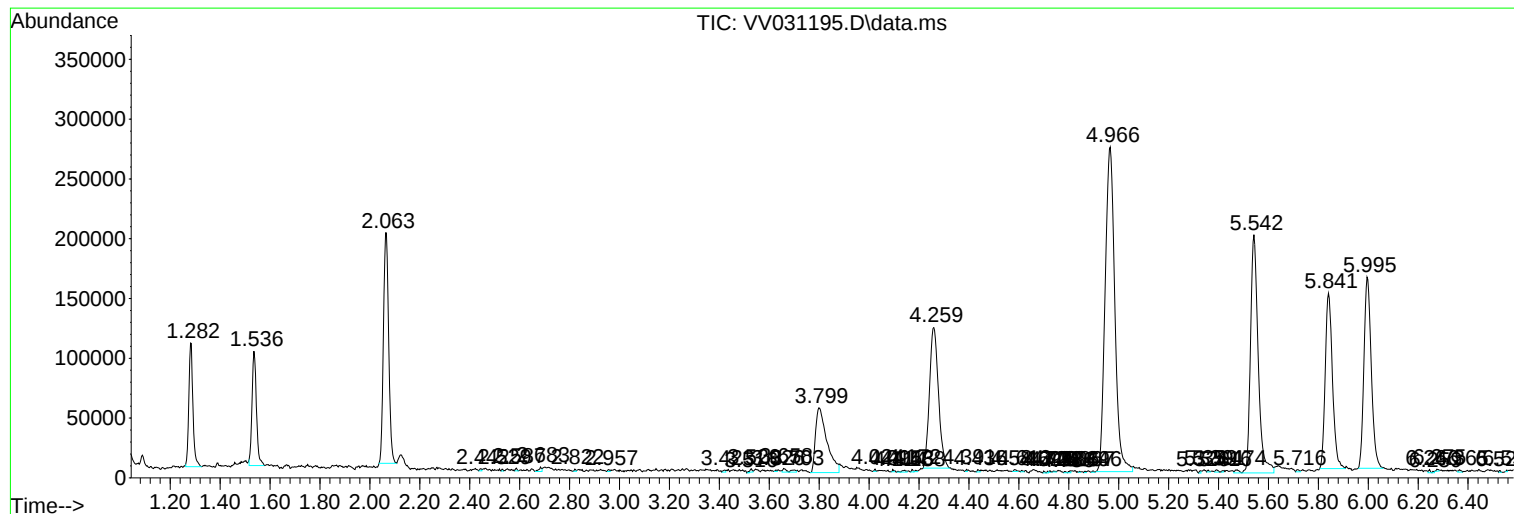

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031195.D
Acq On : 23 May 2023 17:14
Operator : SY/MD
Sample : 02865-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031195.D
Acq On : 23 May 2023 17:14
Operator : SY/MD
Sample : 02865-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc