

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031196.D
 Acq On : 23 May 2023 17:38
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rVB	104696	113393	14.58%	1.786%
2	1.539	148	155	166	rVB	99536	120170	15.45%	1.893%
3	2.063	310	318	331	rVB	201067	291700	37.50%	4.594%
4	2.503	450	455	457	rBV6	1973	2170	0.28%	0.034%
5	2.709	510	519	520	rBV8	3737	5296	0.68%	0.083%
6	2.796	543	546	547	rBV2	1591	867	0.11%	0.014%
7	2.883	570	573	574	rBV3	1325	713	0.09%	0.011%
8	2.918	582	584	588	rVB4	2067	833	0.11%	0.013%
9	2.938	588	590	593	rBV4	1375	941	0.12%	0.015%
10	3.034	617	620	622	rBV4	1448	925	0.12%	0.015%
11	3.069	627	631	632	rBV4	1941	1264	0.16%	0.020%
12	3.220	676	678	679	rBV2	1293	681	0.09%	0.011%
13	3.262	689	691	695	rBV5	1595	1096	0.14%	0.017%
14	3.333	708	713	715	rBV6	2200	1535	0.20%	0.024%
15	3.362	718	722	724	rBV6	1937	1348	0.17%	0.021%
16	3.401	731	734	739	rBV5	1502	1432	0.18%	0.023%
17	3.423	739	741	743	rBV3	1867	1026	0.13%	0.016%
18	3.478	756	758	762	rVV5	1236	863	0.11%	0.014%
19	3.539	775	777	780	rBV4	1253	906	0.12%	0.014%
20	3.622	801	803	805	rBV3	1157	685	0.09%	0.011%
21	3.696	824	826	830	rVB5	1927	1173	0.15%	0.018%
22	3.764	846	847	849	rBV2	1343	668	0.09%	0.011%
23	3.806	849	860	888	rVV3	57937	199773	25.68%	3.146%
24	4.156	967	969	972	rBV3	1985	1187	0.15%	0.019%
25	4.201	981	983	985	rBV3	1495	736	0.09%	0.012%
26	4.256	988	1000	1024	rVV2	131215	337471	43.39%	5.315%
27	4.352	1027	1030	1035	rBV6	2286	1994	0.26%	0.031%
28	4.638	1114	1119	1120	rBV5	2061	1612	0.21%	0.025%
29	4.712	1139	1142	1145	rBV4	1539	1056	0.14%	0.017%
30	4.780	1157	1163	1166	rBV8	1859	1968	0.25%	0.031%
31	4.966	1203	1221	1247	rBV3	288951	777825	100.00%	12.251%
32	5.542	1388	1400	1424	rBV	207382	434212	55.82%	6.839%
33	5.841	1481	1493	1510	rBV	233596	464525	59.72%	7.316%
34	5.995	1531	1541	1560	rVB2	173940	349649	44.95%	5.507%
35	6.333	1642	1646	1648	rBV4	1931	1503	0.19%	0.024%
36	6.577	1720	1722	1724	rBV3	1787	843	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031196.D
 Acq On : 23 May 2023 17:38
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.632	1737	1739	1743	rVB5	1930	1041	0.13%	0.016%
38	6.757	1776	1778	1781	rBV4	1646	1095	0.14%	0.017%
39	6.844	1804	1805	1808	rBV3	1647	804	0.10%	0.013%
40	6.918	1820	1828	1846	rBV	83185	148379	19.08%	2.337%
41	7.249	1920	1931	1948	rBV	336972	583581	75.03%	9.191%
42	7.494	2005	2007	2011	rBV5	1684	1396	0.18%	0.022%
43	7.558	2019	2027	2042	rBV2	62585	109806	14.12%	1.729%
44	7.677	2062	2064	2069	rVB6	2473	1666	0.21%	0.026%
45	7.789	2095	2099	2101	rBV5	1996	1203	0.15%	0.019%
46	7.828	2108	2111	2112	rBV3	1257	716	0.09%	0.011%
47	7.886	2125	2129	2132	rBV5	3642	3061	0.39%	0.048%
48	8.034	2165	2175	2202	rBV	149630	323633	41.61%	5.097%
49	8.461	2306	2308	2311	rBV4	1398	699	0.09%	0.011%
50	8.635	2358	2362	2365	rBV6	1525	1298	0.17%	0.020%
51	8.712	2383	2386	2389	rBV5	947	802	0.10%	0.013%
52	8.793	2400	2411	2433	rBV	313370	524750	67.46%	8.265%
53	9.050	2489	2491	2495	rVB5	1295	801	0.10%	0.013%
54	9.246	2550	2552	2554	rVB3	1976	786	0.10%	0.012%
55	9.304	2568	2570	2571	rBV2	2401	1032	0.13%	0.016%
56	9.342	2580	2582	2583	rBV2	1960	786	0.10%	0.012%
57	9.381	2592	2594	2596	rBV4	1659	857	0.11%	0.013%
58	9.484	2624	2626	2627	rBV2	1594	713	0.09%	0.011%
59	10.018	2790	2792	2795	rBV3	1787	786	0.10%	0.012%
60	10.040	2798	2799	2803	rVB4	1838	1000	0.13%	0.016%
61	10.072	2805	2809	2810	rBV4	2406	1135	0.15%	0.018%
62	10.159	2825	2836	2852	rBV	242915	384489	49.43%	6.056%
63	10.381	2902	2905	2909	rBV6	2112	1956	0.25%	0.031%
64	10.432	2917	2921	2925	rBV7	3267	2580	0.33%	0.041%
65	10.538	2952	2954	2955	rBV2	1648	744	0.10%	0.012%
66	10.616	2976	2978	2984	rVB6	2695	2419	0.31%	0.038%
67	10.667	2991	2994	2995	rBV3	1546	961	0.12%	0.015%
68	11.034	3104	3108	3110	rBV5	2671	2044	0.26%	0.032%
69	11.082	3121	3123	3126	rBV3	1800	1072	0.14%	0.017%
70	11.108	3127	3131	3133	rVV5	2242	1501	0.19%	0.024%
71	11.191	3145	3157	3174	rBV	332930	522785	67.21%	8.234%
72	11.567	3264	3274	3287	rBV	360215	556731	71.58%	8.769%
73	11.963	3394	3397	3399	rBV3	1974	1497	0.19%	0.024%
74	12.117	3443	3445	3448	rBV4	1460	972	0.12%	0.015%
75	12.159	3455	3458	3460	rBV4	1771	1043	0.13%	0.016%
76	12.532	3572	3574	3578	rVB6	2491	1472	0.19%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
 Data File : VV031196.D
 Acq On : 23 May 2023 17:38
 Operator : SY/MD
 Sample : 02865-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.551	3578	3580	3582	rBV3	1515	844	0.11%	0.013%
78	12.567	3582	3585	3587	rBV4	1710	1152	0.15%	0.018%
79	12.735	3633	3637	3639	rVB5	1726	1113	0.14%	0.018%
80	12.747	3639	3641	3644	rBV3	1664	966	0.12%	0.015%
81	12.850	3672	3673	3675	rBV2	1499	694	0.09%	0.011%
82	13.149	3764	3766	3769	rBV4	1909	1258	0.16%	0.020%
83	13.313	3814	3817	3818	rBV2	1852	865	0.11%	0.014%
84	13.339	3823	3825	3828	rBV4	1564	809	0.10%	0.013%
85	13.471	3863	3866	3868	rBV4	1905	1204	0.15%	0.019%
86	13.632	3915	3916	3920	rBV4	1404	978	0.13%	0.015%
87	13.731	3945	3947	3951	rVB4	2290	1585	0.20%	0.025%
88	13.757	3951	3955	3957	rBV5	2778	1735	0.22%	0.027%
89	13.853	3983	3985	3988	rBV4	1538	1155	0.15%	0.018%
90	13.969	4018	4021	4023	rBV4	2105	1378	0.18%	0.022%
91	14.101	4059	4062	4065	rBV5	1925	1361	0.17%	0.021%
92	14.188	4083	4089	4091	rBV6	1712	1852	0.24%	0.029%
93	14.207	4092	4095	4098	rBV5	1411	1068	0.14%	0.017%
94	14.288	4118	4120	4124	rBV4	2452	1977	0.25%	0.031%
95	14.419	4157	4161	4163	rBV6	2389	1801	0.23%	0.028%
96	14.532	4192	4196	4198	rBV4	1844	1403	0.18%	0.022%
97	14.673	4238	4240	4245	rBV6	1910	1596	0.21%	0.025%
98	14.741	4259	4261	4262	rBV2	1943	830	0.11%	0.013%
99	14.898	4308	4310	4314	rBV4	2331	1569	0.20%	0.025%
100	15.091	4368	4370	4374	rBV4	2825	1843	0.24%	0.029%



Sum of corrected areas: 6349167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031196.D
Acq On : 23 May 2023 17:38
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

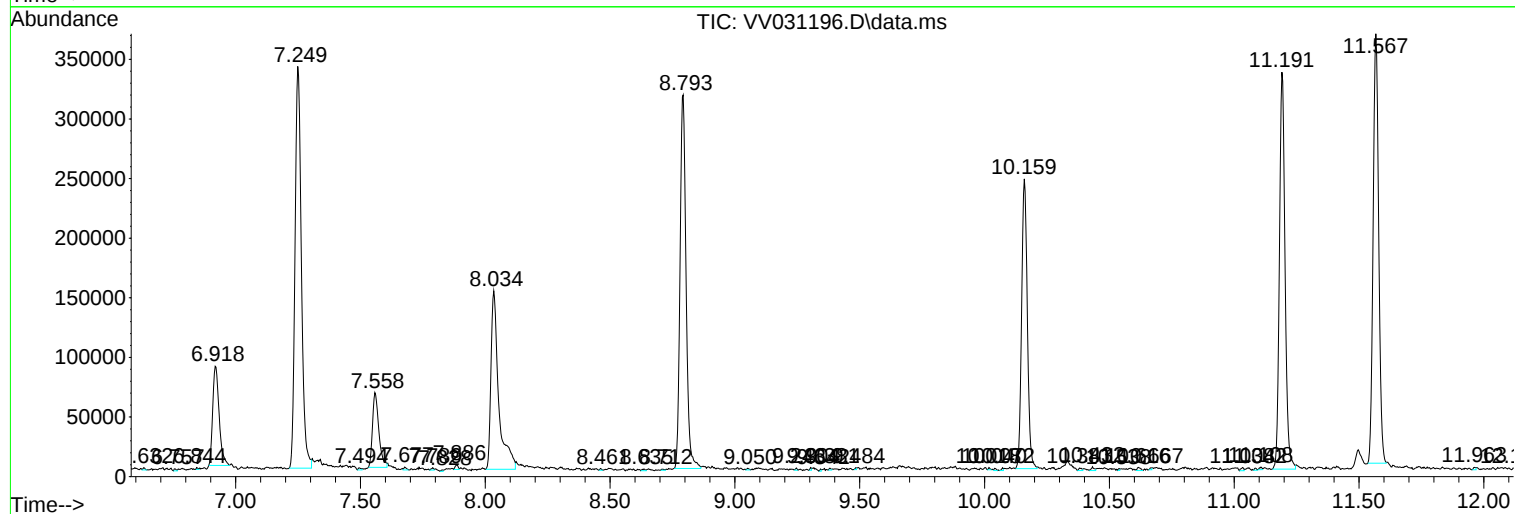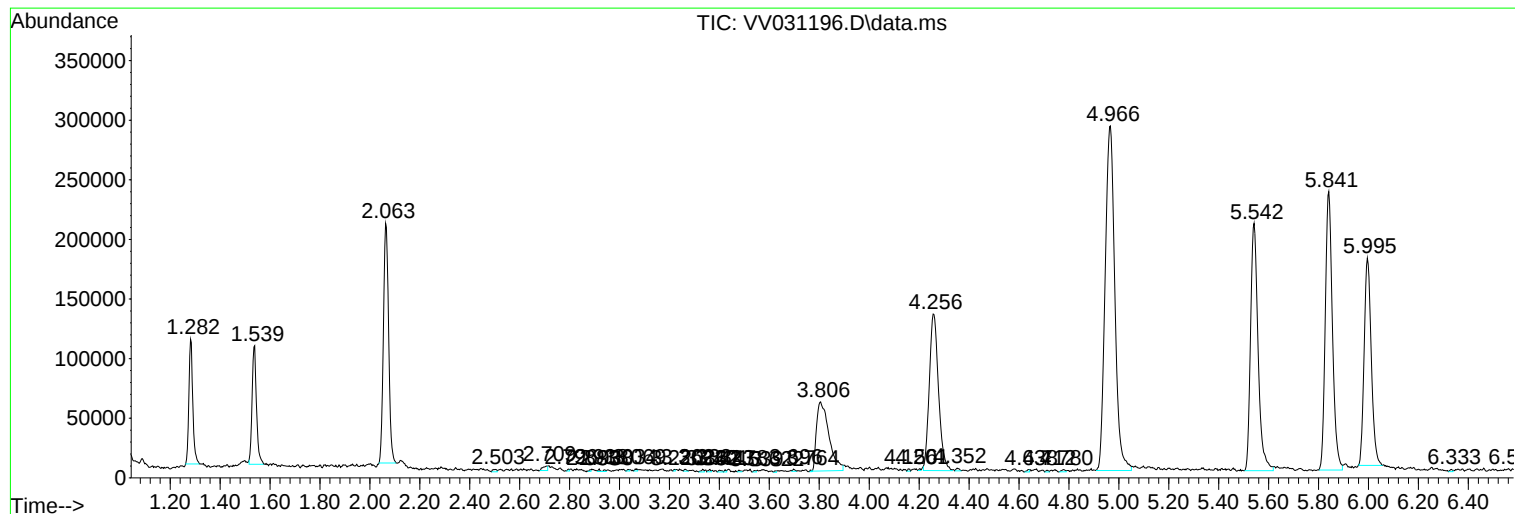

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031196.D
Acq On : 23 May 2023 17:38
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031196.D
Acq On : 23 May 2023 17:38
Operator : SY/MD
Sample : 02865-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------