
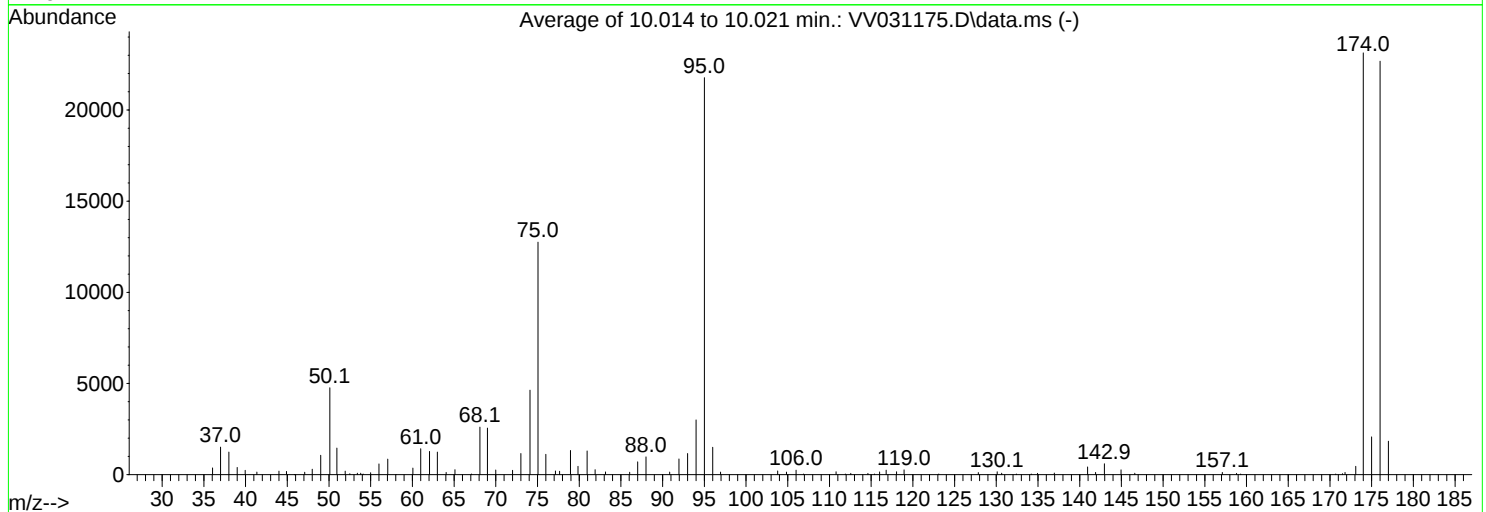


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052323\
Data File : VV031175.D
Acq On : 23 May 2023 08:58
Operator : SY/MD
Sample : BFB378
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB378

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis
Last Update : Thu May 25 01:11:46 2023

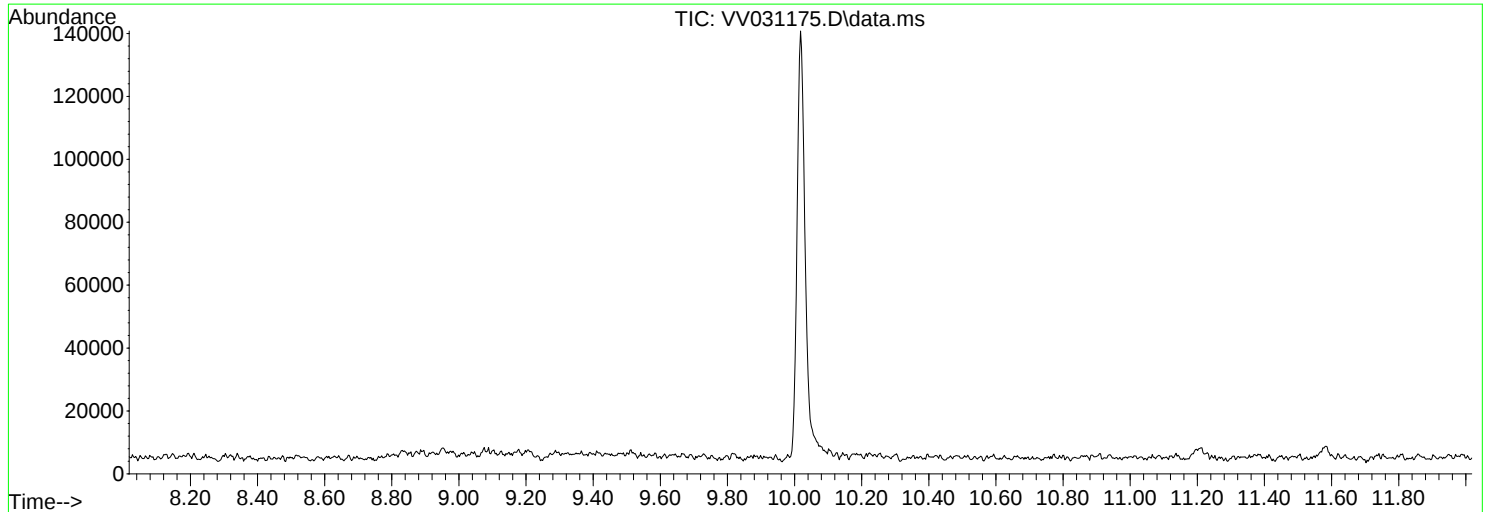

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	4770	PASS
75	95	30	80	58.5	12748	PASS
95	95	100	100	100.0	21773	PASS
96	95	5	9	6.9	1504	PASS
173	174	0.00	2	2.0	459	PASS
174	95	50	120	106.3	23136	PASS
175	174	5	9	9.0	2072	PASS
176	174	95	105	98.0	22677	PASS
177	176	5	10	8.1	1837	PASS

m/z	Abundance
35.30	186.0
36.10	121.0
36.70	149.0
38.00	126.0
38.60	124.0
39.10	150.0
39.70	261.0
40.20	148.0
40.70	162.0
41.60	172.0
42.10	151.0
42.60	173.0
43.30	147.0
44.00	200.0
44.80	111.0
45.80	162.0
47.20	137.0
48.40	104.0
49.10	116.0
49.50	133.0
50.10	119.0
50.80	128.0
53.10	149.0
55.10	105.0
58.20	115.0
61.90	161.0
64.10	124.0
64.70	105.0
66.40	103.0
67.10	102.0
68.40	100.0
69.20	132.0
70.00	103.0
74.90	146.0
79.80	107.0
84.00	116.0
87.00	117.0
93.00	100.0
99.10	107.0
103.00	102.0
113.80	114.0
137.50	112.0
289.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
35.10	168.0
36.00	441.0
37.00	1511.0
38.00	1446.0
39.00	570.0
40.00	215.0
41.40	161.0
42.10	116.0
42.50	135.0
43.20	150.0
44.00	392.0
45.00	338.0
45.90	154.0
47.00	278.0
48.00	347.0
49.00	1263.0
50.10	4849.0
51.00	1532.0
51.90	204.0
53.40	109.0
54.10	105.0
54.90	185.0
56.00	585.0
57.00	939.0
58.00	119.0
60.00	317.0
61.00	1392.0
62.10	1512.0
63.00	1194.0
64.00	195.0
65.10	221.0
67.20	158.0
68.10	2484.0
69.00	2595.0
70.00	398.0
72.00	255.0
73.00	1168.0
74.10	4543.0
75.10	12493.0
76.00	1221.0
77.20	192.0
77.70	193.0
79.00	1349.0
79.90	466.0
80.90	1347.0
81.90	298.0
83.10	135.0
86.10	116.0
87.00	847.0
88.00	877.0
90.90	161.0
91.90	821.0
93.00	1237.0
94.00	3015.0
95.00	21352.0
96.00	1275.0
96.90	131.0
103.80	197.0
104.90	170.0
106.00	203.0
106.90	111.0
110.80	131.0
111.90	101.0
112.60	122.0
114.60	117.0
116.00	109.0
116.80	262.0
118.00	177.0
118.90	249.0
123.10	105.0
127.80	108.0
130.10	185.0
134.20	103.0
140.90	435.0
141.90	108.0
142.90	641.0
145.00	231.0
146.60	126.0
157.10	104.0
159.30	117.0
171.80	202.0
173.10	423.0
174.00	21864.0
175.00	2042.0
176.00	21288.0
177.00	1675.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
36.00	493.0
37.00	1572.0
38.00	1397.0
39.00	526.0
39.90	247.0
40.90	111.0
41.40	144.0
42.00	121.0
42.50	180.0
43.30	159.0
44.00	410.0
45.10	293.0
46.00	159.0
47.10	291.0
48.00	281.0
49.00	1201.0
50.10	5005.0
51.00	1648.0
52.00	182.0
53.40	115.0
53.80	111.0
55.00	230.0
56.00	606.0
57.00	888.0
58.00	109.0
60.10	356.0
61.00	1468.0
62.10	1478.0
63.00	1259.0
64.00	243.0
65.10	297.0
67.10	139.0
68.10	2700.0
69.00	2820.0
70.00	377.0
72.00	233.0
73.00	1176.0
74.10	4813.0
75.10	13273.0
76.00	1129.0
77.10	209.0
77.70	209.0
78.90	1353.0
79.90	609.0
80.90	1324.0
81.90	269.0
83.20	162.0
86.10	131.0
87.10	823.0
88.00	993.0
90.80	144.0
92.00	906.0
93.00	1325.0
94.00	3064.0
95.00	22624.0
96.00	1562.0
97.00	144.0
103.80	200.0
104.90	134.0
106.00	248.0
110.80	165.0
112.50	101.0
114.60	103.0
115.40	105.0
116.00	142.0
116.80	251.0
118.00	155.0
119.00	265.0
127.90	106.0
130.10	171.0
130.70	108.0
134.90	100.0
136.90	110.0
141.00	455.0
141.90	131.0
143.00	641.0
145.00	294.0
146.60	106.0
157.10	132.0
158.80	115.0
171.80	166.0
173.10	480.0
174.00	24096.0
175.00	2186.0
176.00	23480.0
177.00	1949.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
36.10	539.0
37.00	1457.0
38.00	1242.0
39.00	536.0
40.00	247.0
40.90	121.0
41.30	131.0
42.00	121.0
42.60	194.0
44.00	378.0
44.90	227.0
46.00	177.0
47.10	236.0
48.00	257.0
49.00	1081.0
50.10	4813.0
51.00	1569.0
52.00	185.0
52.50	164.0
53.80	118.0
55.10	228.0
56.00	573.0
57.10	729.0
58.00	144.0
60.00	395.0
61.00	1411.0
62.10	1303.0
63.00	1266.0
64.10	293.0
65.10	309.0
67.00	109.0
68.10	2647.0
69.00	2647.0
70.00	300.0
72.00	223.0
73.00	1125.0
74.10	4540.0
75.10	12917.0
76.00	983.0
77.20	216.0
77.60	152.0
78.90	1269.0
79.90	621.0
81.00	1222.0
81.90	238.0
83.20	146.0
86.00	141.0
87.10	784.0
88.00	1056.0
90.90	116.0
92.00	847.0
93.00	1224.0
94.00	2939.0
95.00	21344.0
96.00	1675.0
97.00	136.0
103.80	206.0
104.80	115.0
106.00	277.0
110.80	180.0
116.00	187.0
116.80	215.0
118.10	149.0
119.00	279.0
127.90	127.0
130.10	126.0
130.60	122.0
132.40	105.0
135.00	104.0
137.00	155.0
141.00	386.0
141.90	124.0
143.00	520.0
144.80	273.0
157.10	134.0
158.80	105.0
170.70	118.0
171.50	148.0
173.10	475.0
174.00	23448.0
175.00	1988.0
176.00	23264.0
177.00	1888.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378