


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052421\
 Data File : VV021375.D
 Acq On : 24 May 2021 09:16
 Operator : SY/MD
 Sample : BFB98
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB198

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM052021.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 25 01:36:53 2021

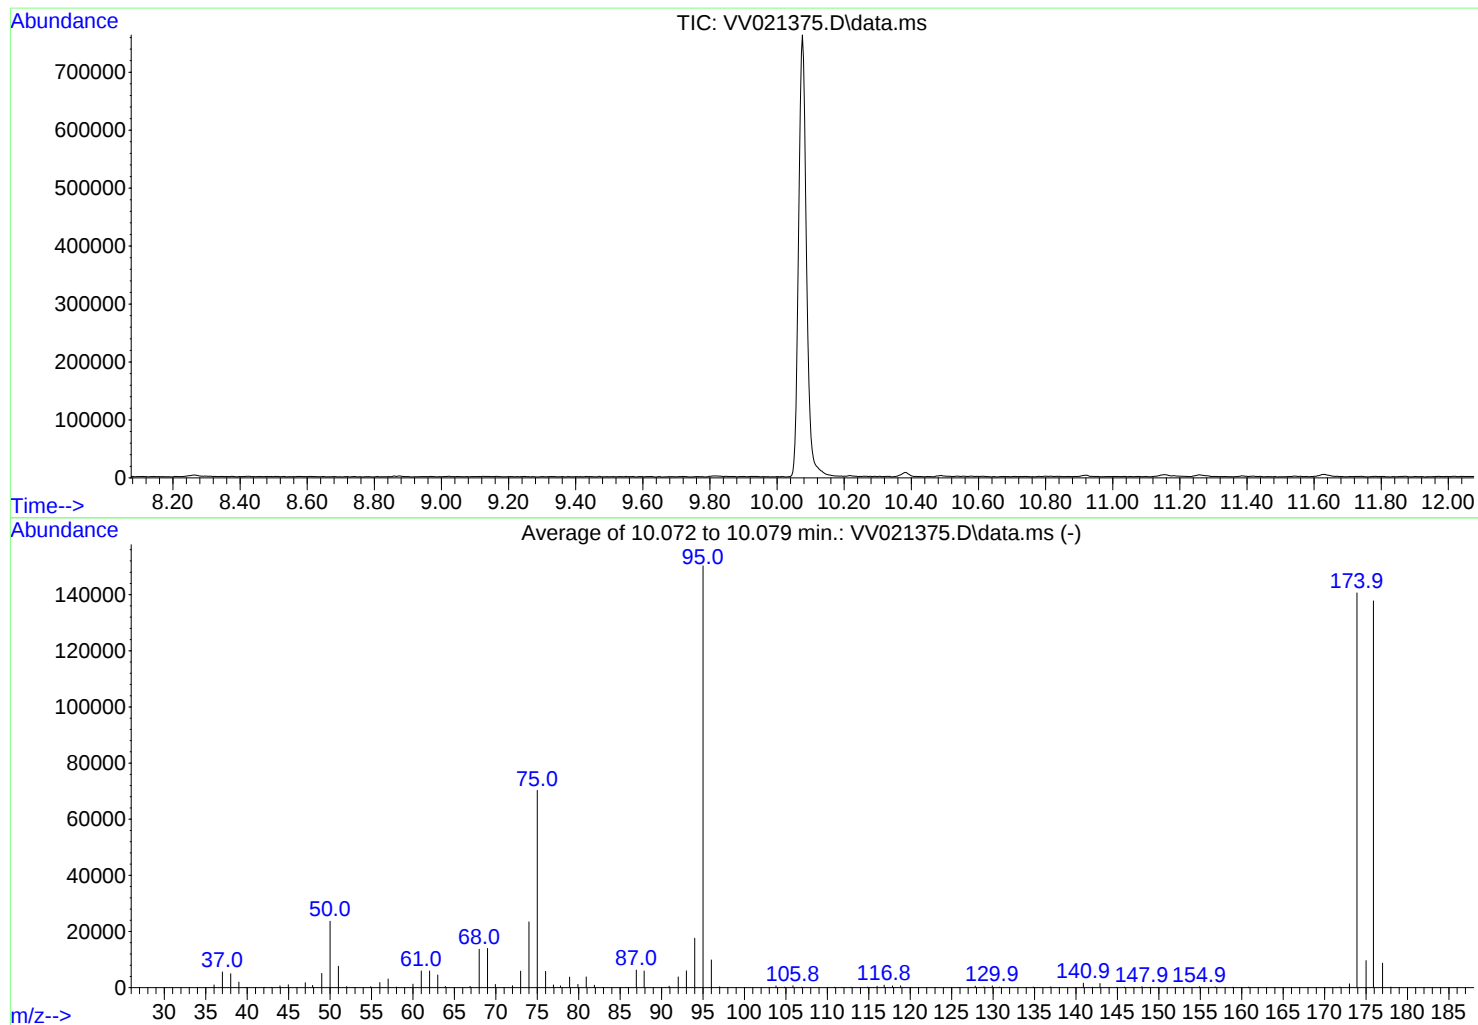

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	23677	PASS
75	95	30	80	46.8	70280	PASS
95	95	100	100	100.0	150272	PASS
96	95	5	9	6.6	9877	PASS
173	174	0.00	2	1.0	1389	PASS
174	95	50	120	93.6	140608	PASS
175	174	5	9	6.9	9660	PASS
176	174	95	101	98.0	137771	PASS
177	176	5	9	6.3	8735	PASS

m/z	Abundance
36.00	1020.0
37.00	5719.0
38.00	5144.0
39.00	2056.0
40.00	335.0
41.10	194.0
42.10	113.0
42.90	303.0
44.00	1192.0
45.00	1071.0
47.00	1865.0
47.90	841.0
49.00	5284.0
50.00	24432.0
51.00	7926.0
52.00	415.0
52.80	108.0
54.90	564.0
56.00	1862.0
57.00	3400.0
58.00	265.0
60.00	1285.0
61.00	6100.0
62.00	6094.0
63.00	4658.0
63.90	513.0
66.90	464.0
68.00	14182.0
69.00	14434.0
70.00	1194.0
70.90	106.0
72.00	721.0
73.00	6025.0
74.00	24144.0
75.00	72560.0
76.00	6021.0
77.00	984.0
77.80	689.0
78.90	3880.0
79.90	1175.0
80.90	4090.0
81.90	883.0
82.90	147.0
85.70	165.0
86.90	6527.0
87.90	6111.0
90.90	511.0
92.00	3947.0
93.00	6158.0
94.00	18192.0
95.00	155264.0
96.00	10279.0
97.00	321.0
103.00	103.0
103.80	692.0
104.90	220.0
105.80	691.0
106.90	202.0
110.80	167.0
111.80	125.0
112.80	170.0
114.90	217.0
116.00	521.0
116.90	958.0
117.90	642.0
118.80	728.0
125.80	105.0
127.90	575.0
128.90	307.0
129.90	642.0
130.80	254.0
134.90	257.0
137.00	303.0
139.90	134.0
140.90	1682.0
142.00	181.0
142.90	1551.0
144.00	121.0
144.90	135.0
145.80	241.0
146.80	122.0
147.90	346.0
148.90	198.0
149.90	194.0
152.00	121.0
154.90	370.0
156.80	276.0
158.90	201.0
160.90	221.0
171.80	241.0
173.00	1459.0
173.90	145344.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198

175.00	9856.0
175.90	142208.0
177.00	8913.0
178.00	247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198

m/z	Abundance
36.00	922.0
37.00	5230.0
38.00	4703.0
39.00	1917.0
39.90	320.0
41.20	199.0
42.10	151.0
42.90	311.0
44.00	1151.0
44.90	1013.0
47.00	1635.0
47.90	790.0
49.00	4963.0
50.00	22888.0
51.00	7241.0
52.00	334.0
52.80	123.0
54.90	514.0
56.00	1874.0
57.00	3286.0
58.00	230.0
60.00	1166.0
61.00	5597.0
62.00	5782.0
63.00	4513.0
63.90	434.0
66.90	455.0
68.00	13180.0
69.00	13424.0
70.00	1078.0
70.90	115.0
72.00	705.0
73.00	5559.0
74.00	22080.0
75.00	67176.0
76.00	5589.0
77.00	809.0
77.80	597.0
78.90	3534.0
79.90	1081.0
80.90	4001.0
81.90	862.0
82.90	145.0
85.70	151.0
86.90	6195.0
87.90	5812.0
90.90	500.0
92.00	3622.0
93.00	5704.0
94.00	16992.0
95.00	145280.0
96.00	9709.0
97.00	271.0
102.90	106.0
103.80	670.0
104.80	226.0
105.90	707.0
106.80	228.0
110.80	166.0
111.70	108.0
112.90	125.0
114.90	224.0
116.00	524.0
116.90	993.0
117.90	575.0
118.90	674.0
127.80	571.0
128.80	355.0
129.90	635.0
130.80	220.0
134.90	283.0
136.90	350.0
139.90	133.0
140.90	1560.0
142.00	168.0
142.90	1533.0
144.90	132.0
145.90	253.0
146.90	115.0
148.00	335.0
148.90	168.0
150.00	209.0
152.00	133.0
154.90	328.0
156.80	239.0
157.00	238.0
158.90	238.0
160.80	198.0
171.40	133.0
171.90	207.0
173.00	1373.0
173.90	140288.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198

175.00	9360.0
175.90	136064.0
177.00	8697.0
178.00	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198

m/z	Abundance
36.00	991.0
37.00	5801.0
38.00	4991.0
39.00	2043.0
40.00	338.0
41.00	185.0
43.00	300.0
44.00	1080.0
45.00	980.0
47.00	1800.0
47.90	775.0
49.00	5030.0
50.00	23712.0
51.00	7722.0
52.00	423.0
55.00	544.0
56.00	1753.0
57.00	3155.0
58.00	286.0
60.00	1274.0
61.00	6104.0
62.00	5995.0
63.00	4353.0
63.90	495.0
66.90	477.0
68.00	13646.0
69.00	14014.0
69.90	1199.0
72.00	696.0
73.00	5988.0
74.00	24088.0
75.00	71104.0
76.00	5908.0
76.90	1064.0
77.80	692.0
78.90	3807.0
79.90	1168.0
80.90	3754.0
81.90	798.0
82.90	138.0
86.00	183.0
87.00	6155.0
87.90	5905.0
90.90	517.0
92.00	3968.0
93.00	6142.0
94.00	17632.0
95.00	150272.0
96.00	9644.0
97.00	327.0
103.80	614.0
104.90	214.0
105.80	624.0
107.00	185.0
110.90	127.0
111.80	138.0
112.80	196.0
114.80	206.0
116.00	478.0
116.80	878.0
117.80	644.0
118.90	707.0
127.90	521.0
129.00	238.0
129.90	588.0
130.80	278.0
134.80	241.0
136.90	246.0
139.90	122.0
140.90	1642.0
142.00	184.0
142.90	1463.0
144.80	112.0
145.80	199.0
146.80	126.0
147.90	329.0
149.00	196.0
149.80	206.0
154.90	346.0
156.80	311.0
159.00	181.0
160.90	225.0
171.80	243.0
173.00	1336.0
173.90	136192.0
175.00	9765.0
175.90	135040.0
177.00	8594.0
178.00	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198

m/z	Abundance
39.80	215.0
41.00	159.0
41.80	104.0
42.90	161.0
43.90	496.0
54.80	200.0
57.10	202.0
80.90	101.0
83.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB198