

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052423\
 Data File : VW031218.D
 Acq On : 24 May 2023 16:21
 Operator : SY/MD
 Sample : 02865-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX75

Quant Time: May 25 01:15:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 25 01:11:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	178278	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	174920	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	89925	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	56413	37.026	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.060%
7) Chloroethane-d5	1.535	69	52448	44.685	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.360%
11) 1,1-Dichloroethene-d2	2.063	65	30276	42.376	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.760%
21) 2-Butanone-d5	3.799	46	78732	96.979	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.980%
24) Chloroform-d	4.259	84	119577	44.364	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.720%
26) 1,2-Dichloroethane-d4	4.950	65	88213	48.432	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.860%
32) Benzene-d6	4.969	84	207501	43.759	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.520%
36) 1,2-Dichloropropane-d6	5.995	67	63316	44.625	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.260%
41) Toluene-d8	7.249	98	181230	40.949	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.900%
43) trans-1,3-Dichloroprop...	7.561	79	30583	42.963	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.920%
47) 2-Hexanone-d5	8.034	63	46314	83.721	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.720%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	89660	42.132	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.260%
66) 1,2-Dichlorobenzene-d4	11.567	152	80763	49.979	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.960%
Target Compounds						
					Qvalue	
13) Acetone	2.127	43	18254	17.295	ug/L	91
34) Trichloroethene	5.841	95	67944	60.510	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031218.D
Acq On : 24 May 2023 16:21
Operator : SY/MD
Sample : 02865-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX75

Quant Time: May 25 01:15:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 25 01:11:46 2023
Response via : Initial Calibration

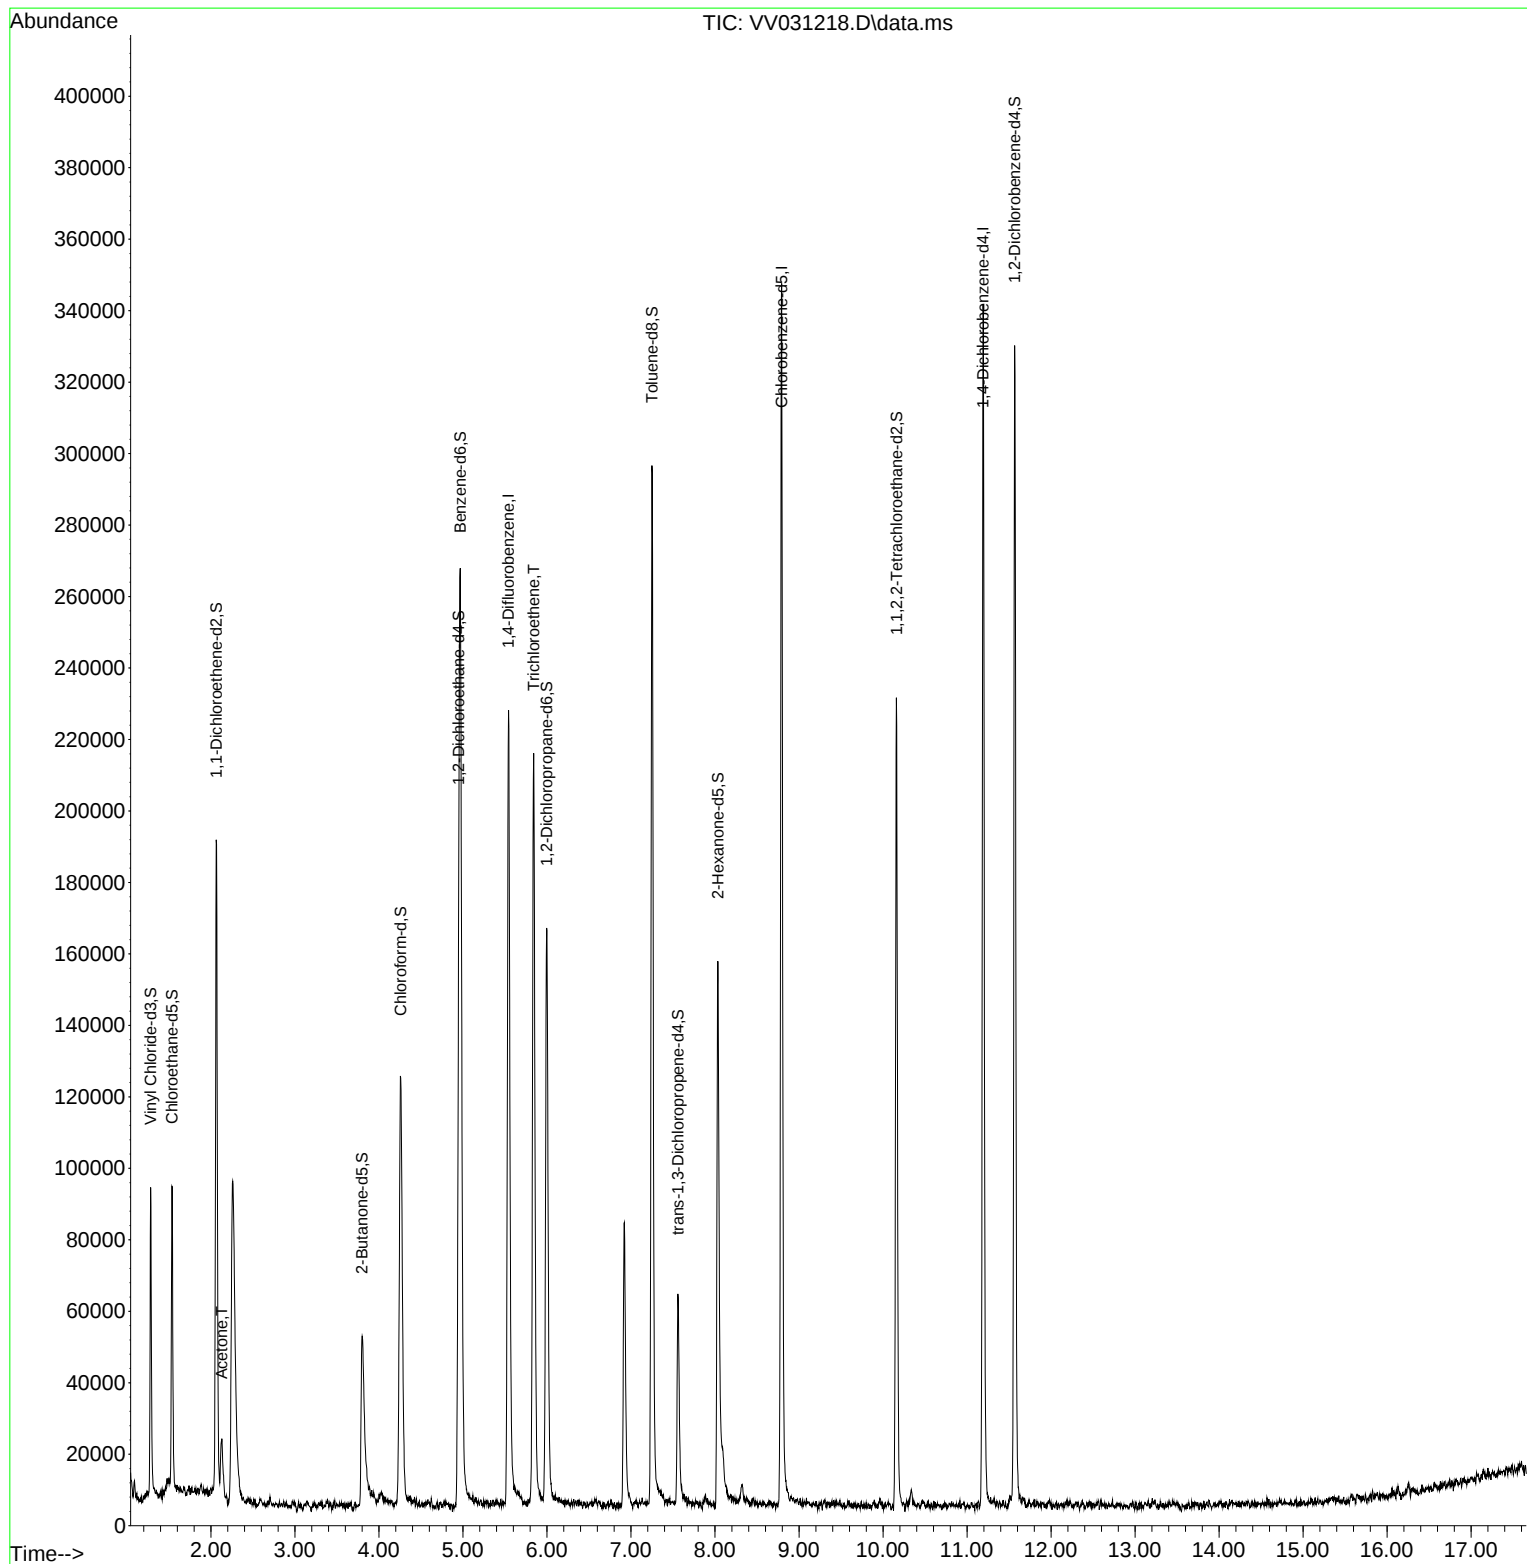

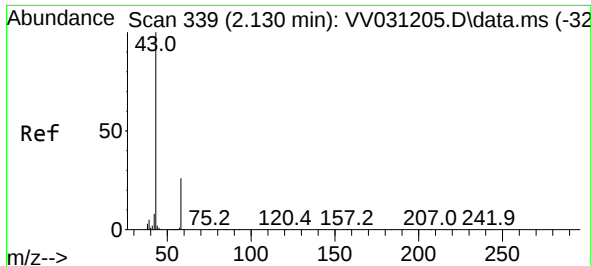

#13

Acetone

Concen: 17.295 ug/L

RT: 2.127 min Scan# 339

Delta R.T. -0.003 min

Lab File: VV031218.D

Acq: 24 May 2023 16:21

Instrument :

MSVOA_V

ClientSampleId :





GBX75

Tgt Ion: 43 Resp: 18254

Ion Ratio Lower Upper

43 100

58 22.3 0.0 54.0

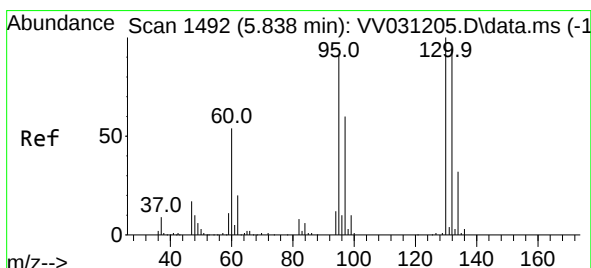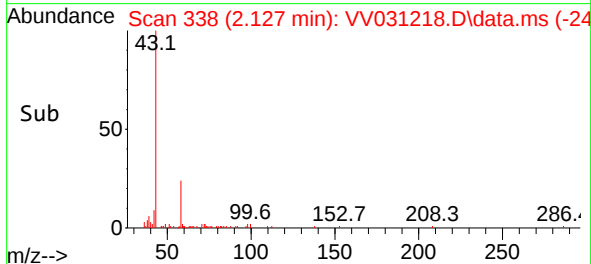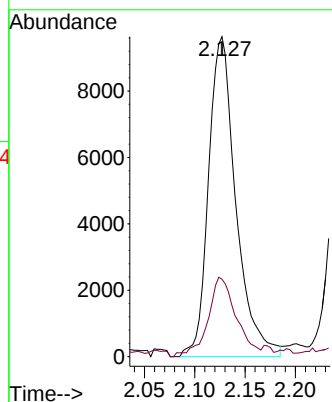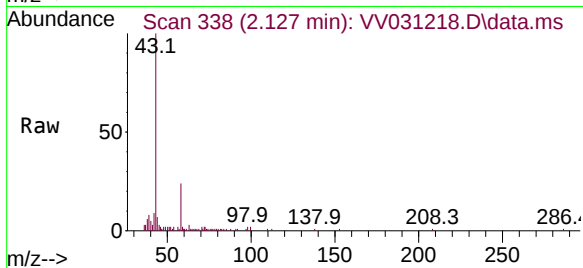

#34

Trichloroethene

Concen: 60.510 ug/L

RT: 5.841 min Scan# 1493

Delta R.T. 0.003 min

Lab File: VV031218.D

Acq: 24 May 2023 16:21

Tgt Ion: 95 Resp: 67944

Ion Ratio Lower Upper

95 100

97 63.9 44.4 82.5

132 102.9 70.2 130.4

130 104.2 71.5 132.7

