

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031224.D
 Acq On : 24 May 2023 18:45
 Operator : SY/MD
 Sample : 02866-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX93

Quant Time: May 25 01:17:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 25 01:11:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	178233	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	175320	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	89075	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	55353	36.340	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.680%
7) Chloroethane-d5	1.536	69	51352	43.762	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.520%
11) 1,1-Dichloroethene-d2	2.063	65	29908	41.871	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.740%
21) 2-Butanone-d5	3.799	46	78618	96.863	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.860%
24) Chloroform-d	4.259	84	120412	44.685	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.360%
26) 1,2-Dichloroethane-d4	4.950	65	90374	49.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.260%
32) Benzene-d6	4.969	84	208198	43.805	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.620%
36) 1,2-Dichloropropane-d6	5.998	67	62046	43.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.260%
41) Toluene-d8	7.249	98	185310	41.775	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.560%
43) trans-1,3-Dichloroprop...	7.558	79	31515	44.171	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.340%
47) 2-Hexanone-d5	8.030	63	48568	87.595	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.590%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	93755	43.956	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.920%
66) 1,2-Dichlorobenzene-d4	11.567	152	79482	49.655	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.320%
Target Compounds						
					Qvalue	
13) Acetone	2.124	43	5219	4.946	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031224.D
Acq On : 24 May 2023 18:45
Operator : SY/MD
Sample : 02866-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX93

Quant Time: May 25 01:17:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 25 01:11:46 2023
Response via : Initial Calibration

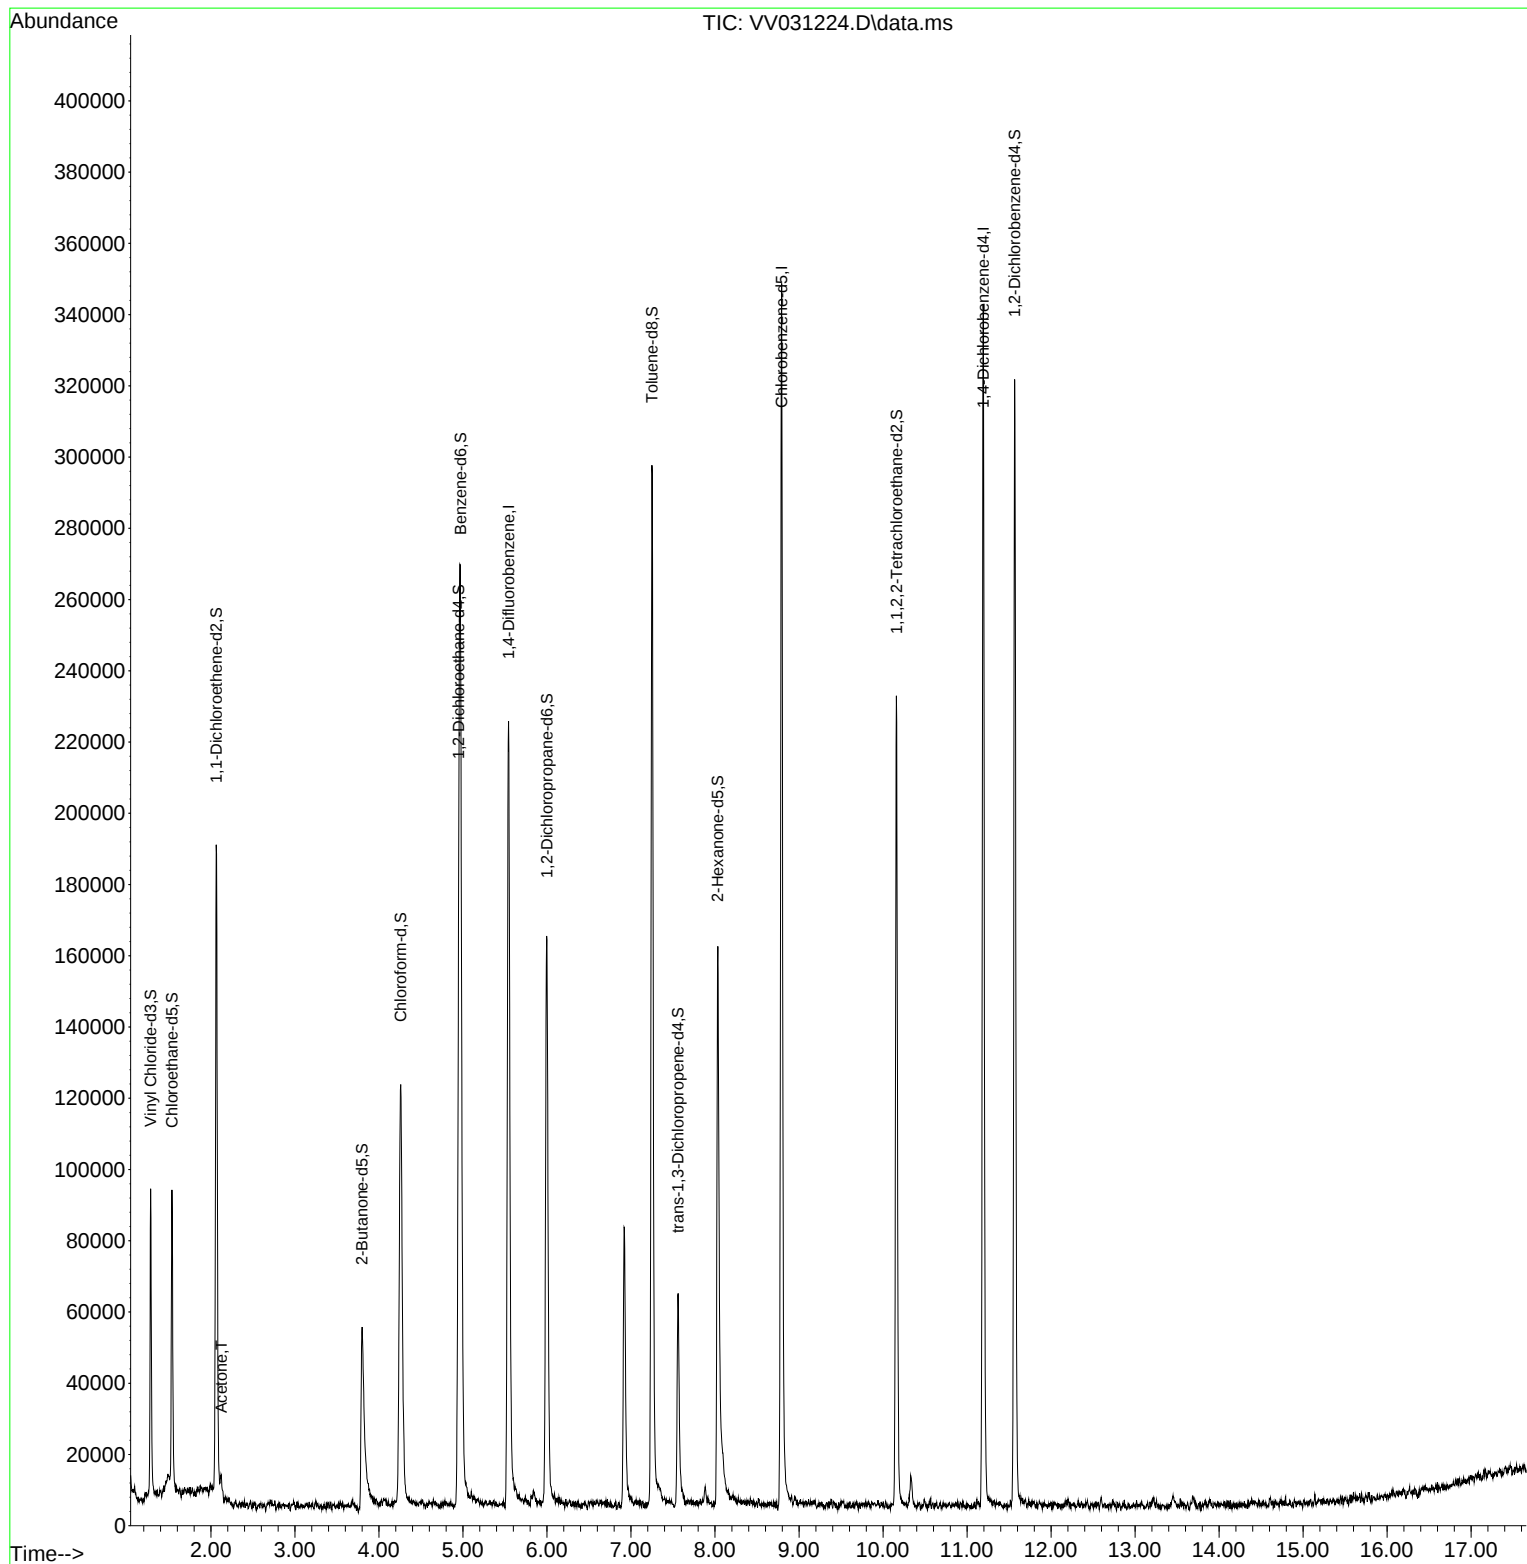

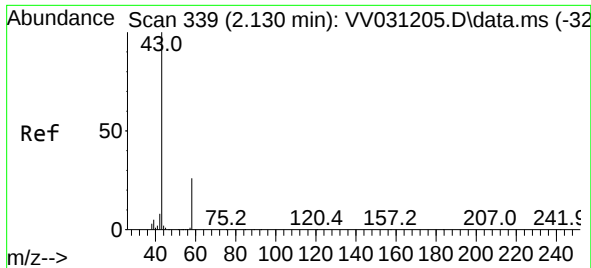

#13

Acetone

Concen: 4.946 ug/L

RT: 2.124 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV031224.D


Acq: 24 May 2023 18:45

Instrument :

MSVOA_V

ClientSampleId :

GBX93

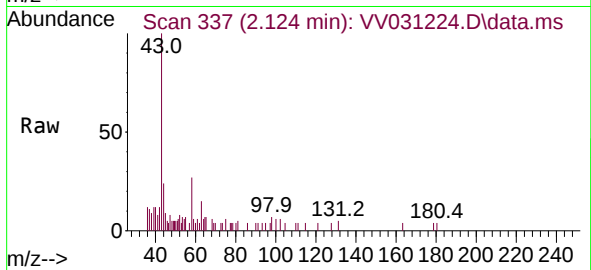

Tgt Ion: 43 Resp: 5219

Ion Ratio Lower Upper

43 100

58 18.0 0.0 54.0

