

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031206.D
 Acq On : 24 May 2023 11:30
 Operator : SY/MD
 Sample : VV0524WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	100946	110229	14.46%	1.904%
2	1.536	148	154	167	rVB	97929	121172	15.89%	2.093%
3	2.066	310	319	330	rVB	200777	286987	37.64%	4.957%
4	2.365	409	412	414	rVV4	1641	691	0.09%	0.012%
5	2.449	435	438	440	rBV4	2358	1763	0.23%	0.030%
6	2.568	473	475	477	rBV3	1515	794	0.10%	0.014%
7	2.629	492	494	496	rVB3	2454	1056	0.14%	0.018%
8	2.648	496	500	504	rBV6	2060	1898	0.25%	0.033%
9	2.841	557	560	561	rBV3	1854	919	0.12%	0.016%
10	2.902	576	579	581	rVB4	1394	695	0.09%	0.012%
11	2.992	603	607	611	rBV7	1102	852	0.11%	0.015%
12	3.098	636	640	644	rBV7	1764	1650	0.22%	0.028%
13	3.117	644	646	649	rBV3	1667	974	0.13%	0.017%
14	3.635	805	807	811	rBV4	1362	756	0.10%	0.013%
15	3.709	825	830	831	rBV5	1503	1240	0.16%	0.021%
16	3.802	849	859	884	rBV	44723	130578	17.13%	2.255%
17	4.172	971	974	977	rBV5	2213	1256	0.16%	0.022%
18	4.256	986	1000	1019	rBV	128446	322005	42.23%	5.562%
19	4.484	1069	1071	1074	rBV4	1245	806	0.11%	0.014%
20	4.606	1107	1109	1116	rVB6	2075	1864	0.24%	0.032%
21	4.732	1141	1148	1153	rBV10	2000	2465	0.32%	0.043%
22	4.751	1153	1154	1159	rVB4	2499	1588	0.21%	0.027%
23	4.831	1176	1179	1181	rVB4	1913	1060	0.14%	0.018%
24	4.844	1181	1183	1188	rBV5	1688	1138	0.15%	0.020%
25	4.870	1189	1191	1195	rVB5	1585	842	0.11%	0.015%
26	4.963	1204	1220	1244	rBV2	283047	762448	100.00%	13.169%
27	5.262	1308	1313	1318	rBV8	2385	2508	0.33%	0.043%
28	5.445	1366	1370	1371	rBV3	2280	1345	0.18%	0.023%
29	5.542	1388	1400	1417	rBV	213137	432754	56.76%	7.474%
30	5.902	1510	1512	1513	rBV2	1883	864	0.11%	0.015%
31	5.995	1530	1541	1559	rBV	172742	346585	45.46%	5.986%
32	6.558	1713	1716	1718	rBV5	1709	1150	0.15%	0.020%
33	6.625	1733	1737	1741	rBV6	1782	1592	0.21%	0.027%
34	6.748	1772	1775	1777	rBV4	1567	891	0.12%	0.015%
35	6.873	1811	1814	1816	rBV3	1813	934	0.12%	0.016%
36	6.921	1819	1829	1845	rVV	85175	159461	20.91%	2.754%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031206.D
 Acq On : 24 May 2023 11:30
 Operator : SY/MD
 Sample : VV0524WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.249	1918	1931	1947	rBV	325606	582258	76.37%	10.057%
38	7.558	2020	2027	2040	rBV	61549	101404	13.30%	1.751%
39	7.786	2096	2098	2100	rBV3	2038	873	0.11%	0.015%
40	7.937	2143	2145	2149	rBV5	1552	911	0.12%	0.016%
41	8.034	2166	2175	2205	rBV	153751	316280	41.48%	5.463%
42	8.265	2245	2247	2251	rBV5	1614	1122	0.15%	0.019%
43	8.352	2270	2274	2277	rBV8	1725	1690	0.22%	0.029%
44	8.532	2327	2330	2334	rVB5	2888	2044	0.27%	0.035%
45	8.657	2367	2369	2370	rBV2	1949	891	0.12%	0.015%
46	8.789	2397	2410	2431	rBV	335814	565788	74.21%	9.772%
47	9.162	2524	2526	2529	rBV4	2588	1967	0.26%	0.034%
48	9.259	2553	2556	2560	rBV5	1974	1779	0.23%	0.031%
49	9.329	2575	2578	2584	rBV8	1945	2713	0.36%	0.047%
50	9.490	2624	2628	2629	rBV4	1700	1163	0.15%	0.020%
51	9.606	2663	2664	2669	rBV4	975	895	0.12%	0.015%
52	9.661	2676	2681	2682	rBV6	1534	1317	0.17%	0.023%
53	9.747	2703	2708	2711	rBV7	1474	1264	0.17%	0.022%
54	9.876	2744	2748	2754	rBV8	2237	3057	0.40%	0.053%
55	9.918	2758	2761	2763	rBV4	1674	1138	0.15%	0.020%
56	9.982	2776	2781	2787	rVB8	2589	2881	0.38%	0.050%
57	10.014	2787	2791	2794	rBV7	2360	1894	0.25%	0.033%
58	10.098	2814	2817	2818	rBV3	1779	970	0.13%	0.017%
59	10.159	2825	2836	2851	rBV	236149	378269	49.61%	6.533%
60	10.416	2913	2916	2918	rBV4	1987	1006	0.13%	0.017%
61	10.561	2959	2961	2968	rVB8	1573	1573	0.21%	0.027%
62	10.599	2968	2973	2976	rBV6	1772	1783	0.23%	0.031%
63	10.622	2976	2980	2981	rBV3	1786	1437	0.19%	0.025%
64	10.731	3010	3014	3015	rBV4	1677	1041	0.14%	0.018%
65	10.841	3045	3048	3052	rBV5	1223	1194	0.16%	0.021%
66	10.860	3052	3054	3057	rBV4	2097	1322	0.17%	0.023%
67	10.998	3093	3097	3103	rVB10	2046	1935	0.25%	0.033%
68	11.043	3109	3111	3114	rBV4	1884	1483	0.19%	0.026%
69	11.191	3146	3157	3173	rBV	318806	513230	67.31%	8.864%
70	11.288	3183	3187	3189	rBV5	2014	1330	0.17%	0.023%
71	11.567	3262	3274	3291	rBV	337796	550303	72.18%	9.505%
72	11.866	3365	3367	3370	rBV4	1832	923	0.12%	0.016%
73	12.140	3449	3452	3454	rBV4	1996	1043	0.14%	0.018%
74	12.294	3496	3500	3502	rBV5	2531	1725	0.23%	0.030%
75	12.503	3562	3565	3568	rVB5	1208	777	0.10%	0.013%
76	12.525	3568	3572	3575	rVB4	2411	1658	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031206.D
 Acq On : 24 May 2023 11:30
 Operator : SY/MD
 Sample : VV0524WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK344

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.545	3575	3578	3580	rBV4	1881	1182	0.16%	0.020%
78	12.577	3585	3588	3591	rBV5	1525	1208	0.16%	0.021%
79	12.731	3633	3636	3640	rVB6	2035	1477	0.19%	0.026%
80	12.805	3656	3659	3662	rBV6	2049	1405	0.18%	0.024%
81	12.889	3682	3685	3687	rBV4	1628	937	0.12%	0.016%
82	12.947	3700	3703	3705	rBV4	1430	957	0.13%	0.017%
83	13.130	3755	3760	3761	rBV3	1921	1458	0.19%	0.025%
84	13.159	3766	3769	3770	rBV2	1974	858	0.11%	0.015%
85	13.201	3778	3782	3783	rBV4	2551	1899	0.25%	0.033%
86	13.352	3827	3829	3832	rVB3	1484	686	0.09%	0.012%
87	13.374	3834	3836	3838	rBV3	1260	791	0.10%	0.014%
88	13.429	3851	3853	3854	rBV2	1866	823	0.11%	0.014%
89	13.792	3962	3966	3969	rBV5	2052	1508	0.20%	0.026%
90	13.847	3980	3983	3985	rBV4	2032	1349	0.18%	0.023%
91	13.927	4006	4008	4012	rBV5	1299	1044	0.14%	0.018%
92	14.140	4072	4074	4077	rBV4	1749	1077	0.14%	0.019%
93	14.172	4081	4084	4085	rBV3	1457	893	0.12%	0.015%
94	14.406	4153	4157	4158	rBV3	1490	742	0.10%	0.013%
95	14.426	4158	4163	4167	rVV8	1703	1751	0.23%	0.030%
96	14.516	4188	4191	4192	rBV3	1801	1167	0.15%	0.020%
97	14.766	4265	4269	4270	rBV3	1694	944	0.12%	0.016%
98	15.156	4388	4390	4394	rVB4	1684	838	0.11%	0.014%
99	15.223	4408	4411	4414	rBV4	2198	1756	0.23%	0.030%
100	15.374	4456	4458	4462	rBV5	1953	938	0.12%	0.016%




Sum of corrected areas: 5789829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031206.D
Acq On : 24 May 2023 11:30
Operator : SY/MD
Sample : VV0524WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK344

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

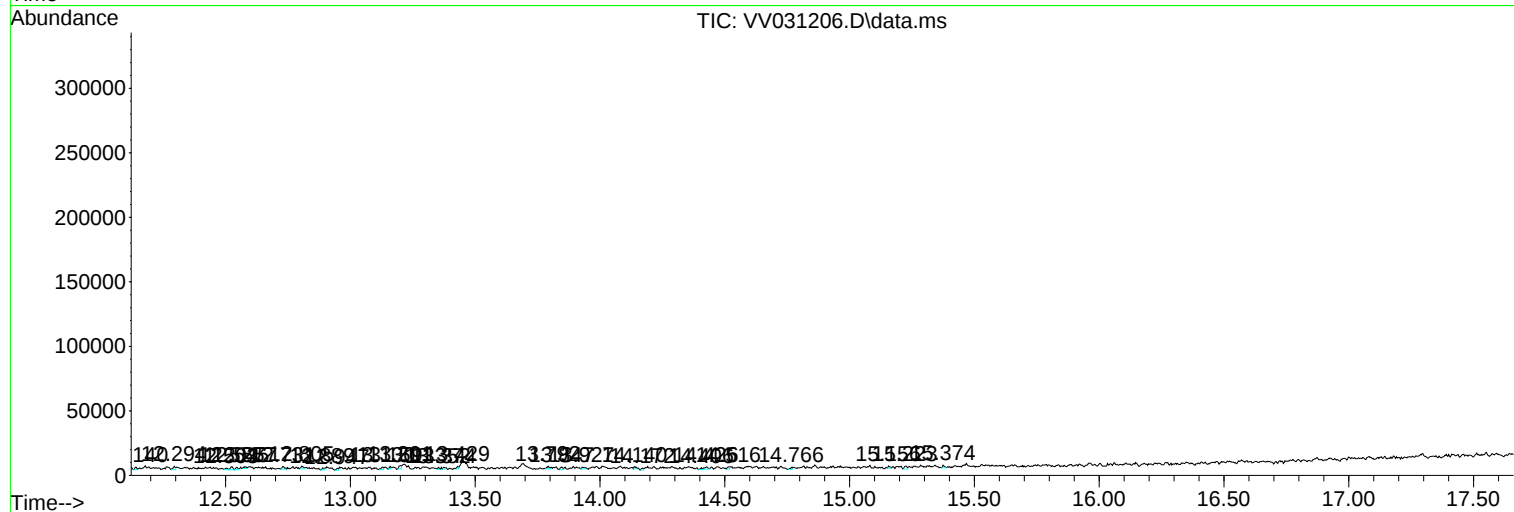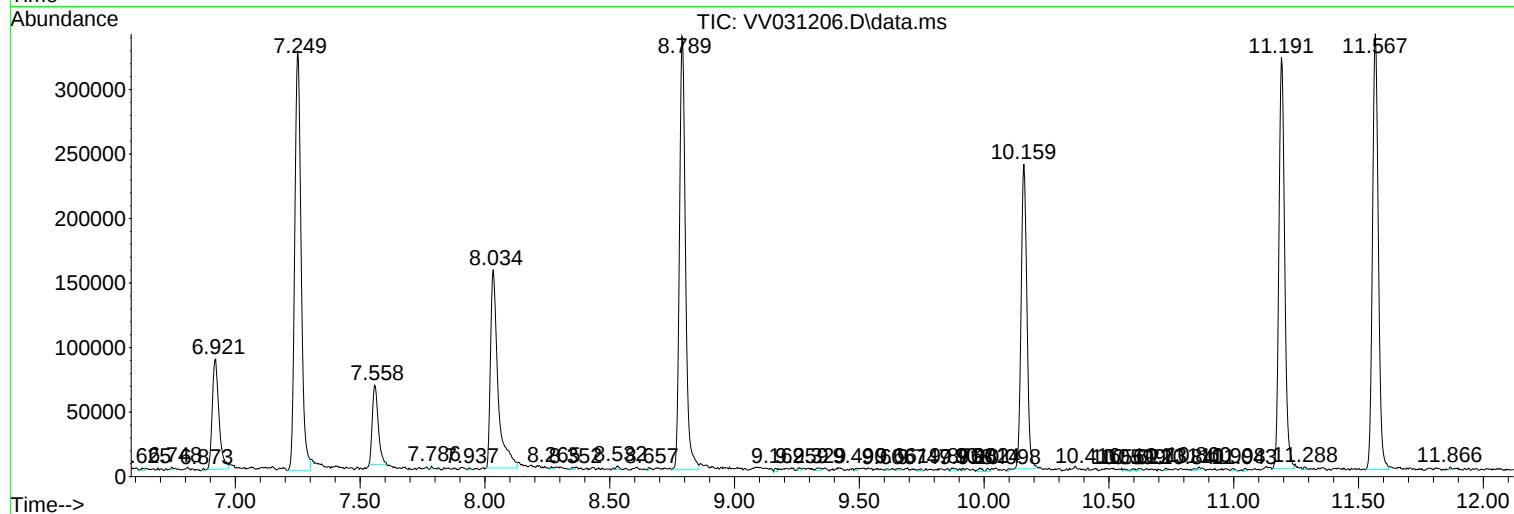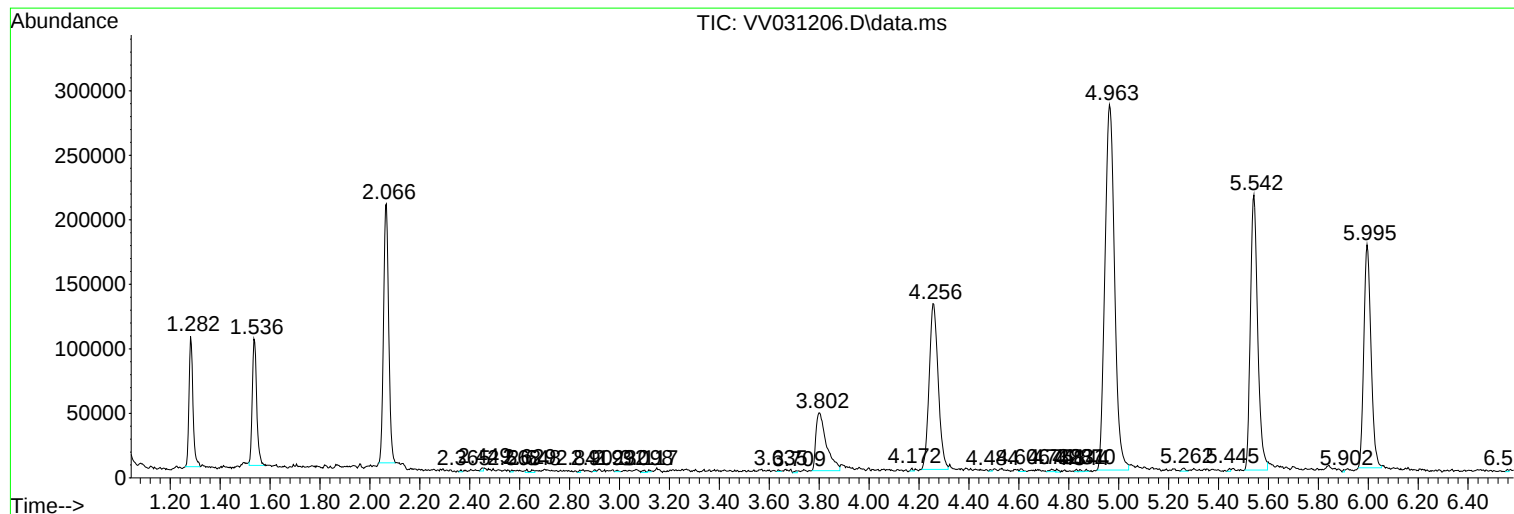

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031206.D
Acq On : 24 May 2023 11:30
Operator : SY/MD
Sample : VV0524WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK344

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031206.D
Acq On : 24 May 2023 11:30
Operator : SY/MD
Sample : VV0524WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK344

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------