

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031208.D
 Acq On : 24 May 2023 12:23
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	60	rBV9	2832	3046	0.41%	0.051%
2	1.285	70	76	84	rBV	93713	96224	12.93%	1.601%
3	1.536	148	154	168	rVB	99709	119933	16.12%	1.996%
4	2.066	309	319	331	rBV	194037	288267	38.75%	4.797%
5	2.519	458	460	462	rVB3	1846	894	0.12%	0.015%
6	2.542	462	467	471	rBV8	1753	1842	0.25%	0.031%
7	2.571	473	476	479	rBV5	1822	1544	0.21%	0.026%
8	2.635	494	496	499	rBV3	1582	943	0.13%	0.016%
9	2.651	499	501	502	rBV2	1238	433	0.06%	0.007%
10	2.700	512	516	519	rBV5	1462	1466	0.20%	0.024%
11	2.761	533	535	538	rVB4	1799	888	0.12%	0.015%
12	2.944	589	592	593	rBV3	1732	719	0.10%	0.012%
13	2.976	600	602	604	rVB3	1594	644	0.09%	0.011%
14	3.172	661	663	666	rBV4	1246	1036	0.14%	0.017%
15	3.214	673	676	679	rBV5	1980	1466	0.20%	0.024%
16	3.249	685	687	690	rBV4	2165	1416	0.19%	0.024%
17	3.304	701	704	706	rBV3	2453	1367	0.18%	0.023%
18	3.494	761	763	765	rVB2	1524	445	0.06%	0.007%
19	3.507	765	767	770	rBV4	1228	584	0.08%	0.010%
20	3.564	783	785	789	rVB6	1601	619	0.08%	0.010%
21	3.626	802	804	807	rVB4	1734	862	0.12%	0.014%
22	3.741	839	840	842	rBV2	1303	532	0.07%	0.009%
23	3.754	842	844	848	rVB4	1744	1158	0.16%	0.019%
24	3.802	849	859	879	rBV2	44758	127191	17.10%	2.117%
25	4.166	968	972	973	rBV4	1782	990	0.13%	0.016%
26	4.259	989	1001	1023	rVB	124352	310877	41.79%	5.173%
27	4.571	1097	1098	1099	rBV	1962	709	0.10%	0.012%
28	4.786	1164	1165	1167	rBV2	1321	543	0.07%	0.009%
29	4.828	1175	1178	1179	rBV3	1315	631	0.08%	0.011%
30	4.857	1185	1187	1189	rBV3	1376	749	0.10%	0.012%
31	4.963	1205	1220	1243	rBV3	279932	743942	100.00%	12.380%
32	5.542	1387	1400	1420	rBV	230279	479332	64.43%	7.977%
33	5.786	1474	1476	1478	rBV3	1914	708	0.10%	0.012%
34	5.841	1484	1493	1510	rVB2	94549	182434	24.52%	3.036%
35	5.995	1530	1541	1562	rBV3	163711	334303	44.94%	5.563%
36	6.561	1711	1717	1721	rBV9	2456	2940	0.40%	0.049%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031208.D
 Acq On : 24 May 2023 12:23
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.667	1748	1750	1753	rVB4	1903	957	0.13%	0.016%
38	6.754	1775	1777	1781	rVB4	1880	1082	0.15%	0.018%
39	6.918	1818	1828	1846	rBV	82389	157380	21.15%	2.619%
40	7.195	1909	1914	1916	rBV5	2117	2235	0.30%	0.037%
41	7.249	1921	1931	1950	rVV	311701	551805	74.17%	9.183%
42	7.558	2016	2027	2040	rBV2	64277	115559	15.53%	1.923%
43	7.686	2064	2067	2068	rBV2	2095	998	0.13%	0.017%
44	8.034	2165	2175	2203	rBV	144813	310887	41.79%	5.173%
45	8.490	2316	2317	2321	rVB4	1810	909	0.12%	0.015%
46	8.519	2321	2326	2328	rBV6	2050	2002	0.27%	0.033%
47	8.789	2397	2410	2428	rBV	357672	611477	82.19%	10.176%
48	9.047	2486	2490	2491	rBV3	1283	860	0.12%	0.014%
49	9.419	2604	2606	2608	rBV2	1525	1009	0.14%	0.017%
50	9.490	2626	2628	2629	rBV2	1519	643	0.09%	0.011%
51	9.770	2712	2715	2720	rVB6	2663	1977	0.27%	0.033%
52	9.796	2720	2723	2725	rBV4	1370	922	0.12%	0.015%
53	9.837	2732	2736	2739	rBV6	1129	1148	0.15%	0.019%
54	9.870	2744	2746	2747	rBV2	1697	581	0.08%	0.010%
55	9.950	2769	2771	2772	rBV3	1449	445	0.06%	0.007%
56	9.969	2775	2777	2780	rVB3	1550	716	0.10%	0.012%
57	9.985	2780	2782	2783	rBV	1375	624	0.08%	0.010%
58	10.059	2803	2805	2807	rBV3	2042	1104	0.15%	0.018%
59	10.159	2825	2836	2851	rBV	230554	371535	49.94%	6.183%
60	10.333	2883	2890	2900	rVB3	9186	16212	2.18%	0.270%
61	10.519	2945	2948	2949	rBV3	1389	635	0.09%	0.011%
62	10.683	2997	2999	3001	rVB3	1666	591	0.08%	0.010%
63	10.712	3007	3008	3009	rBV	2067	444	0.06%	0.007%
64	10.799	3033	3035	3037	rBV3	1619	865	0.12%	0.014%
65	10.989	3090	3094	3096	rBV4	1983	1737	0.23%	0.029%
66	11.124	3133	3136	3140	rBV5	2437	2055	0.28%	0.034%
67	11.191	3147	3157	3177	rVB	350526	559340	75.19%	9.308%
68	11.371	3211	3213	3214	rBV2	1574	614	0.08%	0.010%
69	11.567	3264	3274	3289	rVB	339243	538271	72.35%	8.957%
70	11.680	3306	3309	3313	rBV6	2549	2302	0.31%	0.038%
71	11.908	3377	3380	3382	rBV4	2096	1357	0.18%	0.023%
72	12.133	3447	3450	3451	rBV3	1771	870	0.12%	0.014%
73	12.185	3461	3466	3468	rBV6	2529	2543	0.34%	0.042%
74	12.271	3491	3493	3496	rVB4	1657	804	0.11%	0.013%
75	12.329	3509	3511	3513	rBV3	1584	919	0.12%	0.015%
76	12.368	3518	3523	3527	rBV7	1753	2316	0.31%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031208.D
 Acq On : 24 May 2023 12:23
 Operator : SY/MD
 Sample : 02866-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.570	3582	3586	3588	rBV5	2821	2083	0.28%	0.035%
78	12.696	3623	3625	3629	rVB5	1662	785	0.11%	0.013%
79	12.866	3675	3678	3682	rBV6	1922	1158	0.16%	0.019%
80	12.902	3687	3689	3692	rBV4	1953	1158	0.16%	0.019%
81	13.079	3742	3744	3746	rBV3	1964	1192	0.16%	0.020%
82	13.159	3767	3769	3771	rBV3	1351	507	0.07%	0.008%
83	13.201	3780	3782	3784	rBV3	1949	898	0.12%	0.015%
84	13.259	3795	3800	3801	rBV6	2338	1907	0.26%	0.032%
85	13.297	3810	3812	3814	rBV3	1459	677	0.09%	0.011%
86	13.316	3816	3818	3820	rVV3	1769	628	0.08%	0.010%
87	13.339	3824	3825	3826	rBV	1970	717	0.10%	0.012%
88	13.567	3894	3896	3898	rVB3	2000	852	0.11%	0.014%
89	13.587	3901	3902	3904	rBV2	1130	634	0.09%	0.011%
90	13.673	3926	3929	3931	rBV4	2321	1624	0.22%	0.027%
91	13.808	3968	3971	3972	rBV3	1461	772	0.10%	0.013%
92	13.828	3975	3977	3984	rVB8	1902	1534	0.21%	0.026%
93	13.860	3984	3987	3990	rBV5	2283	2089	0.28%	0.035%
94	13.934	4008	4010	4014	rBV5	2212	1595	0.21%	0.027%
95	14.037	4039	4042	4043	rBV3	1435	920	0.12%	0.015%
96	14.162	4079	4081	4082	rBV2	1486	551	0.07%	0.009%
97	14.230	4099	4102	4103	rBV3	1315	783	0.11%	0.013%
98	14.313	4126	4128	4132	rBV5	2028	1146	0.15%	0.019%
99	14.477	4176	4179	4182	rBV5	2051	1985	0.27%	0.033%
100	15.287	4427	4431	4433	rBV4	3100	2692	0.36%	0.045%




Sum of corrected areas: 6009294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031208.D
Acq On : 24 May 2023 12:23
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

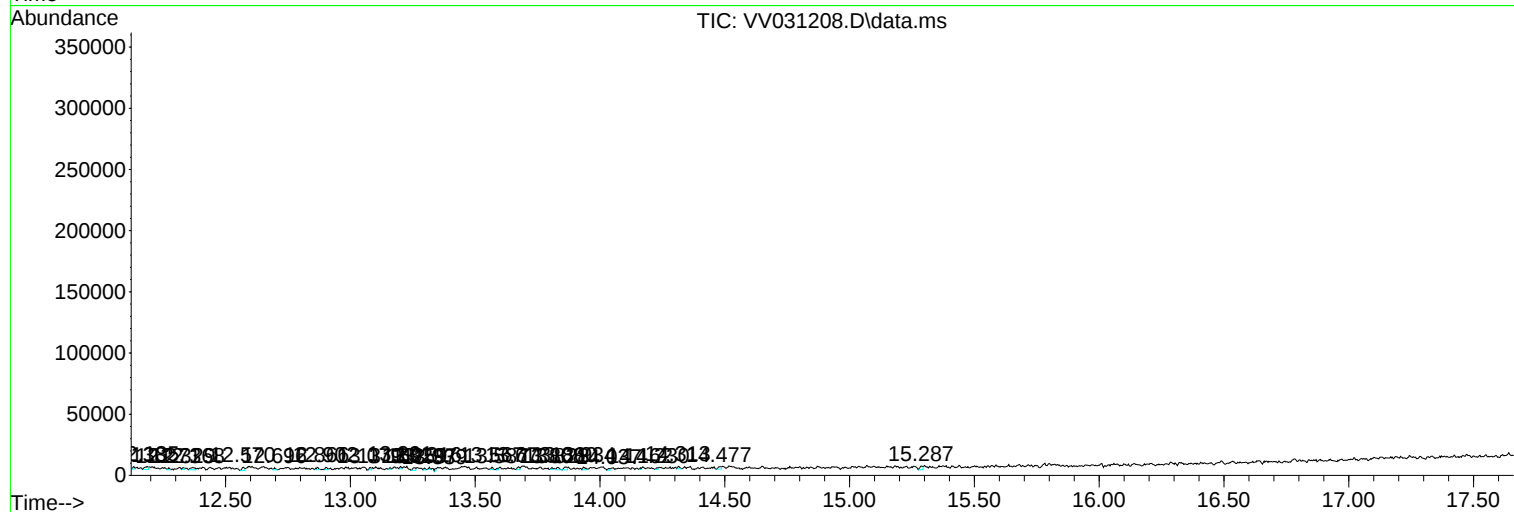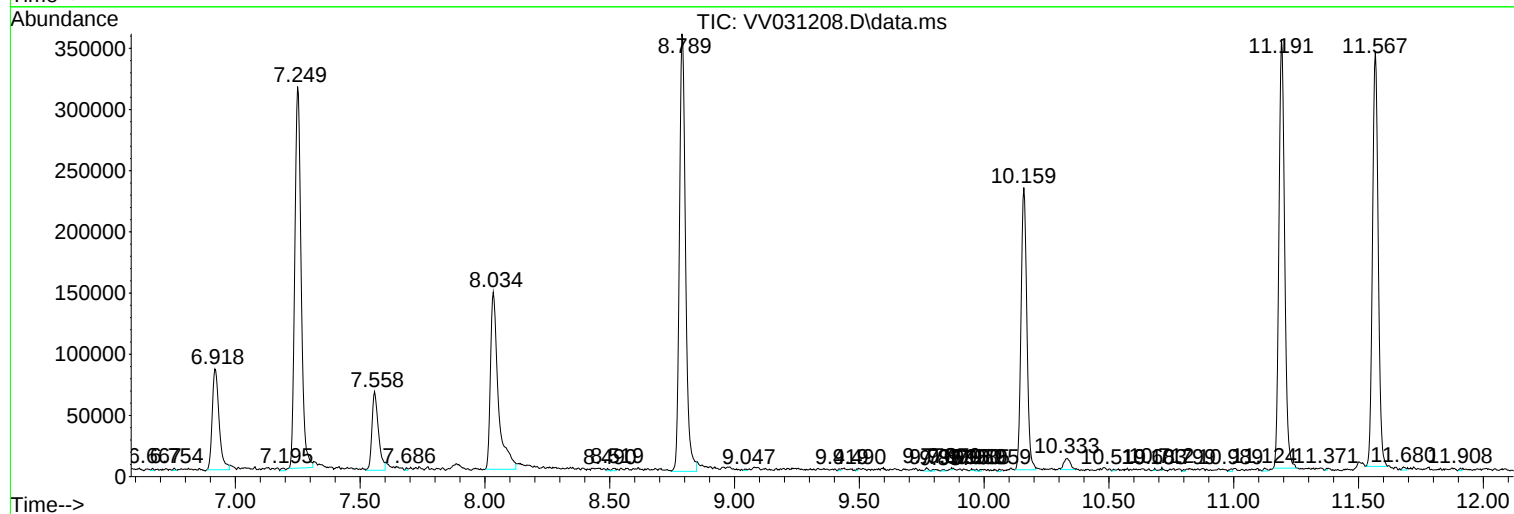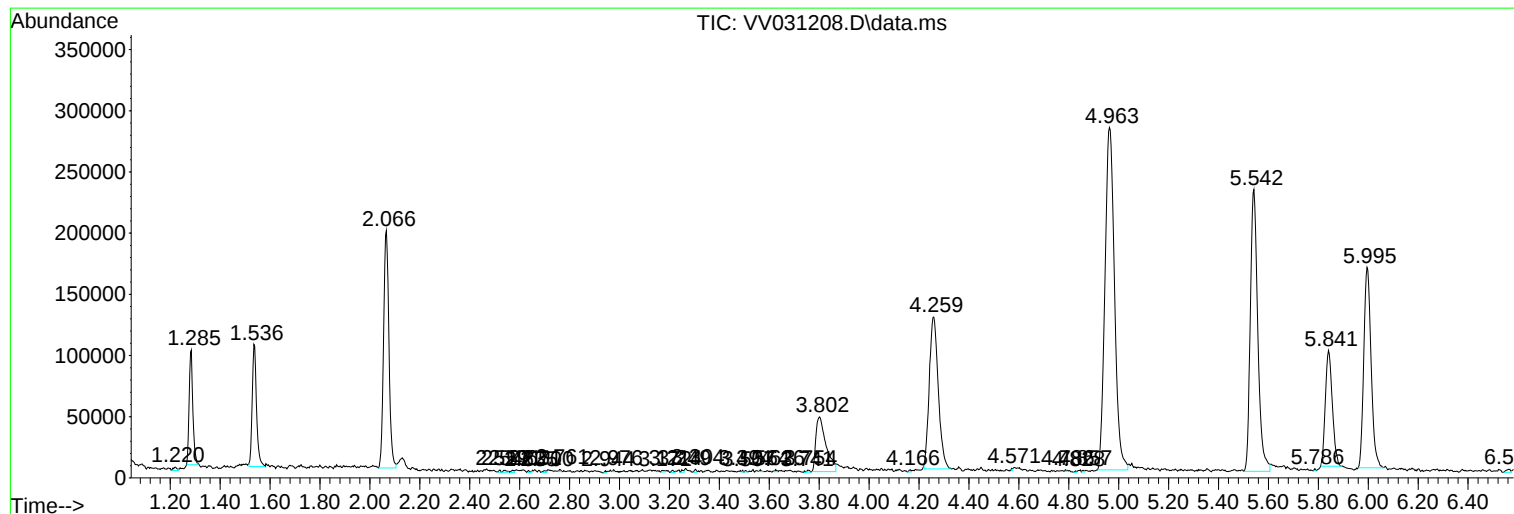

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031208.D
Acq On : 24 May 2023 12:23
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031208.D
Acq On : 24 May 2023 12:23
Operator : SY/MD
Sample : 02866-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------