

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031209.D
 Acq On : 24 May 2023 12:47
 Operator : SY/MD
 Sample : 02865-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

Signal : TIC: VV031209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	88	rVB	96416	105455	13.88%	1.854%
2	1.535	148	154	167	rVB	103380	121829	16.03%	2.142%
3	2.066	310	319	331	rBV	191498	276576	36.40%	4.862%
4	2.561	471	473	474	rBV2	1223	461	0.06%	0.008%
5	2.744	528	530	535	rBV6	864	731	0.10%	0.013%
6	2.889	571	575	578	rBV6	1702	1386	0.18%	0.024%
7	2.918	583	584	585	rBV	1087	357	0.05%	0.006%
8	3.069	628	631	634	rBV5	2134	1480	0.19%	0.026%
9	3.134	648	651	653	rBV4	1695	1214	0.16%	0.021%
10	3.195	667	670	671	rBV3	1090	536	0.07%	0.009%
11	3.301	702	703	705	rBV2	1123	379	0.05%	0.007%
12	3.481	757	759	761	rBV3	1104	607	0.08%	0.011%
13	3.506	765	767	769	rBV3	1285	634	0.08%	0.011%
14	3.571	781	787	788	rBV5	1160	959	0.13%	0.017%
15	3.603	793	797	798	rBV4	1477	1014	0.13%	0.018%
16	3.661	813	815	818	rBV4	1086	587	0.08%	0.010%
17	3.677	818	820	823	rBV4	1834	1435	0.19%	0.025%
18	3.725	833	835	838	rVB4	1683	902	0.12%	0.016%
19	3.741	838	840	842	rBV3	1378	878	0.12%	0.015%
20	3.799	849	858	880	rBV	46534	131599	17.32%	2.313%
21	4.114	954	956	957	rBV2	1314	430	0.06%	0.008%
22	4.259	989	1001	1022	rVB2	124247	307232	40.44%	5.401%
23	4.580	1099	1101	1103	rBV3	1531	840	0.11%	0.015%
24	4.651	1121	1123	1125	rBV2	1752	857	0.11%	0.015%
25	4.693	1132	1136	1137	rBV4	1277	652	0.09%	0.011%
26	4.706	1137	1140	1141	rBV3	1620	1051	0.14%	0.018%
27	4.735	1146	1149	1151	rBV4	2144	1553	0.20%	0.027%
28	4.879	1187	1194	1196	rBV7	1952	1939	0.26%	0.034%
29	4.963	1203	1220	1251	rBV2	280318	759781	100.00%	13.356%
30	5.339	1335	1337	1339	rBV3	1849	1101	0.14%	0.019%
31	5.381	1348	1350	1352	rBV3	1190	552	0.07%	0.010%
32	5.542	1389	1400	1420	rBV	213215	437062	57.52%	7.683%
33	5.995	1530	1541	1562	rBV2	163878	338982	44.62%	5.959%
34	6.484	1691	1693	1694	rBV2	1237	539	0.07%	0.009%
35	6.619	1732	1735	1737	rBV4	1542	1095	0.14%	0.019%
36	6.651	1742	1745	1746	rBV2	1357	698	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031209.D
 Acq On : 24 May 2023 12:47
 Operator : SY/MD
 Sample : 02865-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.918	1819	1828	1846	rBV	83014	159820	21.04%	2.809%
38	7.249	1921	1931	1946	rBV	310886	540519	71.14%	9.501%
39	7.558	2019	2027	2044	rBV	61744	113613	14.95%	1.997%
40	7.982	2157	2159	2161	rBV3	1439	799	0.11%	0.014%
41	8.034	2166	2175	2203	rVV	148441	315332	41.50%	5.543%
42	8.329	2265	2267	2269	rBV3	1850	972	0.13%	0.017%
43	8.352	2272	2274	2275	rBV2	2091	649	0.09%	0.011%
44	8.384	2282	2284	2286	rBV2	2481	1622	0.21%	0.029%
45	8.677	2373	2375	2379	rVB5	1985	1271	0.17%	0.022%
46	8.702	2379	2383	2385	rBV4	2127	1664	0.22%	0.029%
47	8.792	2400	2411	2426	rBV	338185	562487	74.03%	9.888%
48	8.998	2473	2475	2477	rBV3	2295	1332	0.18%	0.023%
49	9.169	2526	2528	2529	rBV2	1294	434	0.06%	0.008%
50	9.339	2579	2581	2583	rBV3	1454	794	0.10%	0.014%
51	9.400	2598	2600	2603	rBV4	1352	746	0.10%	0.013%
52	9.481	2621	2625	2631	rBV7	3272	4524	0.60%	0.080%
53	10.091	2813	2815	2816	rBV2	1299	401	0.05%	0.007%
54	10.159	2824	2836	2850	rBV	239206	376143	49.51%	6.612%
55	10.300	2877	2880	2881	rBV3	1279	789	0.10%	0.014%
56	10.452	2925	2927	2929	rBV3	1452	936	0.12%	0.016%
57	10.847	3045	3050	3051	rBV4	2874	2677	0.35%	0.047%
58	10.918	3070	3072	3076	rVB4	1323	709	0.09%	0.012%
59	10.956	3082	3084	3087	rBV3	1129	674	0.09%	0.012%
60	11.191	3145	3157	3178	rBV	328819	527820	69.47%	9.278%
61	11.339	3199	3203	3207	rVB7	2305	2037	0.27%	0.036%
62	11.378	3207	3215	3217	rBV8	1602	2120	0.28%	0.037%
63	11.567	3264	3274	3289	rVB	332886	522856	68.82%	9.191%
64	11.776	3335	3339	3340	rBV4	1955	1236	0.16%	0.022%
65	11.860	3364	3365	3368	rBV3	1326	588	0.08%	0.010%
66	12.075	3430	3432	3433	rBV2	1027	376	0.05%	0.007%
67	12.172	3457	3462	3465	rBV6	2460	2370	0.31%	0.042%
68	12.207	3471	3473	3475	rBV4	1908	848	0.11%	0.015%
69	12.426	3537	3541	3542	rBV3	1936	1265	0.17%	0.022%
70	12.477	3554	3557	3559	rBV4	2007	1482	0.20%	0.026%
71	12.554	3578	3581	3583	rBV3	1791	1337	0.18%	0.024%
72	12.657	3610	3613	3616	rBV4	1493	908	0.12%	0.016%
73	12.770	3646	3648	3649	rBV2	956	385	0.05%	0.007%
74	12.799	3654	3657	3661	rBV5	2077	1551	0.20%	0.027%
75	12.824	3663	3665	3667	rBV3	2125	1117	0.15%	0.020%
76	12.892	3684	3686	3689	rBV4	1546	947	0.12%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031209.D
 Acq On : 24 May 2023 12:47
 Operator : SY/MD
 Sample : 02865-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.914	3691	3693	3696	rBV3	1424	868	0.11%	0.015%
78	13.004	3718	3721	3724	rBV4	1235	829	0.11%	0.015%
79	13.021	3724	3726	3727	rBV2	1311	642	0.08%	0.011%
80	13.072	3740	3742	3743	rBV2	1967	795	0.10%	0.014%
81	13.143	3760	3764	3768	rBV6	1895	1674	0.22%	0.029%
82	13.287	3806	3809	3811	rVB4	1767	862	0.11%	0.015%
83	13.300	3811	3813	3818	rVB6	2611	1629	0.21%	0.029%
84	13.326	3818	3821	3824	rBV5	1756	1353	0.18%	0.024%
85	13.416	3847	3849	3853	rBV4	2136	1711	0.23%	0.030%
86	13.435	3853	3855	3857	rVV3	1519	630	0.08%	0.011%
87	13.590	3901	3903	3906	rBV3	697	477	0.06%	0.008%
88	13.667	3925	3927	3929	rBV3	1174	595	0.08%	0.010%
89	13.728	3944	3946	3951	rVB6	2622	1964	0.26%	0.035%
90	13.821	3973	3975	3977	rBV3	1276	582	0.08%	0.010%
91	13.869	3986	3990	3994	rBV7	2389	2524	0.33%	0.044%
92	13.892	3995	3997	4000	rVV4	1330	855	0.11%	0.015%
93	14.111	4062	4065	4071	rVB7	2786	2168	0.29%	0.038%
94	14.220	4096	4099	4101	rBV4	1780	1103	0.15%	0.019%
95	14.496	4182	4185	4188	rBV4	1353	1010	0.13%	0.018%
96	14.548	4199	4201	4203	rBV3	2175	1207	0.16%	0.021%
97	14.602	4214	4218	4220	rBV4	1405	1130	0.15%	0.020%
98	14.992	4337	4339	4341	rVB3	1886	704	0.09%	0.012%
99	15.062	4359	4361	4363	rBV2	1149	596	0.08%	0.010%
100	15.622	4533	4535	4537	rBV3	2470	1353	0.18%	0.024%




Sum of corrected areas: 5688794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031209.D
Acq On : 24 May 2023 12:47
Operator : SY/MD
Sample : 02865-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

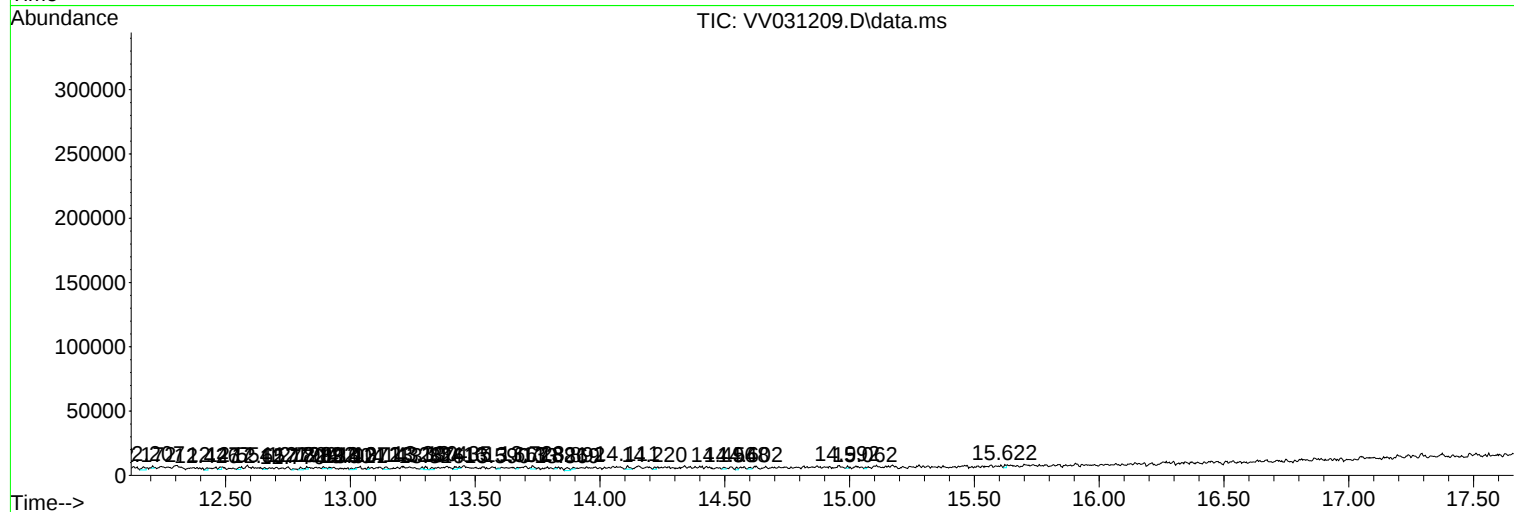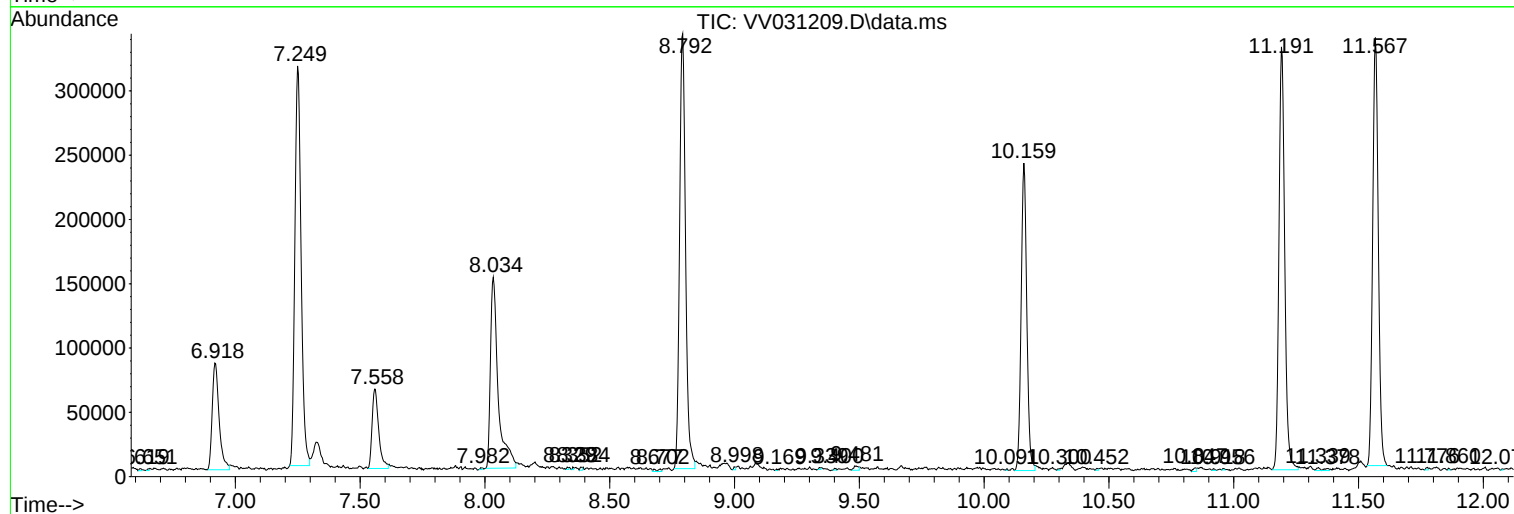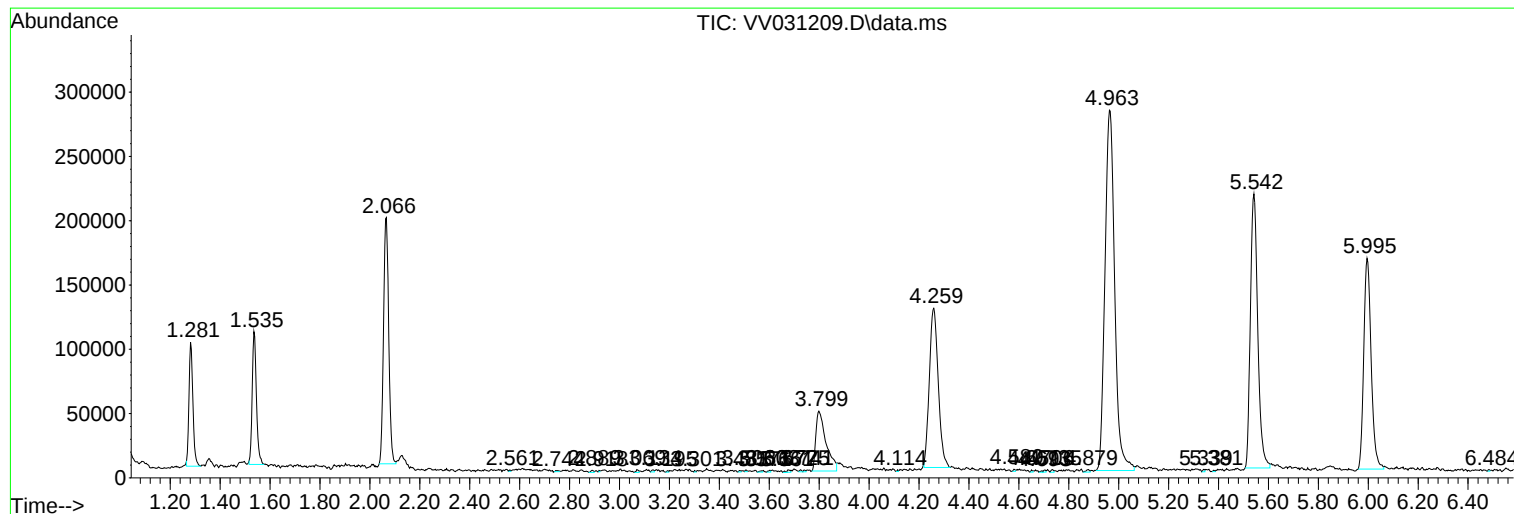

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031209.D
Acq On : 24 May 2023 12:47
Operator : SY/MD
Sample : 02865-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031209.D
Acq On : 24 May 2023 12:47
Operator : SY/MD
Sample : 02865-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc