

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031216.D
 Acq On : 24 May 2023 15:34
 Operator : SY/MD
 Sample : 02865-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	84	rBV	91896	100061	13.62%	1.699%
2	1.539	148	155	162	rVB	86001	103119	14.04%	1.750%
3	2.063	309	318	331	rBV	190294	278576	37.93%	4.729%
4	2.426	428	431	433	rBV4	2452	1671	0.23%	0.028%
5	2.494	449	452	455	rBV5	1215	805	0.11%	0.014%
6	2.561	471	473	475	rBV3	1325	773	0.11%	0.013%
7	2.748	529	531	534	rBV4	2258	1503	0.20%	0.026%
8	2.863	564	567	572	rBV7	2060	2304	0.31%	0.039%
9	2.908	579	581	584	rBV4	1852	951	0.13%	0.016%
10	3.034	618	620	621	rBV2	1776	782	0.11%	0.013%
11	3.098	636	640	643	rBV5	1247	1411	0.19%	0.024%
12	3.259	688	690	693	rVB4	1774	1025	0.14%	0.017%
13	3.275	693	695	698	rBV4	1794	764	0.10%	0.013%
14	3.343	712	716	718	rBV5	1360	1287	0.18%	0.022%
15	3.481	754	759	762	rVB6	1620	1395	0.19%	0.024%
16	3.513	766	769	773	rBV5	2116	1747	0.24%	0.030%
17	3.609	796	799	802	rVV4	2215	1240	0.17%	0.021%
18	3.706	827	829	833	rVB5	1187	755	0.10%	0.013%
19	3.732	833	837	840	rBV6	1897	1577	0.21%	0.027%
20	3.802	848	859	885	rBV4	53220	186451	25.38%	3.165%
21	4.130	959	961	966	rVB5	1592	966	0.13%	0.016%
22	4.259	989	1001	1017	rVV2	117190	291793	39.73%	4.953%
23	4.558	1093	1094	1097	rBV3	1574	890	0.12%	0.015%
24	4.641	1117	1120	1121	rBV3	1470	854	0.12%	0.014%
25	4.873	1189	1192	1193	rBV3	2175	1062	0.14%	0.018%
26	4.966	1204	1221	1242	rVV2	275396	734513	100.00%	12.469%
27	5.243	1304	1307	1310	rBV5	1701	1234	0.17%	0.021%
28	5.420	1360	1362	1367	rVV6	1633	1218	0.17%	0.021%
29	5.542	1388	1400	1420	rBV	224298	466471	63.51%	7.919%
30	5.844	1485	1494	1508	rBV2	46455	87848	11.96%	1.491%
31	5.995	1529	1541	1562	rBV	169235	341851	46.54%	5.803%
32	6.217	1608	1610	1613	rBV4	1432	1056	0.14%	0.018%
33	6.342	1644	1649	1652	rVB4	2517	2209	0.30%	0.037%
34	6.365	1652	1656	1659	rBV6	1654	1677	0.23%	0.028%
35	6.654	1741	1746	1748	rBV6	1897	1853	0.25%	0.031%
36	6.719	1761	1766	1767	rBV4	1740	1181	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031216.D
 Acq On : 24 May 2023 15:34
 Operator : SY/MD
 Sample : 02865-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.825	1793	1799	1800	rBV6	1354	1376	0.19%	0.023%
38	6.921	1820	1829	1845	rBV	79118	143630	19.55%	2.438%
39	7.194	1912	1914	1919	rBV6	1423	1434	0.20%	0.024%
40	7.252	1921	1932	1951	rVV	308185	550042	74.89%	9.337%
41	7.503	2008	2010	2012	rBV3	1998	814	0.11%	0.014%
42	7.561	2020	2028	2042	rBV	59273	100075	13.62%	1.699%
43	7.969	2153	2155	2158	rVB3	2366	1411	0.19%	0.024%
44	7.992	2158	2162	2163	rBV3	1507	1128	0.15%	0.019%
45	8.034	2166	2175	2208	rVV	156818	333698	45.43%	5.665%
46	8.436	2297	2300	2304	rBV7	2162	1574	0.21%	0.027%
47	8.542	2331	2333	2336	rVB4	1758	910	0.12%	0.015%
48	8.558	2336	2338	2343	rBV6	1841	1930	0.26%	0.033%
49	8.680	2373	2376	2379	rBV5	2069	1551	0.21%	0.026%
50	8.792	2400	2411	2429	rBV	362602	585321	79.69%	9.936%
51	9.452	2612	2616	2619	rBV5	1747	1635	0.22%	0.028%
52	9.526	2636	2639	2642	rBV5	1745	1212	0.17%	0.021%
53	9.664	2680	2682	2685	rBV4	1727	1025	0.14%	0.017%
54	9.712	2694	2697	2698	rBV3	1851	1024	0.14%	0.017%
55	9.731	2700	2703	2705	rBV4	1851	1164	0.16%	0.020%
56	10.024	2791	2794	2797	rVB5	1899	1026	0.14%	0.017%
57	10.095	2813	2816	2817	rBV3	1643	747	0.10%	0.013%
58	10.159	2826	2836	2853	rVB	233284	370742	50.47%	6.293%
59	10.329	2882	2889	2891	rBV7	4871	5991	0.82%	0.102%
60	10.455	2926	2928	2932	rVB4	2258	1425	0.19%	0.024%
61	10.490	2933	2939	2942	rBV6	2147	2372	0.32%	0.040%
62	10.525	2946	2950	2955	rBV8	2474	2721	0.37%	0.046%
63	10.616	2974	2978	2980	rBV5	1952	1254	0.17%	0.021%
64	10.661	2989	2992	2997	rBV5	2008	2381	0.32%	0.040%
65	10.689	2997	3001	3004	rVV6	1871	1703	0.23%	0.029%
66	10.715	3004	3009	3010	rVV5	1375	905	0.12%	0.015%
67	10.731	3013	3014	3021	rVB6	1772	1373	0.19%	0.023%
68	10.773	3024	3027	3029	rBV3	1727	1005	0.14%	0.017%
69	10.921	3070	3073	3074	rBV3	2052	1060	0.14%	0.018%
70	11.191	3147	3157	3176	rBV	352132	559785	76.21%	9.503%
71	11.381	3213	3216	3217	rBV3	1478	802	0.11%	0.014%
72	11.468	3241	3243	3245	rBV3	1486	838	0.11%	0.014%
73	11.567	3263	3274	3292	rBV	338935	541050	73.66%	9.185%
74	11.882	3368	3372	3376	rBV6	1849	1562	0.21%	0.027%
75	11.992	3404	3406	3409	rVB4	2152	1178	0.16%	0.020%
76	12.017	3409	3414	3417	rBV7	2115	1993	0.27%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031216.D
 Acq On : 24 May 2023 15:34
 Operator : SY/MD
 Sample : 02865-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.098	3435	3439	3440	rVB4	1809	1152	0.16%	0.020%
78	12.236	3480	3482	3486	rBV4	1518	886	0.12%	0.015%
79	12.307	3500	3504	3506	rBV4	1798	1354	0.18%	0.023%
80	12.432	3540	3543	3548	rBV6	2269	1814	0.25%	0.031%
81	12.458	3549	3551	3556	rVB5	1720	1440	0.20%	0.024%
82	12.519	3567	3570	3572	rBV4	1589	1277	0.17%	0.022%
83	12.577	3583	3588	3590	rBV5	2270	1669	0.23%	0.028%
84	12.712	3627	3630	3636	rBV8	2355	2578	0.35%	0.044%
85	12.786	3647	3653	3655	rBV7	1670	1671	0.23%	0.028%
86	12.940	3698	3701	3704	rBV4	1917	1720	0.23%	0.029%
87	13.040	3729	3732	3734	rBV4	1791	1303	0.18%	0.022%
88	13.127	3754	3759	3760	rBV4	1511	1062	0.14%	0.018%
89	13.416	3846	3849	3853	rBV5	1203	1029	0.14%	0.017%
90	13.564	3893	3895	3901	rVB6	1968	1786	0.24%	0.030%
91	13.738	3944	3949	3950	rBV5	2225	1280	0.17%	0.022%
92	13.898	3994	3999	4001	rBV7	1874	1586	0.22%	0.027%
93	14.011	4031	4034	4035	rBV3	1473	912	0.12%	0.015%
94	14.143	4072	4075	4077	rBV4	1973	984	0.13%	0.017%
95	14.500	4183	4186	4188	rBV4	2311	1227	0.17%	0.021%
96	14.686	4242	4244	4246	rBV3	1805	1073	0.15%	0.018%
97	14.783	4272	4274	4278	rBV4	1766	1321	0.18%	0.022%
98	14.985	4334	4337	4340	rBV5	1965	1654	0.23%	0.028%
99	15.053	4356	4358	4363	rBV6	1784	1521	0.21%	0.026%
100	15.377	4457	4459	4461	rBV3	1743	840	0.11%	0.014%




Sum of corrected areas: 5890879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031216.D
Acq On : 24 May 2023 15:34
Operator : SY/MD
Sample : 02865-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

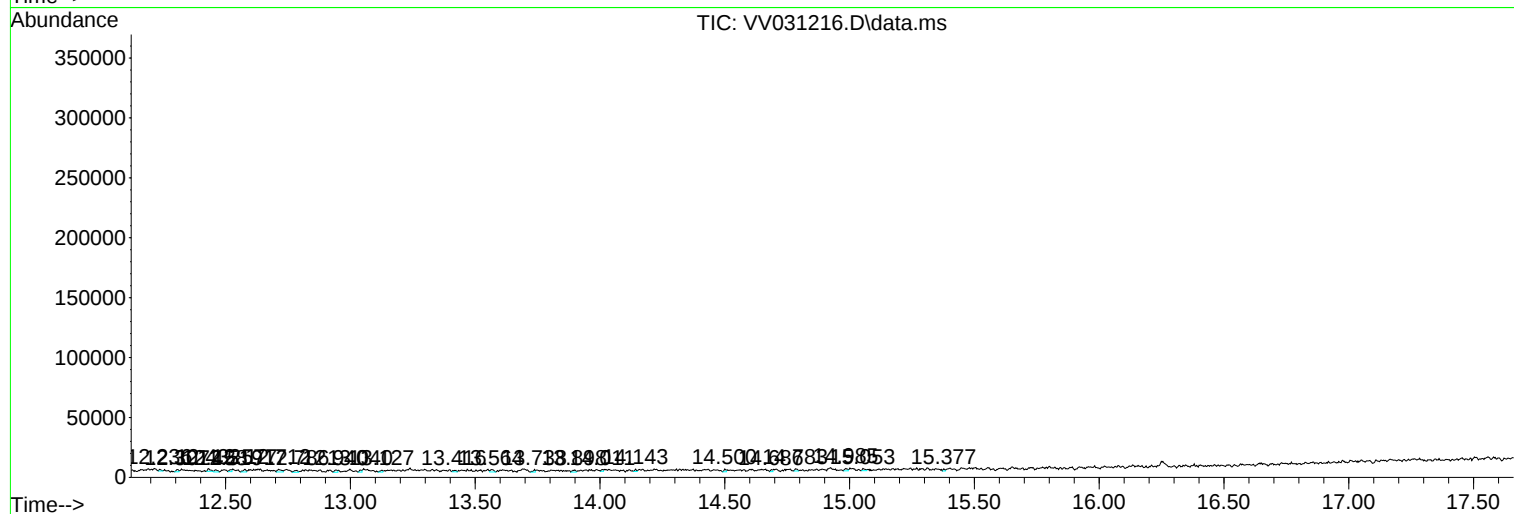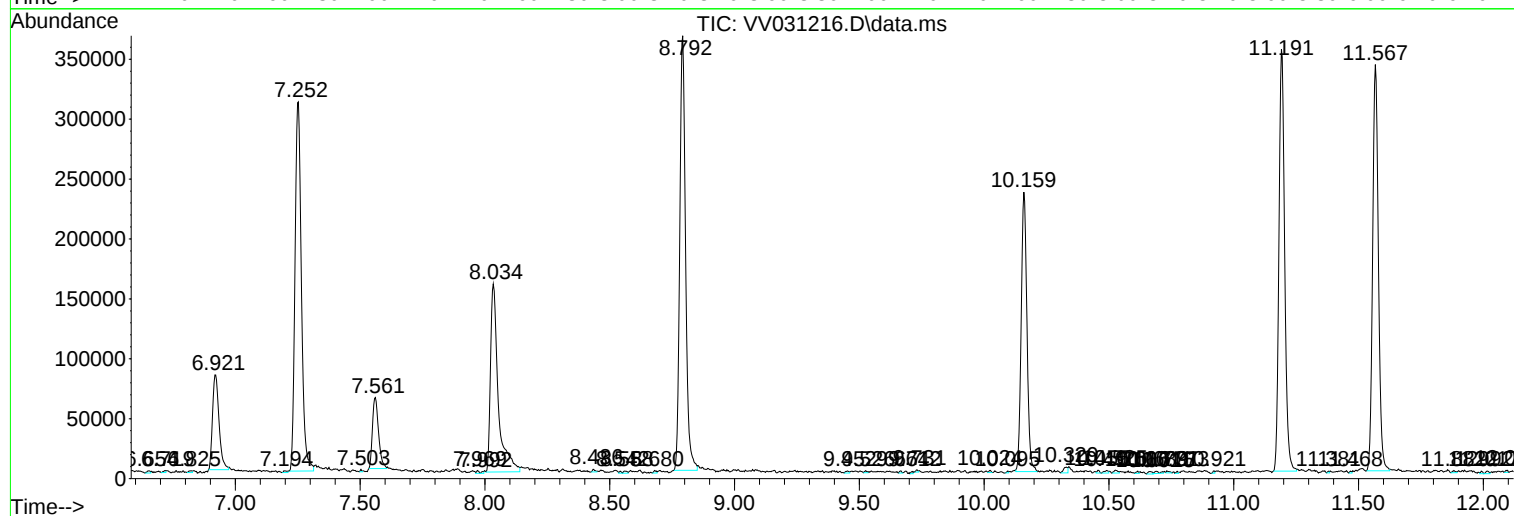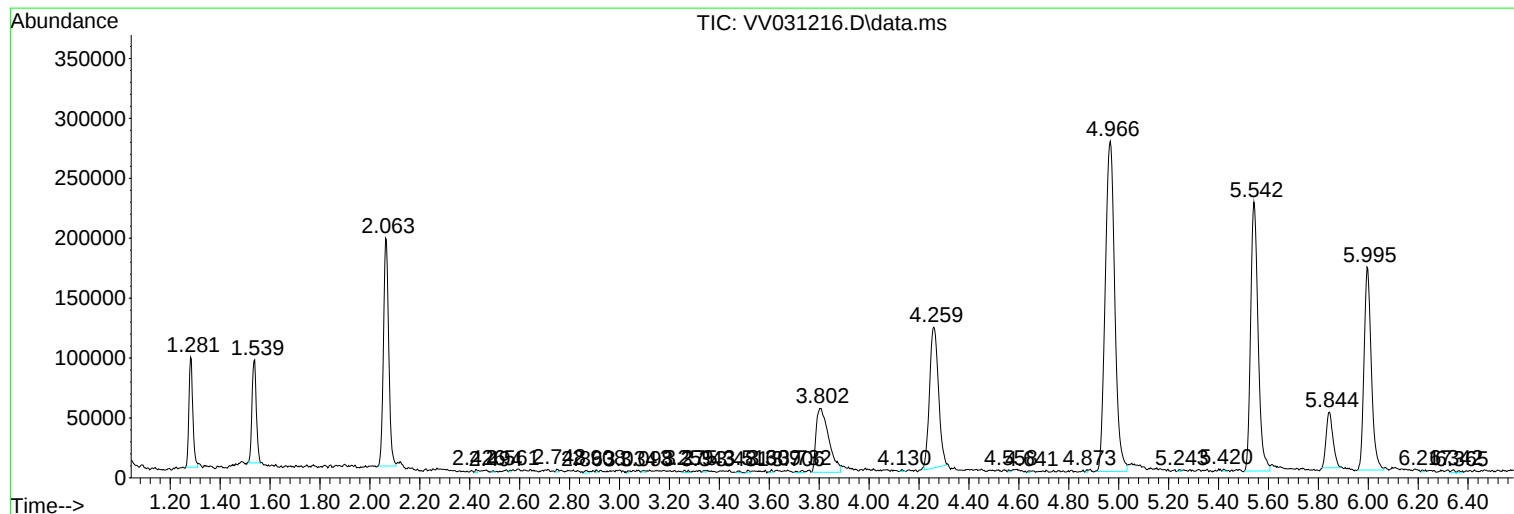

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031216.D
Acq On : 24 May 2023 15:34
Operator : SY/MD
Sample : 02865-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031216.D
Acq On : 24 May 2023 15:34
Operator : SY/MD
Sample : 02865-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc