

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031224.D
 Acq On : 24 May 2023 18:45
 Operator : SY/MD
 Sample : 02866-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	88	rVB	85561	92252	13.31%	1.669%
2	1.536	148	154	166	rVB	83381	99413	14.34%	1.799%
3	2.063	310	318	331	rVB	179313	255535	36.86%	4.624%
4	2.667	501	506	508	rBV6	2089	1962	0.28%	0.036%
5	2.761	533	535	539	rVB5	2759	1552	0.22%	0.028%
6	2.793	539	545	548	rBV6	1663	1829	0.26%	0.033%
7	2.957	592	596	597	rBV4	1765	1259	0.18%	0.023%
8	3.024	612	617	619	rBV5	2204	1616	0.23%	0.029%
9	3.246	680	686	690	rBV8	2173	2740	0.40%	0.050%
10	3.333	709	713	715	rBV5	974	867	0.13%	0.016%
11	3.381	725	728	731	rBV5	2019	1454	0.21%	0.026%
12	3.426	739	742	746	rVB6	2238	1800	0.26%	0.033%
13	3.452	746	750	751	rBV4	1654	1225	0.18%	0.022%
14	3.532	773	775	776	rBV2	1559	696	0.10%	0.013%
15	3.568	783	786	790	rVB6	2187	1545	0.22%	0.028%
16	3.587	790	792	793	rBV2	1138	544	0.08%	0.010%
17	3.741	838	840	844	rVB5	1675	1103	0.16%	0.020%
18	3.767	844	848	849	rBV3	1576	1079	0.16%	0.020%
19	3.799	849	858	880	rBV2	50811	138795	20.02%	2.511%
20	4.092	948	949	953	rVB4	1619	766	0.11%	0.014%
21	4.172	972	974	976	rBV3	1720	859	0.12%	0.016%
22	4.259	989	1001	1024	rVB	116170	290154	41.85%	5.250%
23	4.564	1092	1096	1099	rBV5	1678	1494	0.22%	0.027%
24	4.584	1099	1102	1104	rBV4	1103	632	0.09%	0.011%
25	4.648	1119	1122	1126	rBV5	1921	1452	0.21%	0.026%
26	4.963	1205	1220	1241	rBV3	263014	693244	100.00%	12.544%
27	5.542	1387	1400	1422	rBV	220948	461255	66.54%	8.346%
28	5.809	1481	1483	1487	rBV5	2812	2679	0.39%	0.048%
29	5.995	1531	1541	1562	rVB2	157160	316144	45.60%	5.720%
30	6.339	1646	1648	1653	rVB6	1554	1174	0.17%	0.021%
31	6.497	1692	1697	1700	rBV6	2362	2512	0.36%	0.045%
32	6.719	1764	1766	1768	rBV3	2421	1194	0.17%	0.022%
33	6.850	1801	1807	1810	rBV7	2056	2083	0.30%	0.038%
34	6.918	1819	1828	1842	rBV	77580	141227	20.37%	2.555%
35	7.133	1893	1895	1897	rBV2	1764	1251	0.18%	0.023%
36	7.172	1903	1907	1908	rBV3	1297	769	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031224.D
 Acq On : 24 May 2023 18:45
 Operator : SY/MD
 Sample : 02866-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.188	1911	1912	1915	rBV3	1433	672	0.10%	0.012%
38	7.249	1921	1931	1948	rBV	289853	506790	73.10%	9.170%
39	7.561	2019	2028	2041	rBV	58621	103546	14.94%	1.874%
40	8.034	2166	2175	2209	rBV	156453	328344	47.36%	5.941%
41	8.420	2293	2295	2299	rBV5	2106	1652	0.24%	0.030%
42	8.735	2391	2393	2397	rVB5	2403	1316	0.19%	0.024%
43	8.792	2397	2411	2436	rBV	344388	586629	84.62%	10.615%
44	9.236	2547	2549	2551	rBV3	1162	470	0.07%	0.009%
45	9.410	2600	2603	2606	rBV4	2075	1444	0.21%	0.026%
46	9.442	2611	2613	2615	rVV3	1287	699	0.10%	0.013%
47	9.471	2619	2622	2624	rBV4	2065	1045	0.15%	0.019%
48	9.583	2655	2657	2660	rBV4	1306	824	0.12%	0.015%
49	9.718	2696	2699	2702	rVB5	1607	933	0.13%	0.017%
50	9.863	2742	2744	2747	rBV3	1712	1331	0.19%	0.024%
51	10.030	2793	2796	2802	rVB8	1861	1520	0.22%	0.028%
52	10.095	2814	2816	2818	rBV3	1810	1066	0.15%	0.019%
53	10.159	2826	2836	2852	rBV	226153	356396	51.41%	6.449%
54	10.410	2912	2914	2917	rBV4	1335	786	0.11%	0.014%
55	10.455	2926	2928	2930	rBV3	1234	594	0.09%	0.011%
56	10.538	2951	2954	2955	rBV3	1564	862	0.12%	0.016%
57	10.593	2966	2971	2976	rVB9	1688	1703	0.25%	0.031%
58	10.619	2976	2979	2982	rBV4	1550	1251	0.18%	0.023%
59	10.889	3062	3063	3067	rVB4	1807	854	0.12%	0.015%
60	10.918	3070	3072	3075	rBV4	1822	1370	0.20%	0.025%
61	10.947	3079	3081	3086	rBV6	1658	1323	0.19%	0.024%
62	10.992	3092	3095	3096	rVB3	1408	546	0.08%	0.010%
63	11.079	3119	3122	3124	rBV5	1205	571	0.08%	0.010%
64	11.091	3124	3126	3131	rVB5	2014	964	0.14%	0.017%
65	11.117	3131	3134	3138	rBV5	2789	2505	0.36%	0.045%
66	11.191	3146	3157	3175	rBV	337603	547086	78.92%	9.899%
67	11.484	3246	3248	3249	rBV	1395	558	0.08%	0.010%
68	11.567	3263	3274	3291	rBV	314857	505459	72.91%	9.146%
69	11.776	3337	3339	3342	rBV4	1319	797	0.11%	0.014%
70	11.831	3354	3356	3359	rVB3	1799	837	0.12%	0.015%
71	12.021	3412	3415	3416	rBV3	1737	955	0.14%	0.017%
72	12.223	3476	3478	3482	rVB5	1953	965	0.14%	0.017%
73	12.239	3482	3483	3486	rBV2	1170	726	0.10%	0.013%
74	12.545	3576	3578	3581	rBV4	1030	697	0.10%	0.013%
75	12.596	3587	3594	3599	rBV10	3451	4613	0.67%	0.083%
76	12.693	3622	3624	3626	rBV3	1596	1009	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031224.D
 Acq On : 24 May 2023 18:45
 Operator : SY/MD
 Sample : 02866-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBX93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	12.786	3651	3653	3657	rBV5	2412	1916	0.28%	0.035%
78	12.841	3667	3670	3672	rBV3	1147	888	0.13%	0.016%
79	13.017	3723	3725	3730	rVB6	1895	1293	0.19%	0.023%
80	13.255	3796	3799	3804	rBV6	2209	1680	0.24%	0.030%
81	13.394	3840	3842	3844	rBV3	1431	719	0.10%	0.013%
82	13.413	3844	3848	3849	rBV3	1326	988	0.14%	0.018%
83	13.538	3884	3887	3891	rBV6	2767	1664	0.24%	0.030%
84	13.558	3891	3893	3896	rVV4	1535	852	0.12%	0.015%
85	13.583	3900	3901	3903	rBV2	1543	717	0.10%	0.013%
86	13.657	3922	3924	3926	rBV3	1811	1053	0.15%	0.019%
87	13.760	3952	3956	3958	rBV5	1537	1319	0.19%	0.024%
88	13.773	3958	3960	3963	rVB4	2678	1431	0.21%	0.026%
89	13.792	3963	3966	3967	rBV3	1368	660	0.10%	0.012%
90	13.802	3967	3969	3973	rVV5	1084	768	0.11%	0.014%
91	13.940	4009	4012	4015	rBV4	1409	1145	0.17%	0.021%
92	14.095	4058	4060	4064	rVB5	1837	1192	0.17%	0.022%
93	14.133	4070	4072	4074	rBV3	2389	926	0.13%	0.017%
94	14.156	4078	4079	4081	rBV2	1243	564	0.08%	0.010%
95	14.345	4135	4138	4140	rBV4	2514	1678	0.24%	0.030%
96	14.654	4231	4234	4236	rBV4	1754	966	0.14%	0.017%
97	14.673	4236	4240	4242	rBV5	2165	1588	0.23%	0.029%
98	14.792	4274	4277	4281	rBV6	2697	1655	0.24%	0.030%
99	14.895	4306	4309	4312	rBV5	2341	1973	0.28%	0.036%
100	15.008	4341	4344	4345	rBV3	1758	1067	0.15%	0.019%




Sum of corrected areas: 5526565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031224.D
Acq On : 24 May 2023 18:45
Operator : SY/MD
Sample : 02866-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

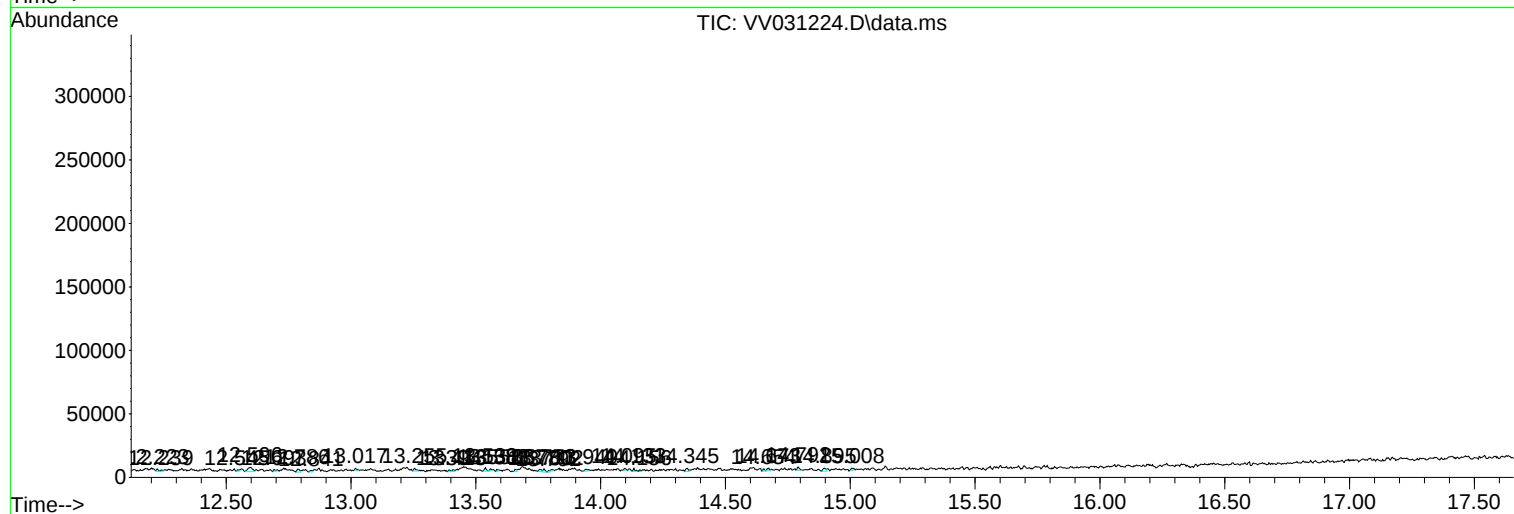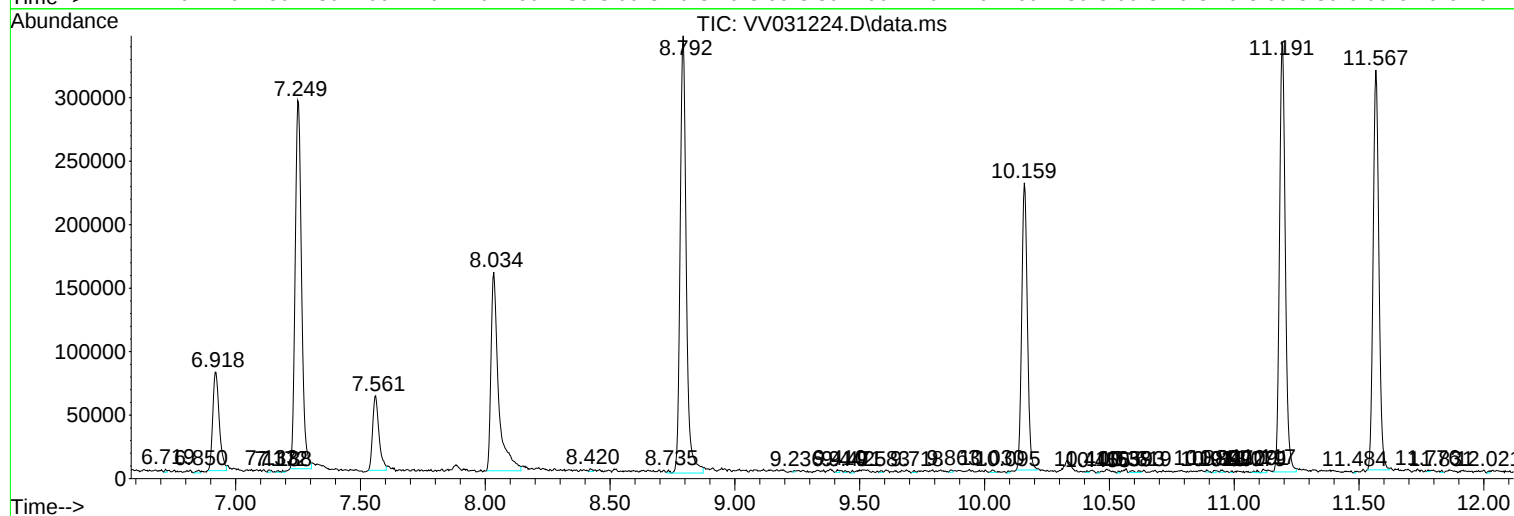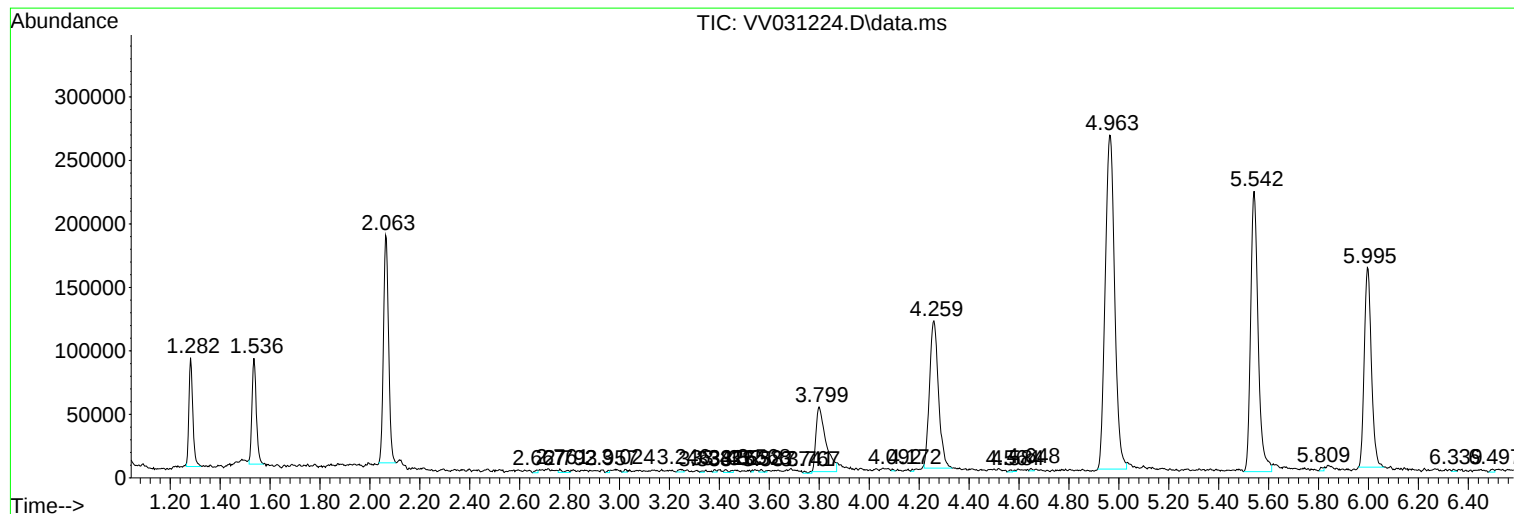

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031224.D
Acq On : 24 May 2023 18:45
Operator : SY/MD
Sample : 02866-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031224.D
Acq On : 24 May 2023 18:45
Operator : SY/MD
Sample : 02866-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBX93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc