

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031225.D
 Acq On : 24 May 2023 19:09
 Operator : SY/MD
 Sample : 02866-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	86	rVB	92957	96521	12.99%	1.674%
2	1.536	148	154	166	rVB	96204	111588	15.01%	1.935%
3	2.063	310	318	332	rVB	191294	279677	37.63%	4.849%
4	2.246	371	375	378	rBV6	1669	1222	0.16%	0.021%
5	2.333	399	402	405	rVB5	1536	985	0.13%	0.017%
6	2.391	414	420	424	rBV8	2265	3186	0.43%	0.055%
7	2.593	477	483	487	rVB8	1865	2270	0.31%	0.039%
8	2.616	487	490	494	rBV6	1369	974	0.13%	0.017%
9	2.654	499	502	503	rBV3	1923	921	0.12%	0.016%
10	2.687	508	512	513	rBV4	2171	1125	0.15%	0.020%
11	2.761	532	535	542	rVB9	3062	2765	0.37%	0.048%
12	2.818	549	553	556	rBV6	1904	1583	0.21%	0.027%
13	2.925	584	586	591	rVB6	2809	2115	0.28%	0.037%
14	2.966	591	599	604	rBV6	3476	4603	0.62%	0.080%
15	3.021	613	616	620	rBV5	1582	1440	0.19%	0.025%
16	3.314	702	707	709	rBV5	1536	1288	0.17%	0.022%
17	3.368	720	724	726	rBV4	1750	1236	0.17%	0.021%
18	3.452	747	750	753	rBV4	1807	1387	0.19%	0.024%
19	3.799	849	858	876	rBV	48366	126953	17.08%	2.201%
20	4.156	967	969	973	rBV5	1577	930	0.13%	0.016%
21	4.259	986	1001	1024	rVB	124517	317322	42.70%	5.502%
22	4.339	1024	1026	1029	rBV4	1710	960	0.13%	0.017%
23	4.664	1123	1127	1130	rBV5	1499	1473	0.20%	0.026%
24	4.902	1198	1201	1202	rBV3	2203	1345	0.18%	0.023%
25	4.966	1205	1221	1247	rVV2	277640	743210	100.00%	12.887%
26	5.407	1353	1358	1363	rBV8	1558	2135	0.29%	0.037%
27	5.542	1387	1400	1422	rBV	222293	467553	62.91%	8.107%
28	5.995	1529	1541	1558	rBV	165522	342196	46.04%	5.933%
29	6.365	1653	1656	1659	rBV5	1389	1043	0.14%	0.018%
30	6.497	1695	1697	1698	rBV2	1813	783	0.11%	0.014%
31	6.535	1704	1709	1711	rBV5	2274	1902	0.26%	0.033%
32	6.719	1762	1766	1767	rBV4	1554	1074	0.14%	0.019%
33	6.844	1802	1805	1810	rVB6	2053	1616	0.22%	0.028%
34	6.870	1810	1813	1815	rBV3	1946	1355	0.18%	0.023%
35	6.921	1820	1829	1845	rVV	78916	144046	19.38%	2.498%
36	7.130	1892	1894	1897	rBV4	2183	1122	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031225.D
 Acq On : 24 May 2023 19:09
 Operator : SY/MD
 Sample : 02866-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	7.249	1920	1931	1950	rBV	310057	552649	74.36%	9.582%
38	7.490	2003	2006	2013	rBV9	1952	2146	0.29%	0.037%
39	7.558	2014	2027	2041	rBV	62067	114699	15.43%	1.989%
40	7.747	2082	2086	2087	rBV4	1724	1122	0.15%	0.019%
41	8.034	2165	2175	2208	rBV	153529	326017	43.87%	5.653%
42	8.648	2359	2366	2369	rBV9	2376	3214	0.43%	0.056%
43	8.690	2375	2379	2382	rBV6	1210	1134	0.15%	0.020%
44	8.792	2400	2411	2432	rVV	346957	580117	78.06%	10.059%
45	8.998	2474	2475	2480	rVB5	1483	1047	0.14%	0.018%
46	9.188	2530	2534	2536	rBV5	1375	1003	0.13%	0.017%
47	9.622	2665	2669	2673	rVB5	2119	1965	0.26%	0.034%
48	9.645	2673	2676	2680	rBV5	1924	1684	0.23%	0.029%
49	9.664	2680	2682	2685	rBV4	1562	1026	0.14%	0.018%
50	9.780	2715	2718	2721	rBV4	2275	1804	0.24%	0.031%
51	9.834	2734	2735	2740	rVB5	1522	1071	0.14%	0.019%
52	9.870	2740	2746	2749	rBV9	2237	2806	0.38%	0.049%
53	9.908	2756	2758	2762	rBV5	1030	886	0.12%	0.015%
54	10.159	2825	2836	2851	rBV	228832	368805	49.62%	6.395%
55	10.294	2874	2878	2880	rBV5	1375	964	0.13%	0.017%
56	10.378	2902	2904	2908	rBV4	2474	2013	0.27%	0.035%
57	10.513	2944	2946	2950	rBV5	1212	961	0.13%	0.017%
58	10.561	2959	2961	2962	rBV2	1889	864	0.12%	0.015%
59	10.599	2970	2973	2975	rBV4	1547	945	0.13%	0.016%
60	10.609	2975	2976	2979	rVB3	1821	815	0.11%	0.014%
61	10.741	3013	3017	3019	rBV5	1954	1170	0.16%	0.020%
62	10.763	3022	3024	3026	rBV3	1967	1154	0.16%	0.020%
63	10.818	3038	3041	3043	rBV4	2445	1534	0.21%	0.027%
64	10.850	3048	3051	3053	rVB4	2016	1001	0.13%	0.017%
65	11.107	3126	3131	3132	rBV5	1518	1229	0.17%	0.021%
66	11.191	3147	3157	3174	rBV	344076	549879	73.99%	9.534%
67	11.342	3202	3204	3209	rBV6	1312	1053	0.14%	0.018%
68	11.378	3212	3215	3218	rBV4	1631	1206	0.16%	0.021%
69	11.567	3264	3274	3291	rVB	331934	525185	70.66%	9.106%
70	11.702	3314	3316	3320	rBV4	2416	1944	0.26%	0.034%
71	12.001	3407	3409	3414	rVB6	2479	1972	0.27%	0.034%
72	12.033	3414	3419	3421	rBV5	2382	2150	0.29%	0.037%
73	12.059	3425	3427	3431	rVV4	1270	1061	0.14%	0.018%
74	12.078	3431	3433	3436	rVV3	2010	1582	0.21%	0.027%
75	12.101	3438	3440	3443	rVB4	3147	1429	0.19%	0.025%
76	12.117	3443	3445	3447	rBV2	1355	810	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031225.D
 Acq On : 24 May 2023 19:09
 Operator : SY/MD
 Sample : 02866-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M

Title : VOC Analysis

77	12.207	3471	3473	3475	rBV3	1862	1162	0.16%	0.020%
78	12.284	3494	3497	3499	rBV4	1973	1273	0.17%	0.022%
79	12.426	3537	3541	3543	rBV4	1623	1122	0.15%	0.019%
80	12.567	3579	3585	3587	rBV7	1723	1722	0.23%	0.030%
81	12.638	3603	3607	3609	rBV4	2272	1775	0.24%	0.031%
82	12.664	3612	3615	3619	rVB5	1907	1414	0.19%	0.025%
83	12.754	3639	3643	3645	rBV4	1763	1331	0.18%	0.023%
84	12.844	3668	3671	3674	rVB5	1511	924	0.12%	0.016%
85	12.857	3674	3675	3680	rVB5	2423	1588	0.21%	0.028%
86	12.889	3680	3685	3686	rBV5	1868	1185	0.16%	0.021%
87	12.918	3692	3694	3698	rBV5	1419	1023	0.14%	0.018%
88	12.992	3714	3717	3720	rBV5	1461	1122	0.15%	0.019%
89	13.059	3733	3738	3739	rBV4	2823	1836	0.25%	0.032%
90	13.098	3745	3750	3752	rBV6	1847	1377	0.19%	0.024%
91	13.136	3760	3762	3767	rBV6	1425	1060	0.14%	0.018%
92	13.316	3815	3818	3820	rBV5	1340	1027	0.14%	0.018%
93	13.561	3892	3894	3902	rVB8	2210	1901	0.26%	0.033%
94	13.599	3902	3906	3908	rBV5	1209	1098	0.15%	0.019%
95	13.744	3949	3951	3955	rVB5	2626	1304	0.18%	0.023%
96	13.898	3996	3999	4002	rVB3	2480	1456	0.20%	0.025%
97	13.914	4002	4004	4006	rBV3	1179	801	0.11%	0.014%
98	14.294	4118	4122	4125	rBV6	2090	1782	0.24%	0.031%
99	14.657	4231	4235	4237	rVV4	1545	1107	0.15%	0.019%
100	15.175	4395	4396	4399	rBV3	1434	898	0.12%	0.016%




Sum of corrected areas: 5767308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031225.D
Acq On : 24 May 2023 19:09
Operator : SY/MD
Sample : 02866-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

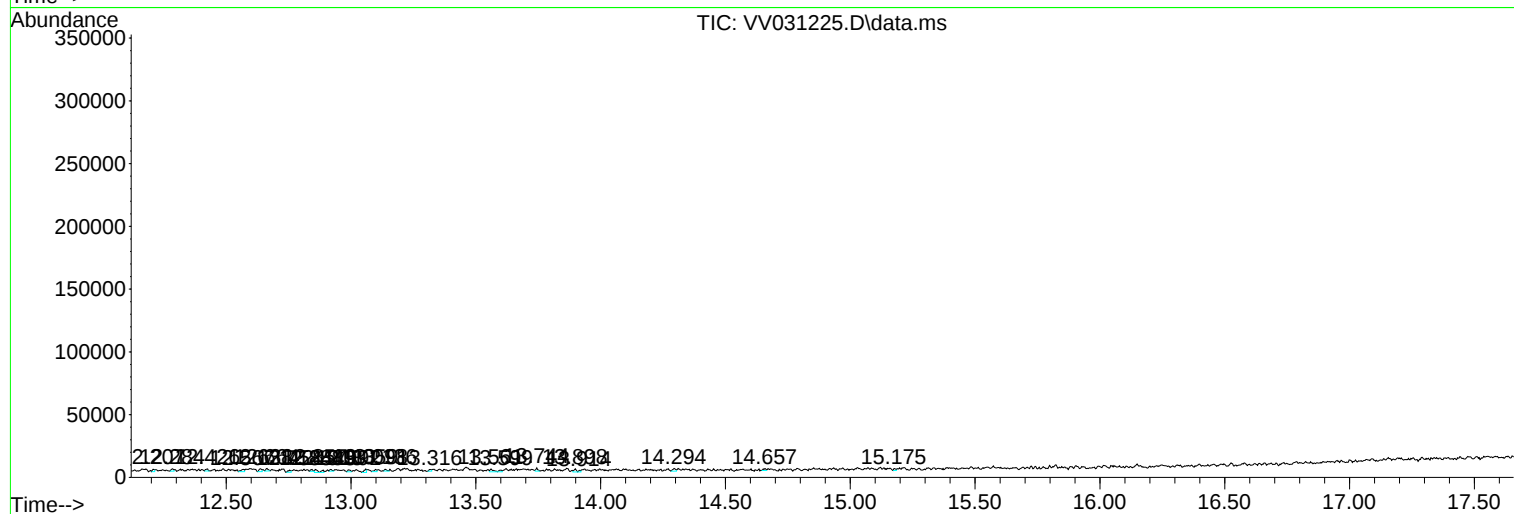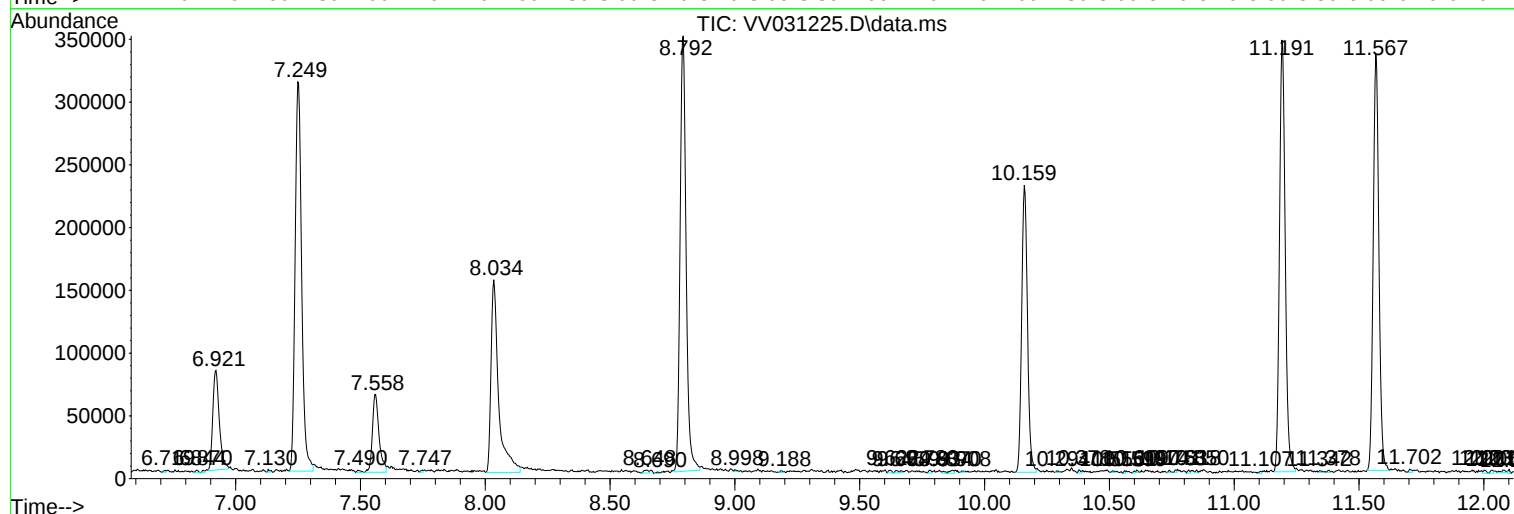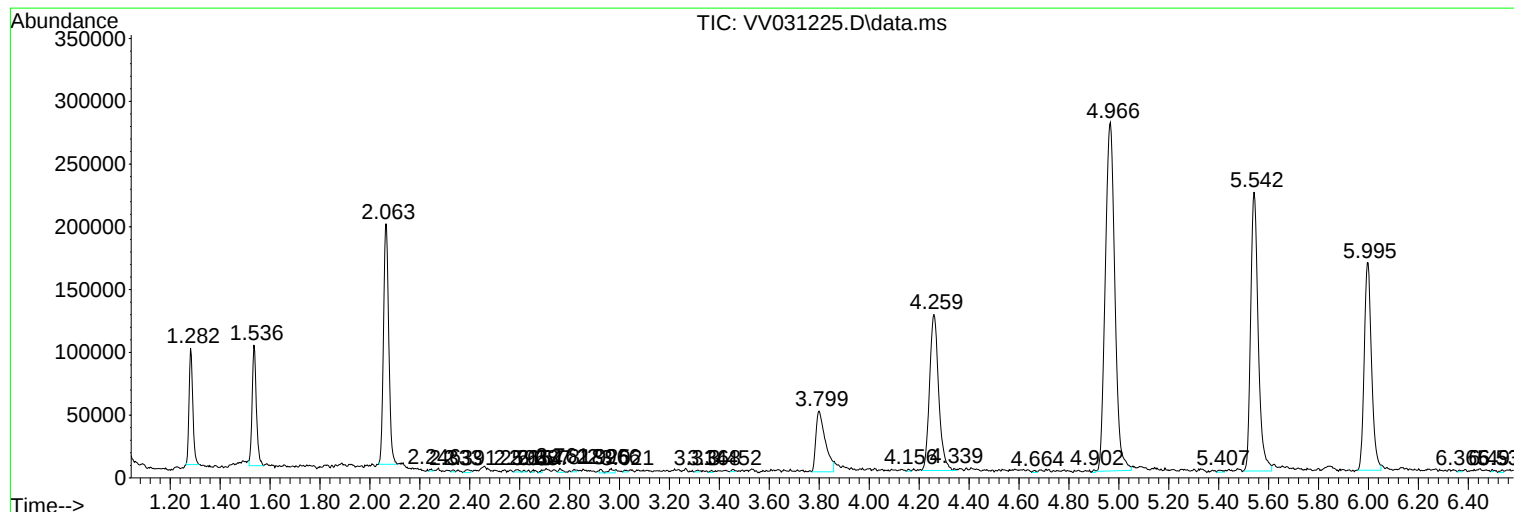

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031225.D
Acq On : 24 May 2023 19:09
Operator : SY/MD
Sample : 02866-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
Data File : VV031225.D
Acq On : 24 May 2023 19:09
Operator : SY/MD
Sample : 02866-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc