
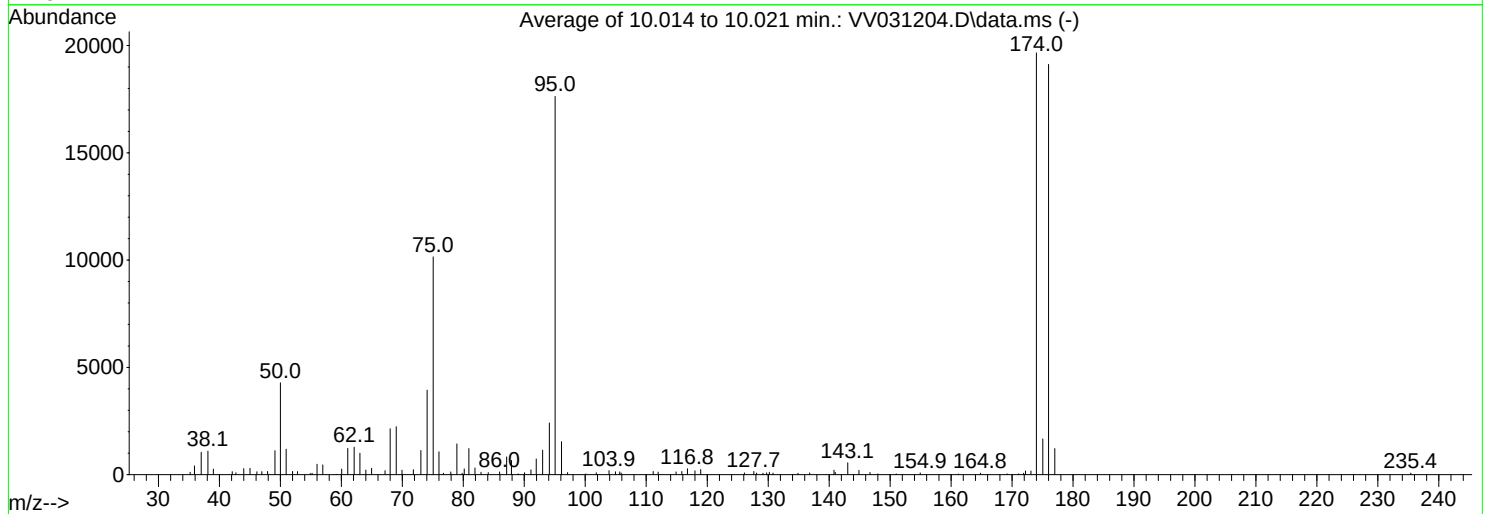


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052423\
 Data File : VV031204.D
 Acq On : 24 May 2023 10:08
 Operator : SY/MD
 Sample : BFB379
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB379

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis
 Last Update : Thu May 25 01:11:46 2023

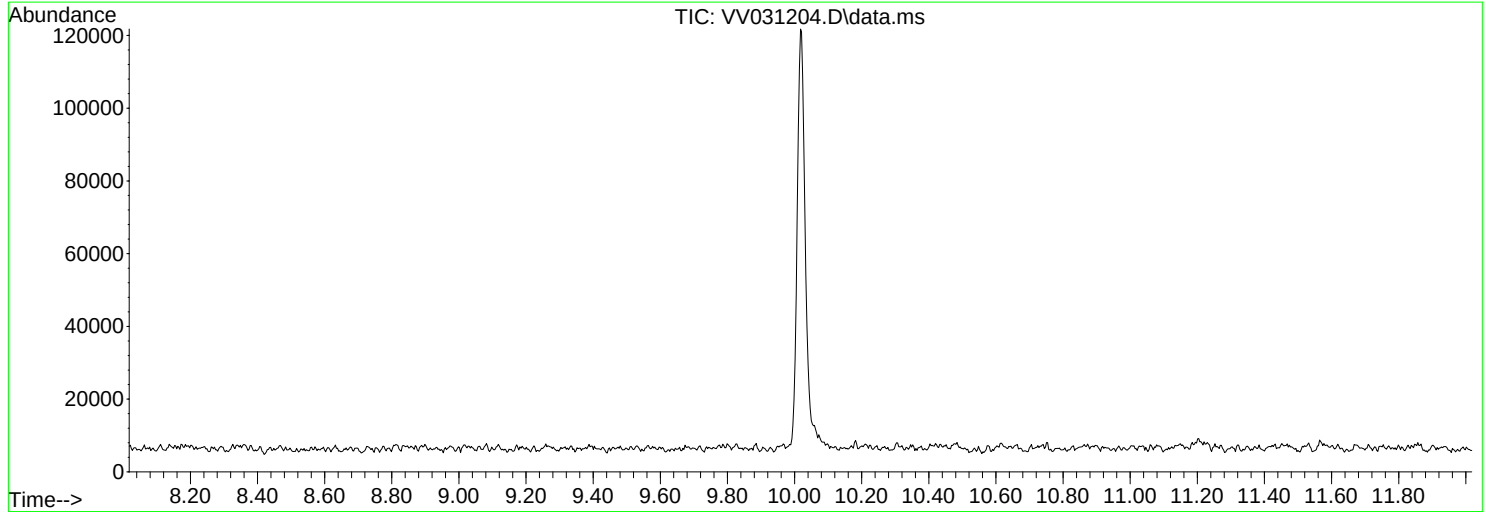

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	4282	PASS
75	95	30	80	57.5	10147	PASS
95	95	100	100	100.0	17632	PASS
96	95	5	9	8.7	1538	PASS
173	174	0.00	2	0.9	169	PASS
174	95	50	120	111.5	19661	PASS
175	174	5	9	8.4	1660	PASS
176	174	95	105	97.2	19120	PASS
177	176	5	10	6.4	1215	PASS

m/z	Abundance
35.80	125.0
36.50	128.0
37.20	144.0
38.30	177.0
38.90	198.0
40.00	1889.0
40.90	148.0
41.50	131.0
43.10	155.0
43.90	196.0
44.50	119.0
45.00	141.0
46.60	104.0
47.10	118.0
47.80	102.0
48.40	113.0
48.70	115.0
50.00	125.0
50.80	127.0
51.40	117.0
54.10	136.0
54.60	131.0
55.70	103.0
57.10	121.0
57.60	121.0
59.10	130.0
60.40	141.0
61.20	120.0
62.30	113.0
64.00	107.0
64.70	110.0
71.30	107.0
73.10	134.0
74.20	101.0
75.50	101.0
76.70	124.0
77.30	120.0
78.10	122.0
83.30	124.0
87.90	100.0
92.00	130.0
94.10	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
35.90	454.0
37.00	1090.0
38.10	1130.0
39.00	449.0
40.00	1405.0
41.10	121.0
42.10	144.0
42.80	159.0
44.00	487.0
45.00	403.0
46.10	128.0
47.00	253.0
47.90	288.0
49.10	1084.0
50.00	4091.0
51.00	1324.0
52.00	135.0
52.80	156.0
54.70	157.0
56.00	466.0
56.90	523.0
57.80	156.0
59.20	156.0
60.10	242.0
61.10	1236.0
62.10	1391.0
63.00	986.0
64.00	357.0
64.90	305.0
67.10	162.0
68.00	1981.0
69.00	2249.0
69.90	245.0
71.80	249.0
73.00	1152.0
74.10	3908.0
75.00	9708.0
76.00	1090.0
76.90	238.0
77.80	267.0
79.00	1318.0
80.10	299.0
80.90	1104.0
81.90	318.0
82.90	110.0
84.10	180.0
86.00	122.0
87.10	747.0
88.00	643.0
90.10	141.0
91.10	204.0
92.00	827.0
93.00	1020.0
94.10	2335.0
95.10	16744.0
96.10	1487.0
97.10	156.0
100.10	101.0
103.80	214.0
105.00	125.0
105.60	172.0
111.20	133.0
111.90	101.0
114.90	132.0
115.80	133.0
116.70	312.0
118.00	168.0
118.90	237.0
126.10	120.0
127.70	161.0
129.70	132.0
130.30	104.0
136.80	122.0
140.80	310.0
143.00	570.0
144.90	196.0
146.70	109.0
151.00	102.0
155.00	133.0
171.90	198.0
174.00	18080.0
175.00	1534.0
176.00	17824.0
177.00	1199.0
235.40	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
35.20	151.0
36.00	577.0
37.00	1210.0
38.10	1306.0
39.00	475.0
40.00	1432.0
41.00	142.0
42.10	145.0
43.00	122.0
44.10	502.0
45.10	490.0
46.20	129.0
46.90	267.0
48.00	249.0
49.10	1134.0
50.00	4553.0
51.00	1335.0
52.00	154.0
52.80	135.0
53.90	103.0
54.90	165.0
56.00	485.0
57.00	576.0
59.20	154.0
60.00	263.0
61.10	1386.0
62.10	1465.0
63.00	1019.0
64.10	334.0
65.00	299.0
67.10	206.0
68.00	2176.0
69.00	2290.0
69.90	212.0
71.80	237.0
73.10	1329.0
74.10	4160.0
75.00	10421.0
76.00	1105.0
76.90	191.0
77.90	265.0
78.90	1511.0
80.10	271.0
80.90	1260.0
81.90	317.0
82.90	125.0
84.10	120.0
86.00	122.0
87.10	846.0
88.00	806.0
89.00	111.0
90.00	127.0
91.10	234.0
92.00	895.0
93.00	1208.0
94.10	2597.0
95.00	18088.0
96.10	1661.0
97.10	135.0
101.80	118.0
103.90	186.0
104.90	145.0
105.70	200.0
111.10	152.0
112.00	129.0
114.90	127.0
115.80	152.0
116.70	274.0
118.00	185.0
118.90	240.0
126.10	133.0
127.60	144.0
128.10	117.0
129.20	103.0
129.80	121.0
130.20	117.0
130.80	102.0
134.90	105.0
136.80	118.0
140.80	315.0
143.10	600.0
144.90	208.0
146.70	115.0
148.00	102.0
154.90	107.0
164.80	100.0
172.20	242.0
174.00	20232.0
175.00	1739.0
176.00	19880.0
177.00	1270.0
235.40	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
35.20	176.0
36.00	580.0
37.00	1266.0
38.10	1390.0
39.10	462.0
40.00	1484.0
40.90	162.0
41.70	113.0
42.10	130.0
42.60	116.0
43.10	128.0
44.00	452.0
45.10	426.0
46.10	144.0
47.00	252.0
48.00	208.0
49.10	1131.0
50.00	4578.0
51.00	1280.0
52.00	149.0
52.80	129.0
53.90	128.0
55.20	205.0
56.00	509.0
57.00	624.0
59.20	126.0
60.00	283.0
61.00	1403.0
62.10	1331.0
63.10	999.0
64.10	284.0
65.00	295.0
67.20	196.0
68.00	2276.0
69.00	2179.0
70.00	165.0
71.80	197.0
73.00	1309.0
74.00	4054.0
75.10	10312.0
76.00	999.0
76.80	151.0
78.00	218.0
78.90	1467.0
79.80	201.0
80.20	225.0
80.90	1276.0
81.90	317.0
82.90	100.0
85.90	145.0
87.10	886.0
87.90	845.0
91.10	232.0
91.90	854.0
93.00	1191.0
94.10	2641.0
95.00	18064.0
96.10	1467.0
101.80	143.0
104.00	157.0
104.90	135.0
105.90	217.0
111.10	160.0
112.00	128.0
114.90	115.0
115.90	174.0
116.80	232.0
118.00	191.0
119.00	249.0
127.70	138.0
128.10	118.0
129.10	104.0
130.10	107.0
130.80	117.0
134.90	105.0
141.00	322.0
143.10	485.0
144.90	206.0
146.70	101.0
161.20	100.0
164.80	105.0
169.20	103.0
171.10	106.0
172.20	281.0
173.10	506.0
174.00	20672.0
175.10	1706.0
176.00	19656.0
177.00	1175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379