

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052424\
 Data File : VV035754.D
 Acq On : 24 May 2024 18:03
 Operator : SY/MD
 Sample : P2577-11
 Misc : 5.37g/10.0mL/MSVOA_V/SOIL/VIAL A
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHBN9

Quant Time: May 24 23:49:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 24 23:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	288508	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	201127	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	39196	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	149748	33.581	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	134.320%
7) Chloroethane-d5	1.529	69	118119	32.834	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	131.320%
11) 1,1-Dichloroethene-d2	2.053	65	59179	29.977	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	119.920%#
21) 2-Butanone-d5	3.854	46	43188	34.127	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.260%
24) Chloroform-d	4.246	84	222979	25.997	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.000%
26) 1,2-Dichloroethane-d4	4.944	65	120411	28.397	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	113.600%
32) Benzene-d6	4.957	84	396318	35.997	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	144.000%#
36) 1,2-Dichloropropane-d6	5.989	67	132338	38.950	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	155.800%#
41) Toluene-d8	7.243	98	258924	26.425	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.680%
43) trans-1,3-Dichloroprop...	7.561	79	31804	21.887	ug/L	0.01
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.560%
47) 2-Hexanone-d5	8.040	63	19216	31.453	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.900%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	88758	27.110	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.440%
66) 1,2-Dichlorobenzene-d4	11.561	152	32938	24.214	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.840%
Target Compounds					Qvalue	
13) Acetone	2.147	43	10086	5.445	ug/L	73
16) Methylene chloride	2.442	84	26423	3.972	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052424\
Data File : VV035754.D
Acq On : 24 May 2024 18:03
Operator : SY/MD
Sample : P2577-11
Misc : 5.37g/10.0mL/MSVOA_V/SOIL/VIAL A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHBN9

Quant Time: May 24 23:49:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 24 23:42:56 2024
Response via : Initial Calibration




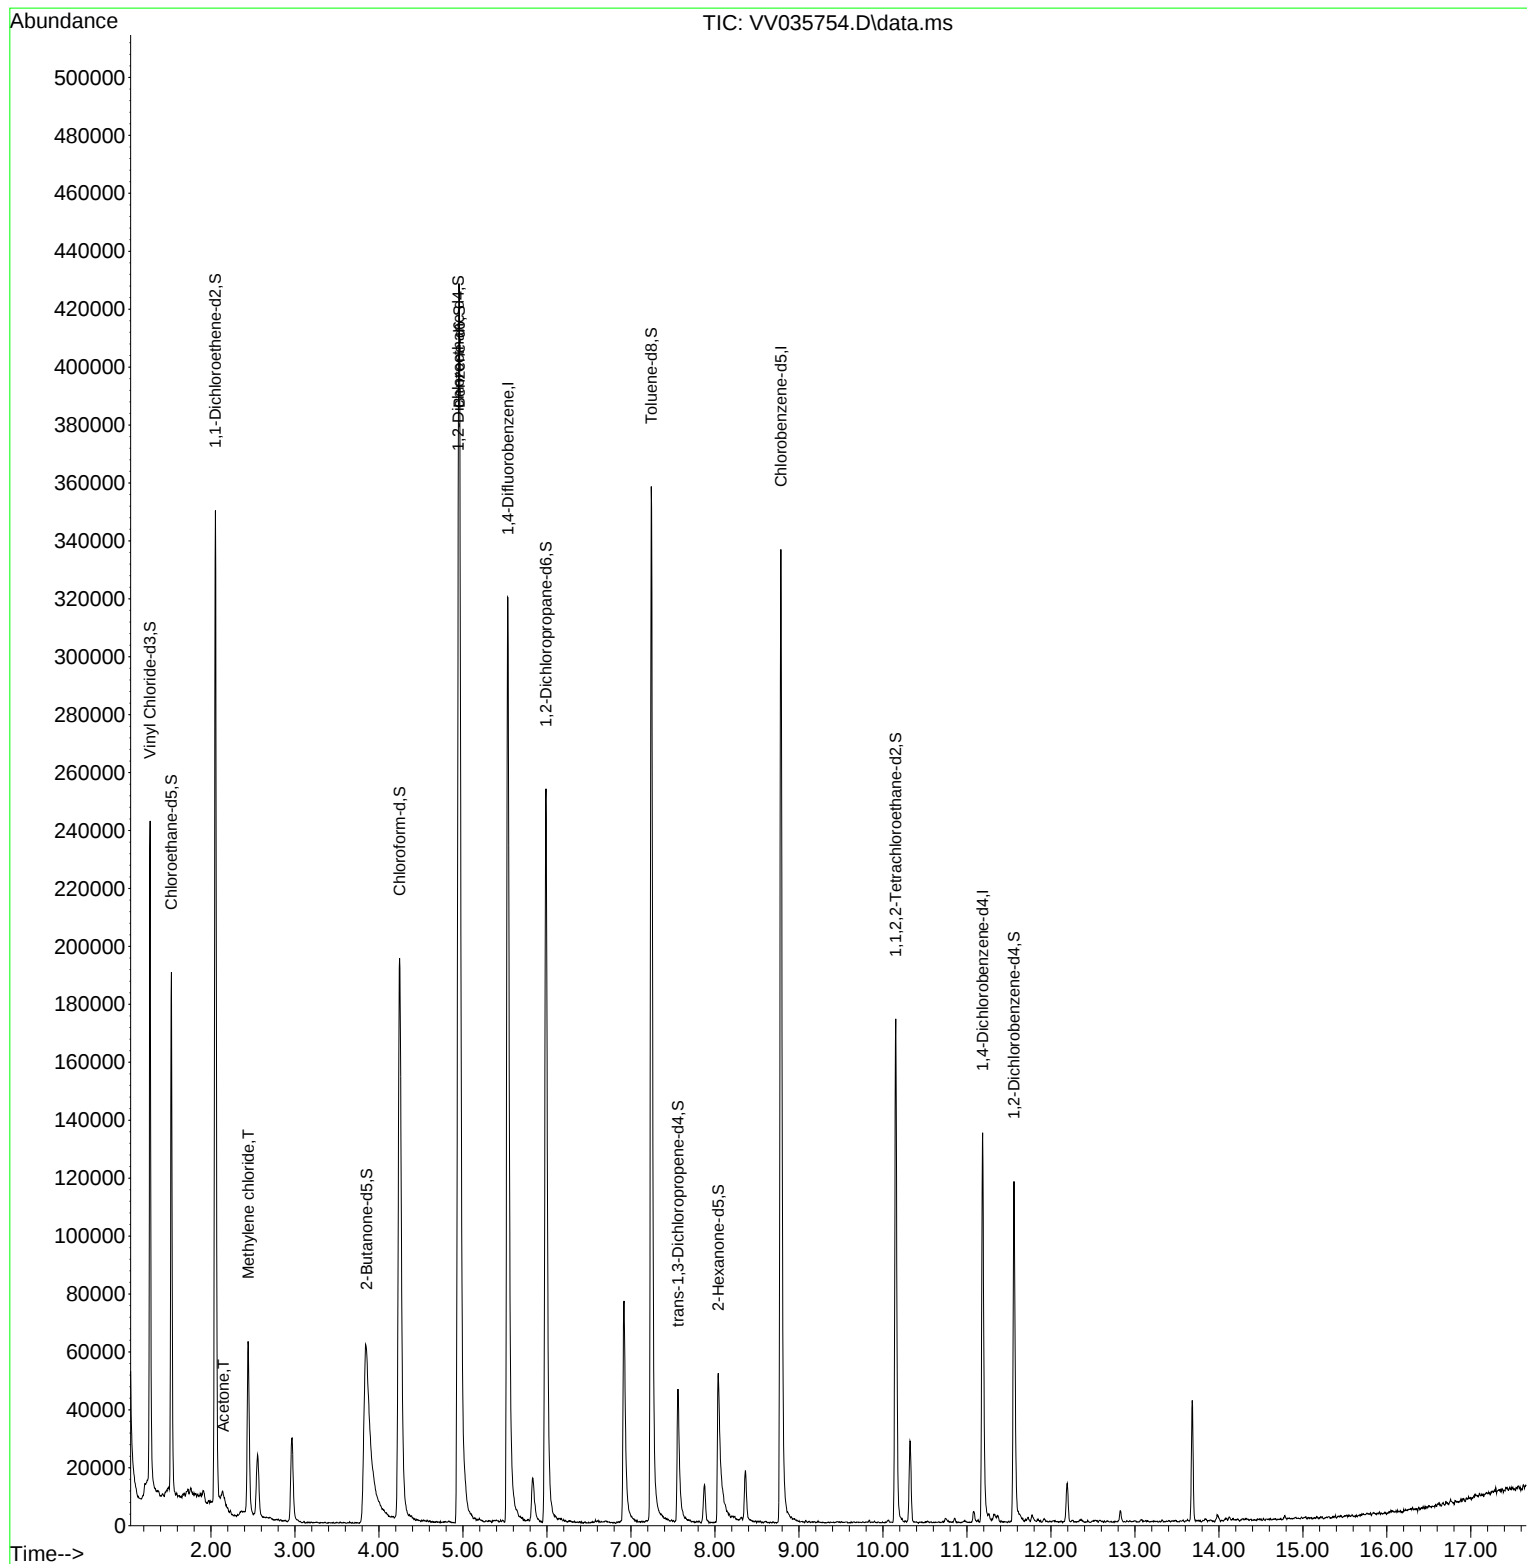


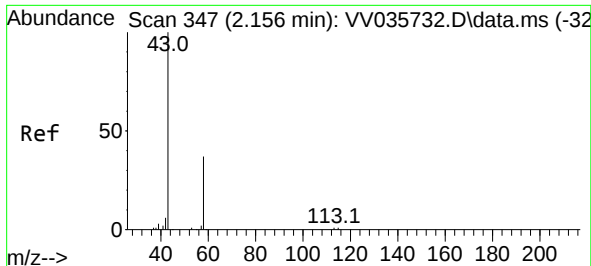

#13
Acetone
Concen: 5.445 ug/L
RT: 2.147 min Scan# 34
Delta R.T. -0.009 min
Lab File: VV035754.D
Acq: 24 May 2024 18:03

Instrument :
MSVOA_V
ClientSampleId :
BHBN9

Tgt Ion: 43 Resp: 10086
Ion Ratio Lower Upper
43 100
58 21.6 0.0 22.8

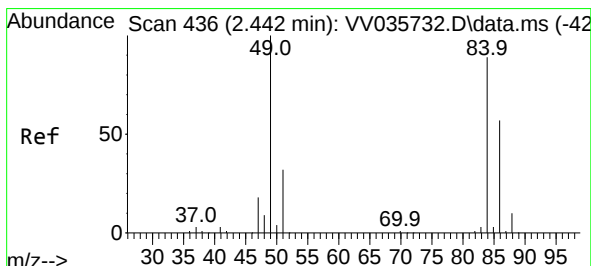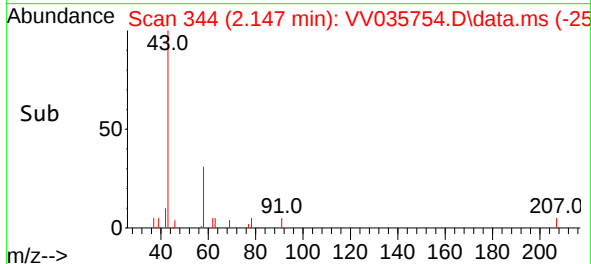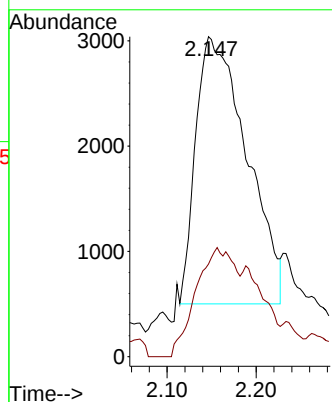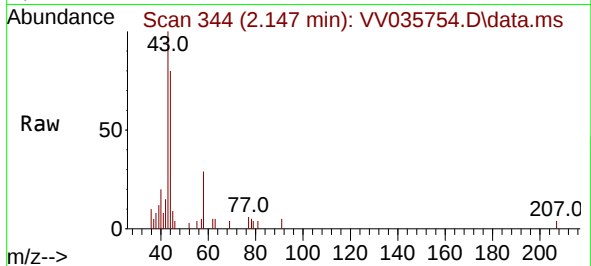

#16
Methylene chloride
Concen: 3.972 ug/L
RT: 2.442 min Scan# 436
Delta R.T. 0.000 min
Lab File: VV035754.D
Acq: 24 May 2024 18:03

Tgt Ion: 84 Resp: 26423
Ion Ratio Lower Upper
84 100
86 64.1 43.8 81.3
49 112.4 75.3 139.9

