


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021393.D
Acq On : 25 May 2021 17:13
Operator : SY/MD
Sample : M2496-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB443

Manual Integrations
APPROVED

MMDadoda
5/26/2021 3:13:15 PM

Quant Time: May 26 07:53:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 26 07:52:48 2021
Response via : Initial Calibration

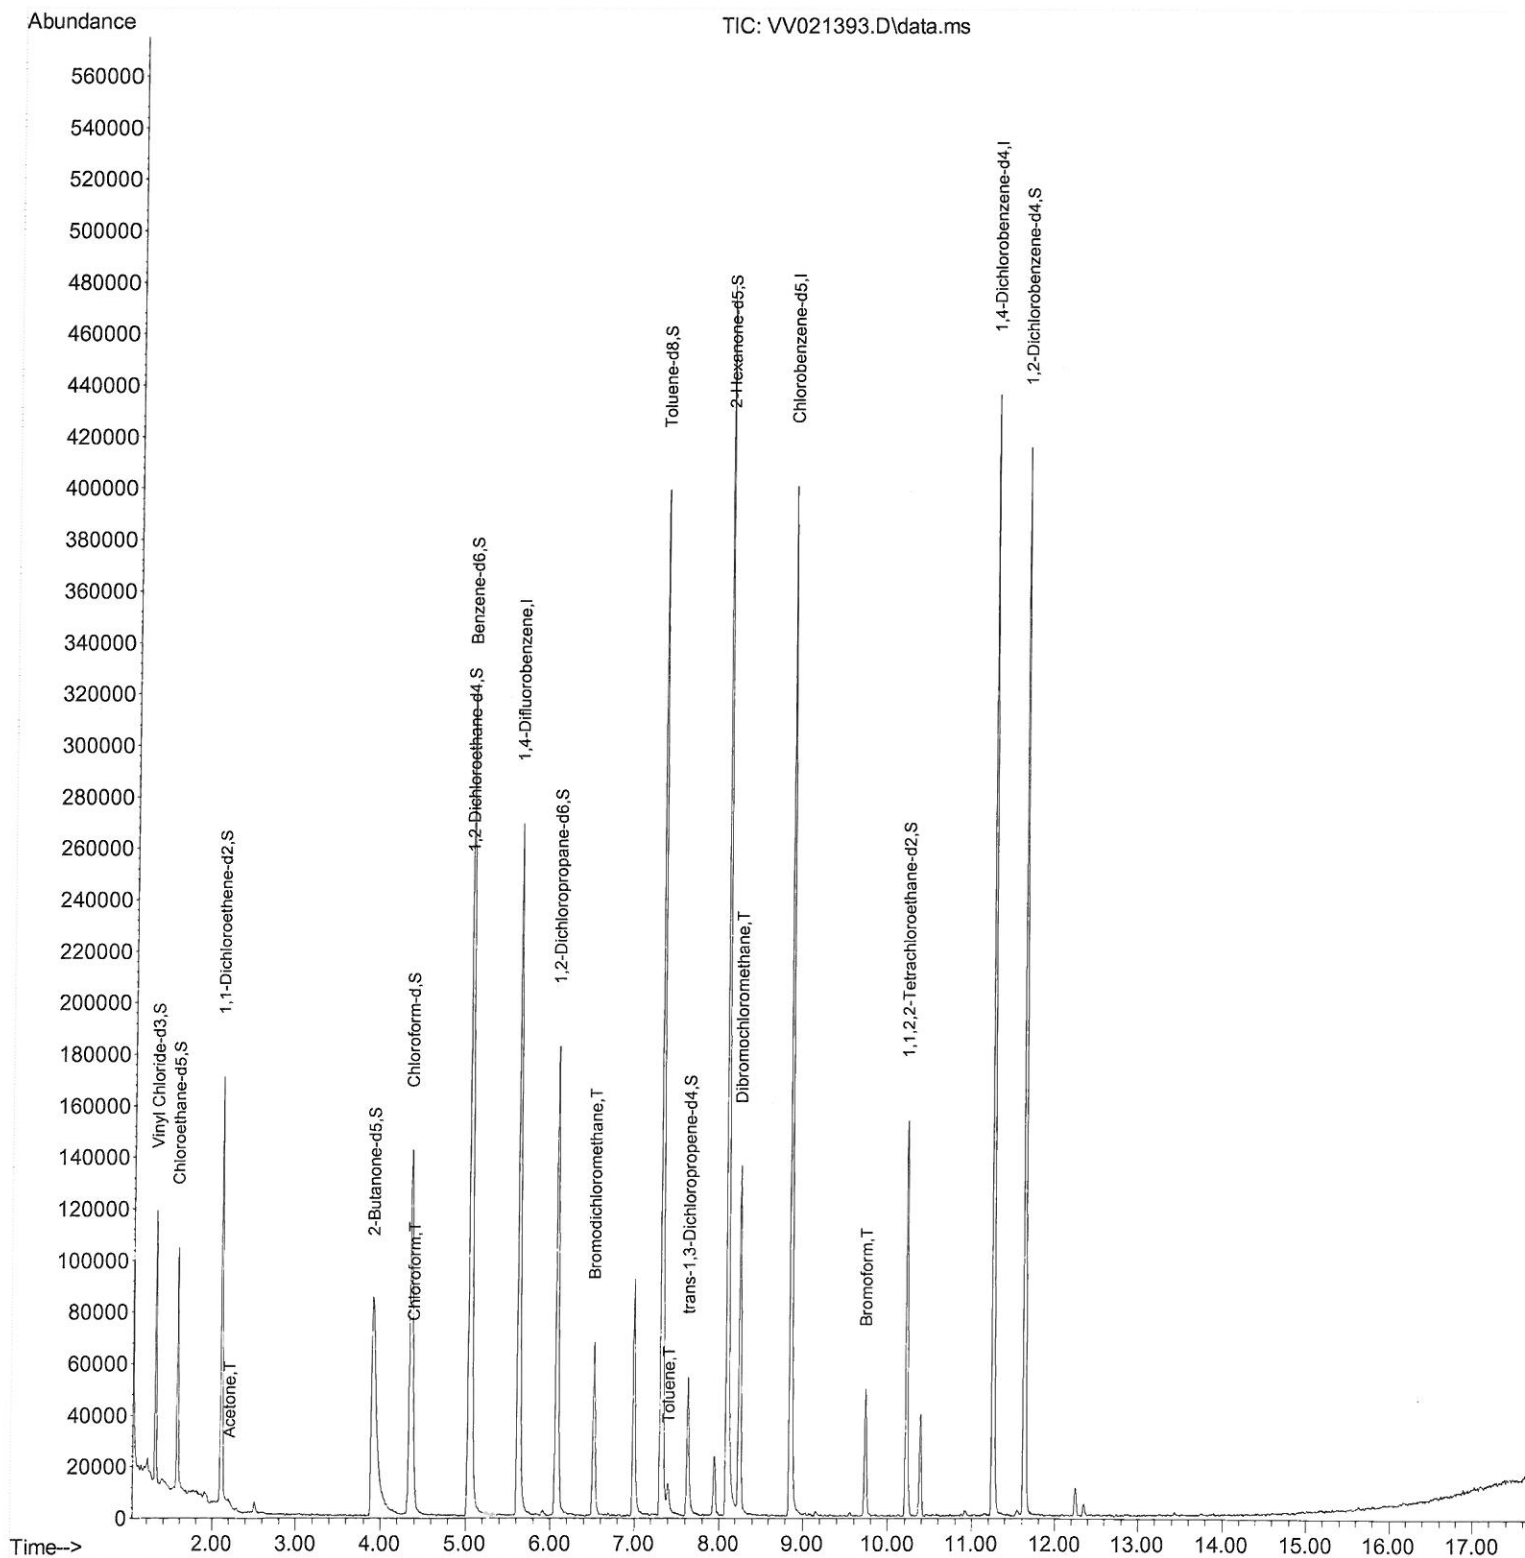



Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021393.D
 Acq On : 25 May 2021 17:13
 Operator : SY/MD
 Sample : M2496-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB443

Manual Integrations
 APPROVED

MMDadoda
 5/26/2021 3:13:15 PM

Quant Time: May 26 07:53:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

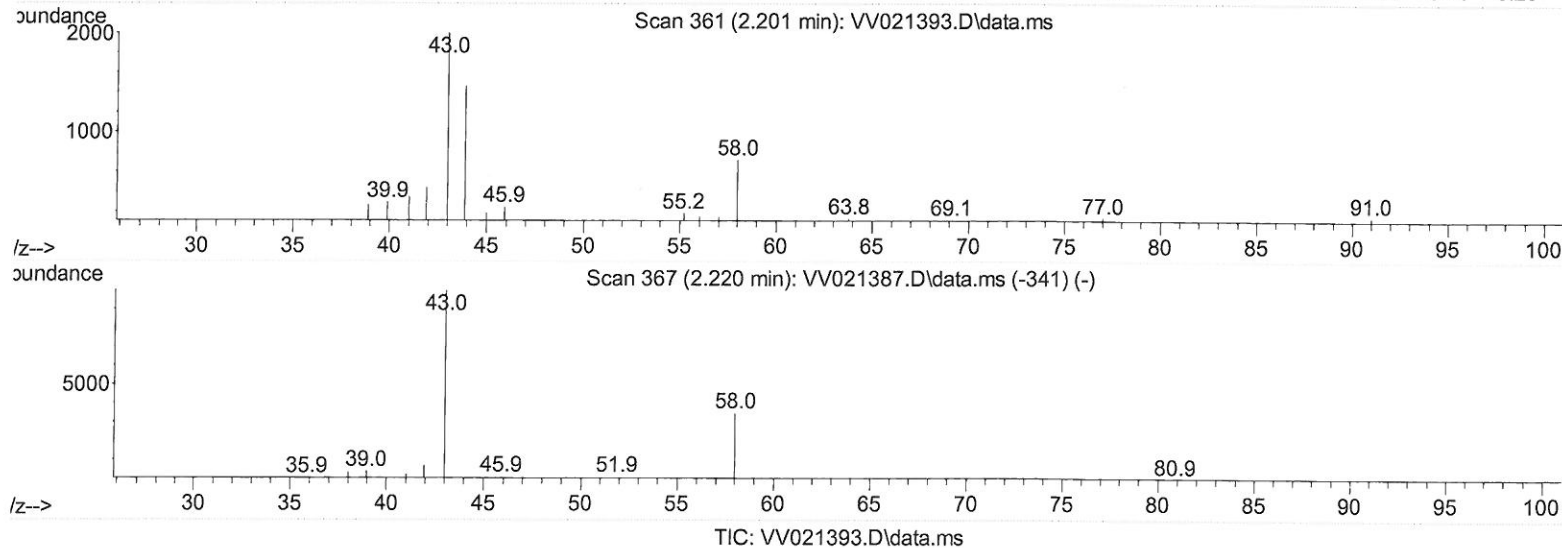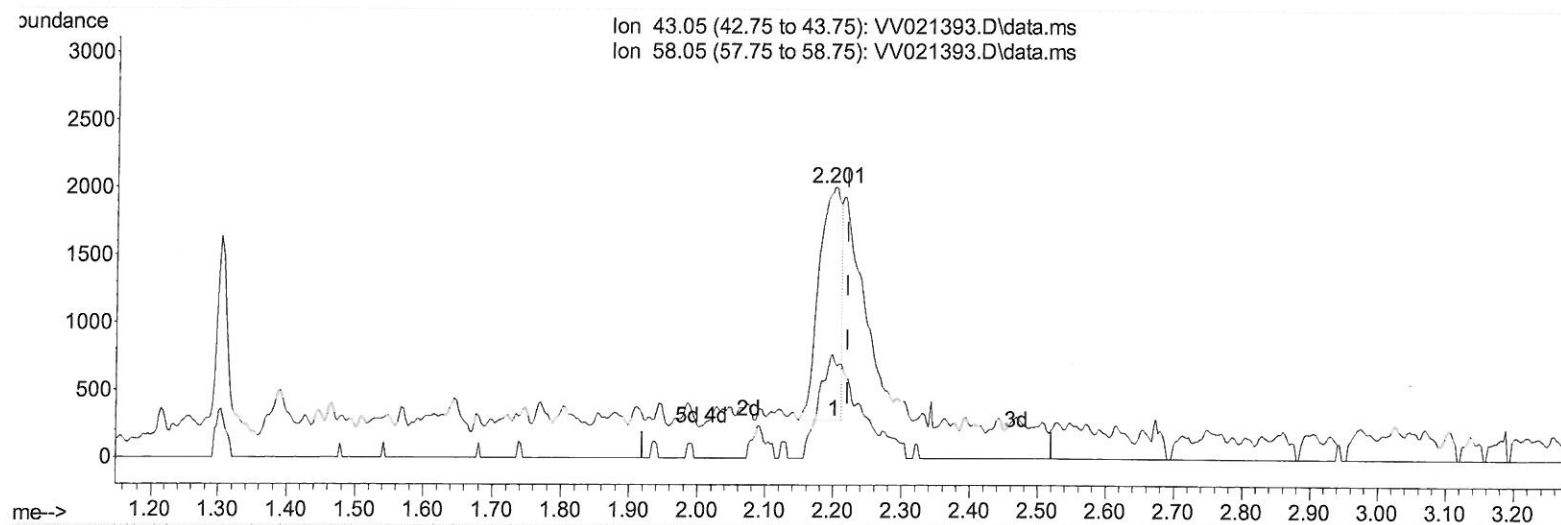

(13) Acetone (T)

2.201min (-0.019) 1.80 ug/L

response 3910

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	74.42#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021393.D
 Acq On : 25 May 2021 17:13
 Operator : SY/MD
 Sample : M2496-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB443

Manual Integrations
 APPROVED

MMDadoda
 5/26/2021 3:13:15 PM

Quant Time: May 26 07:53:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

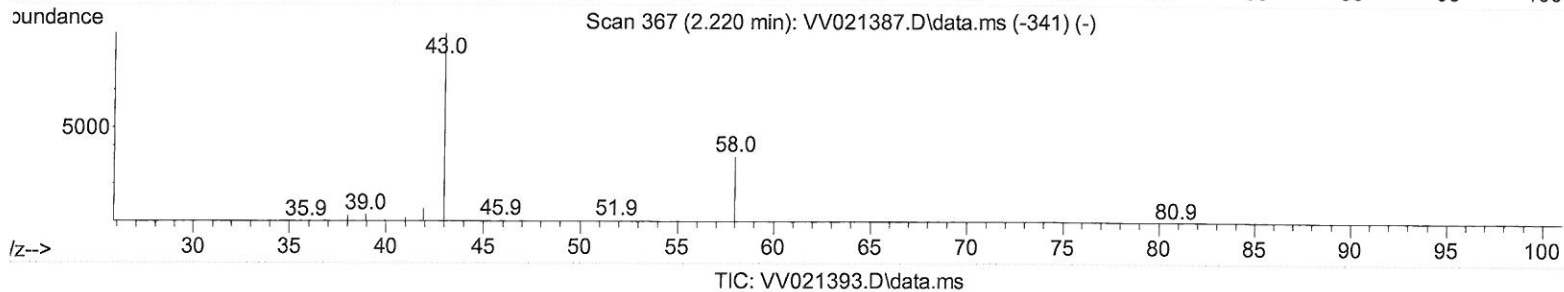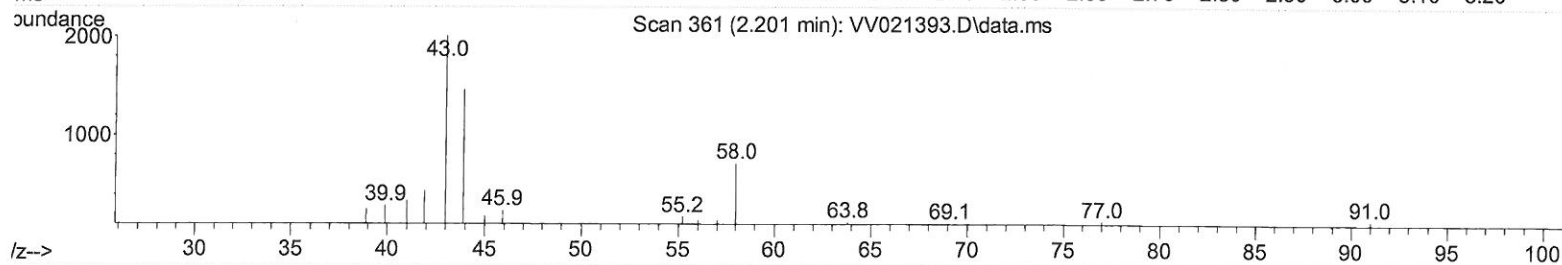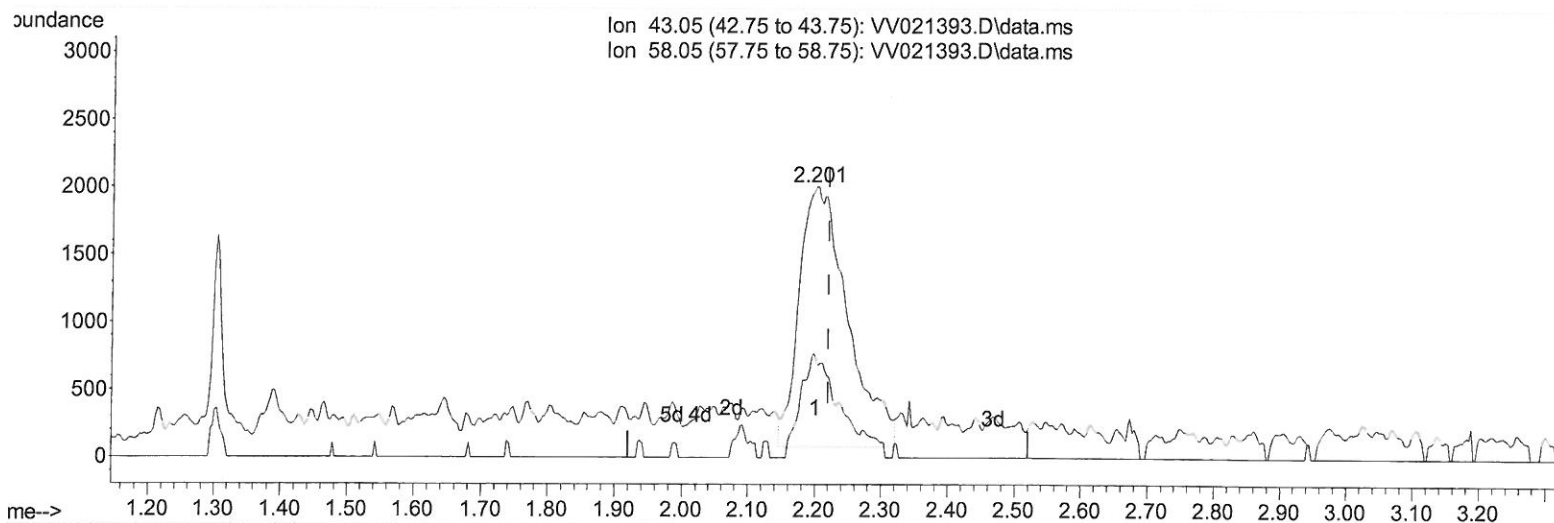

(13) Acetone (T)

2.201min (-0.019) 4.49 ug/L m

response 9750

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	29.85#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 5/28/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021393.D
 Acq On : 25 May 2021 17:13
 Operator : SY/MD
 Sample : M2496-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 GB443

Manual Integrations
 APPROVED

MMDadoda
 5/26/2021 3:13:15 PM

Quant Time: May 26 07:53:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 Last Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	253012	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	230742	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	124575	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	63373	5.92	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 118.40%			
7) Chloroethane-d5	1.564	69	57837	5.66	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 113.20%			
11) 1,1-Dichloroethene-d2	2.105	63	83637	4.12	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 82.40%			
20) 2-Butanone-d5	3.902	46	199635	51.88	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery = 103.76%			
24) Chloroform-d	4.352	84	148405	5.00	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 100.00%			
26) 1,2-Dichloroethane-d4	5.037	65	71704	5.25	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 105.00%			
32) Benzene-d6	5.053	84	299088	5.39	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 107.80%			
36) 1,2-Dichloropropane-d6	6.072	67	95372	5.30	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 106.00%			
41) Toluene-d8	7.320	98	275631	5.41	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 108.20%			
43) trans-1,3-Dichloroprop...	7.628	79	35559	4.75	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 95.00%			
46) 2-Hexanone-d5	8.091	63	179701	50.93	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 101.86%			
56) 1,1,2,2-Tetrachloroeth...	10.217	84	74885	5.16	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 103.20%			
66) 1,2-Dichlorobenzene-d4	11.625	152	115513	5.38	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 107.60%			
Target Compounds						
13) Acetone	2.201	43	9750m	4.49	ug/L	Qvalue
25) Chloroform	4.381	83	18760	0.66	ug/L	93
38) Bromodichloromethane	6.516	83	48513	2.38	ug/L	96
42) Toluene	7.403	91	9260	0.14	ug/L	95
49) Dibromochloromethane	8.249	129	72283	4.82	ug/L	99
59) Bromoform	9.735	173	23621	2.62	ug/L	100

MD
 5/28/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed