

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021390.D
 Acq On : 25 May 2021 16:01
 Operator : SY/MD
 Sample : M2496-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB433

Quant Time: May 26 07:53:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	239187	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	219425	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	119670	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	62572	6.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	123.60%
7) Chloroethane-d5	1.564	69	56997	5.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.00%
11) 1,1-Dichloroethene-d2	2.105	63	82393	4.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.00%
20) 2-Butanone-d5	3.921	46	205742	56.56	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.12%
24) Chloroform-d	4.352	84	149750	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.034	65	73459	5.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.80%
32) Benzene-d6	5.050	84	304818	5.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.40%
36) 1,2-Dichloropropane-d6	6.072	67	97331	5.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.80%
41) Toluene-d8	7.320	98	275880	5.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.00%
43) trans-1,3-Dichloroprop...	7.628	79	36547	5.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.60%
46) 2-Hexanone-d5	8.092	63	188532	56.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.38%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	75890	5.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.00%
66) 1,2-Dichlorobenzene-d4	11.625	152	116319	5.64	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.80%
Target Compounds					Qvalue	
42) Toluene	7.400	91	5505	0.09	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021390.D
Acq On : 25 May 2021 16:01
Operator : SY/MD
Sample : M2496-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB433

Quant Time: May 26 07:53:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 26 07:52:48 2021
Response via : Initial Calibration

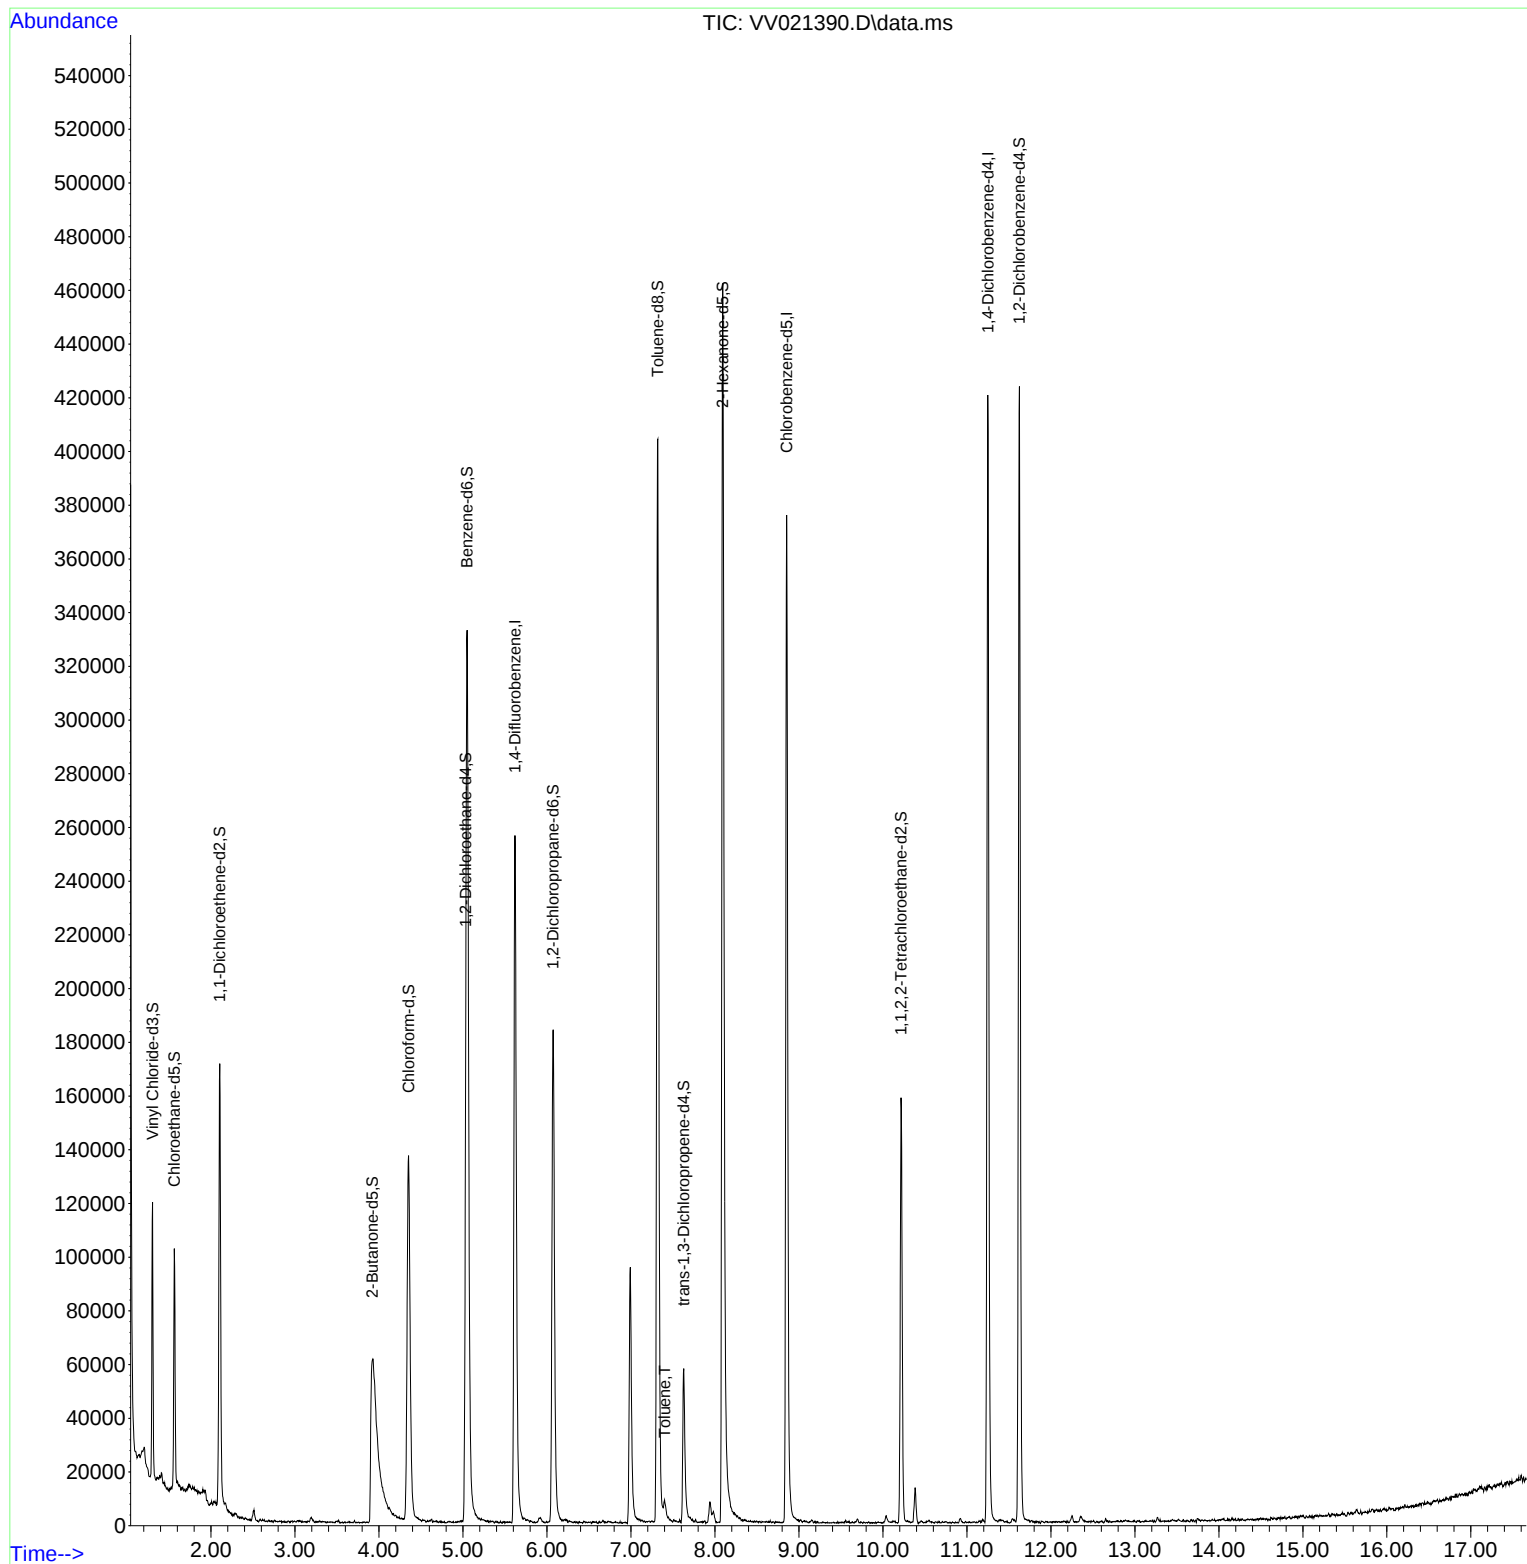

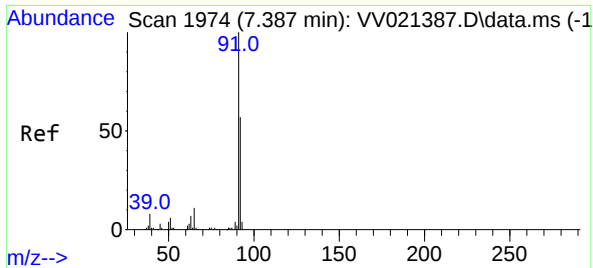

#42
Toluene
Concen: 0.09 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.013 min
Lab File: VV021390.D
Acq: 25 May 2021 16:01

Instrument :
MSVOA_V
ClientSampleId :
GB433

Tgt Ion: 91 Resp: 5505
Ion Ratio Lower Upper
91 100
92 58.8 40.9 76.0

