

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052521\
 Data File : VW021401.D
 Acq On : 25 May 2021 20:25
 Operator : SY/MD
 Sample : M2496-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB436

Quant Time: May 26 07:54:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	241884	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	227687	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	123062	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	60712	5.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.60%
7) Chloroethane-d5	1.568	69	56439	5.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.60%
11) 1,1-Dichloroethene-d2	2.108	63	81046	4.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.60%
20) 2-Butanone-d5	3.908	46	224607	61.06	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.12%
24) Chloroform-d	4.352	84	148696	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.037	65	73996	5.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.40%
32) Benzene-d6	5.053	84	298194	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.80%
36) 1,2-Dichloropropane-d6	6.072	67	95901	5.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.00%
41) Toluene-d8	7.320	98	271117	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
43) trans-1,3-Dichloroprop...	7.628	79	36373	4.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.40%
46) 2-Hexanone-d5	8.091	63	208139	59.78	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.56%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	81477	5.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.80%
66) 1,2-Dichlorobenzene-d4	11.625	152	117337	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%
Target Compounds						Qvalue
19) 1,1-Dichloroethane	3.198	63	3172	0.12	ug/L	97
47) Tetrachloroethene	7.979	164	1579	0.11	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021401.D
Acq On : 25 May 2021 20:25
Operator : SY/MD
Sample : M2496-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB436

Quant Time: May 26 07:54:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 26 07:52:48 2021
Response via : Initial Calibration

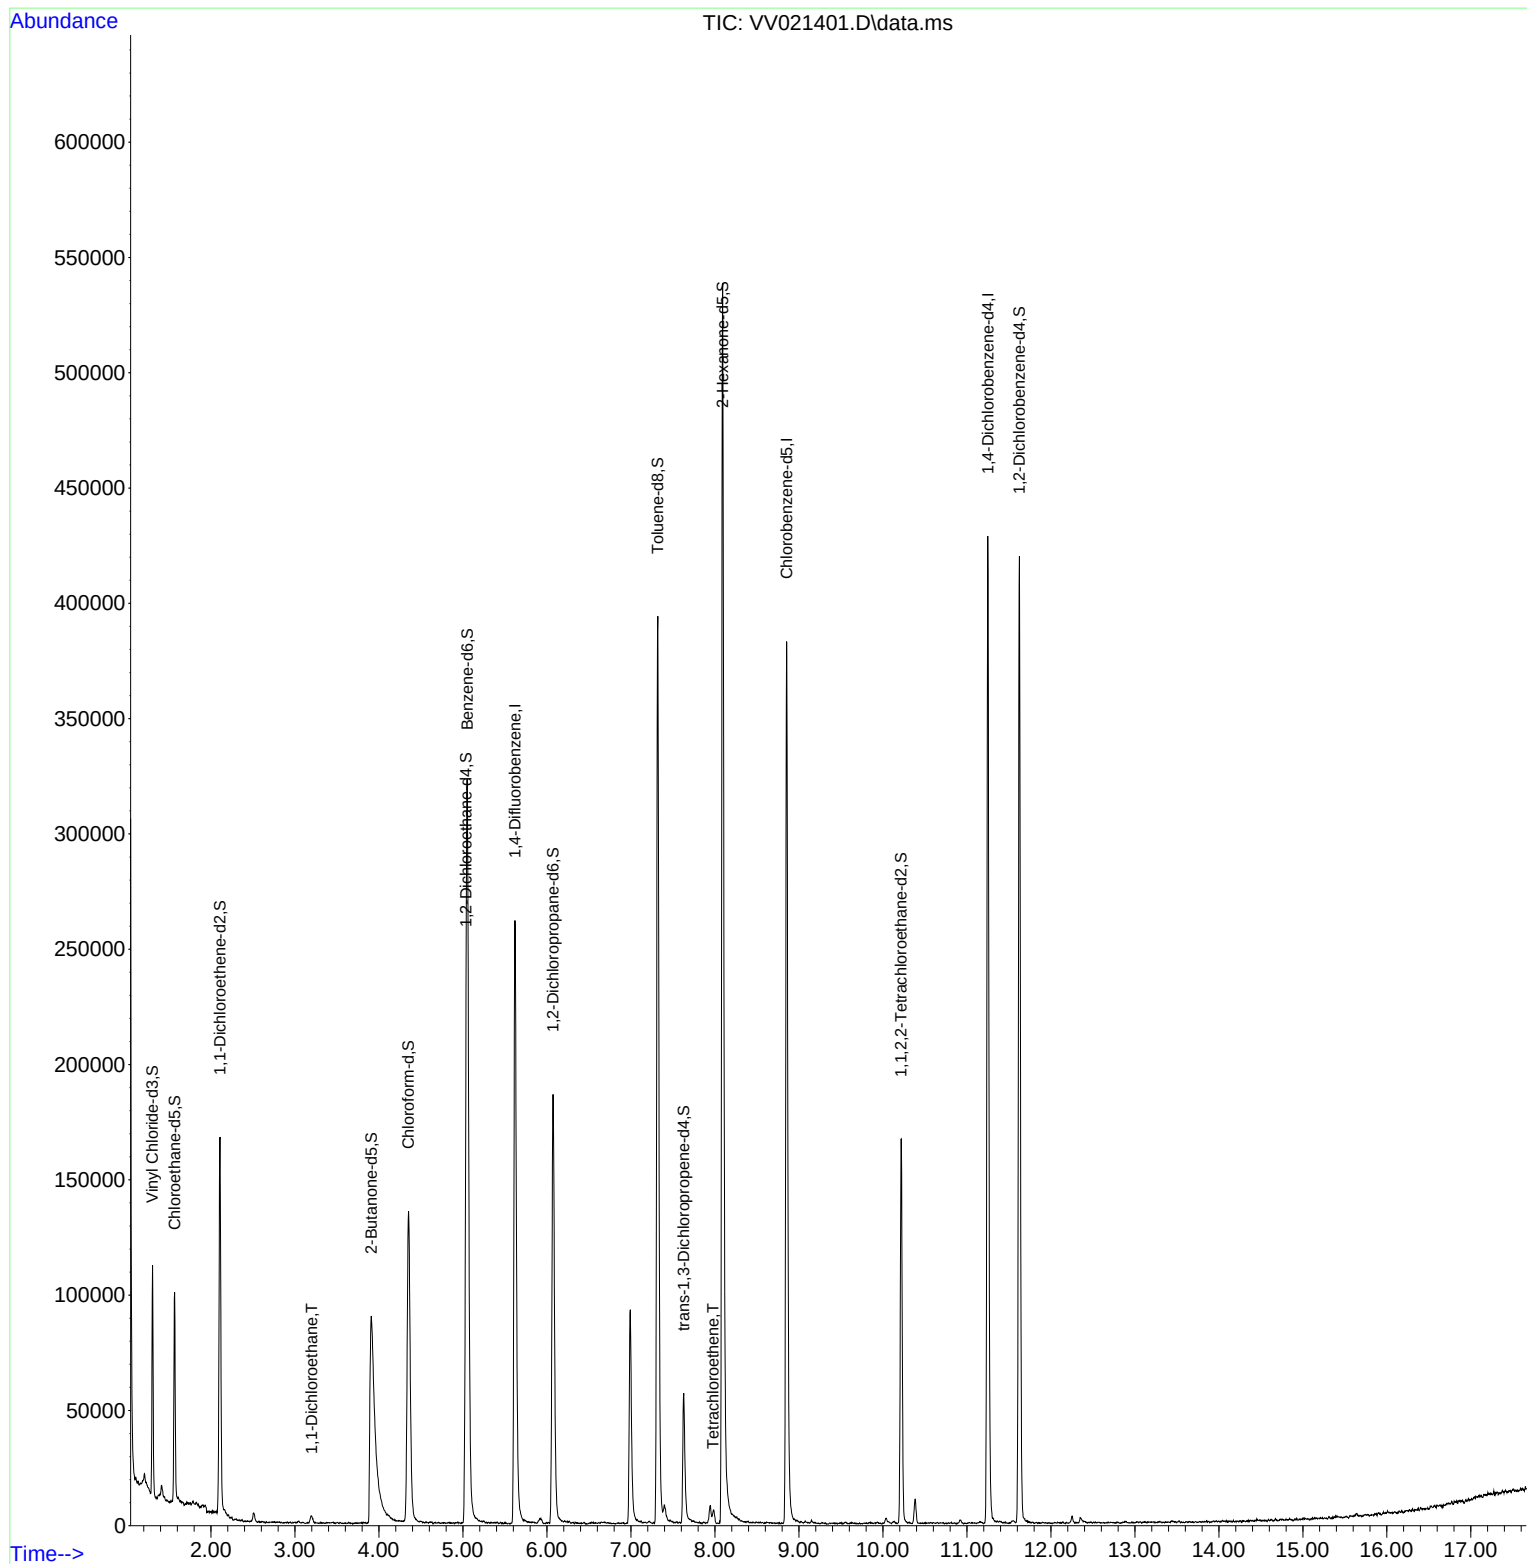

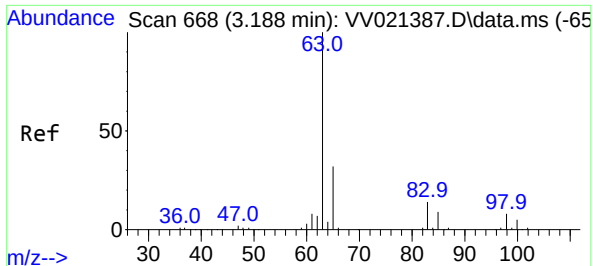

#19

1,1-Dichloroethane

Concen: 0.12 ug/L

RT: 3.198 min Scan# 671





Delta R.T. 0.010 min

Lab File: VV021401.D

Acq: 25 May 2021 20:25

Tgt Ion: 63 Resp: 3172

Ion	Ratio	Lower	Upper
63	100		
65	32.3	23.2	43.2
83	16.5	9.4	17.4

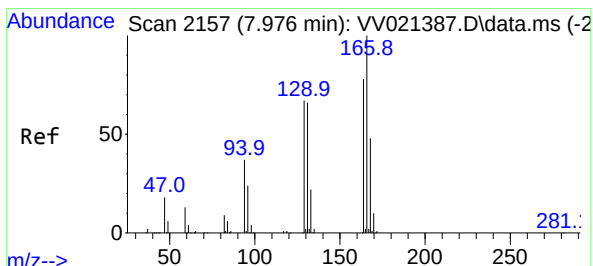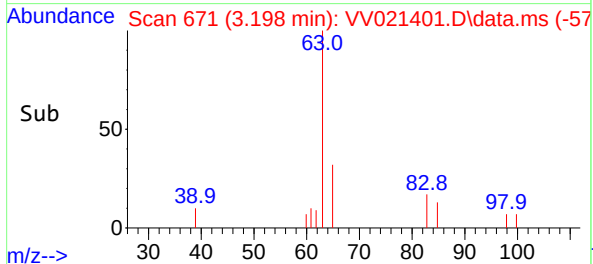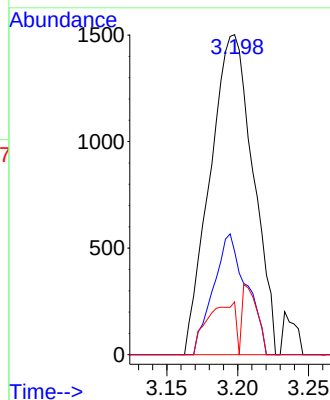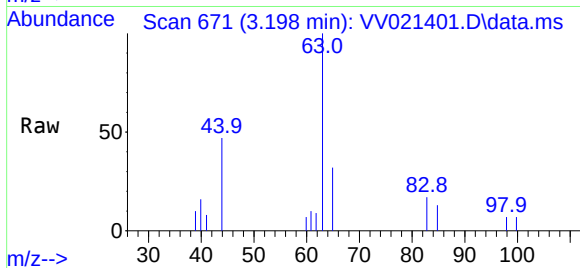

#47

Tetrachloroethene

Concen: 0.11 ug/L

RT: 7.979 min Scan# 2158

Delta R.T. 0.003 min

Lab File: VV021401.D

Acq: 25 May 2021 20:25

Tgt Ion: 164 Resp: 1579

Ion	Ratio	Lower	Upper
164	100		
129	77.2	61.8	114.8
131	76.8	57.8	107.4
166	94.2	87.4	162.4

