

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021402.D
 Acq On : 25 May 2021 20:49
 Operator : SY/MD
 Sample : M2496-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB438

Quant Time: May 26 07:54:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 26 07:52:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	242557	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	223776	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	123175	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	59991	5.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	117.00%
7) Chloroethane-d5	1.568	69	54621	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.105	63	77605	3.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.80%
20) 2-Butanone-d5	3.908	46	229875	62.32	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.64%
24) Chloroform-d	4.352	84	144484	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.040	65	72518	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.80%
32) Benzene-d6	5.053	84	293384	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.00%
36) 1,2-Dichloropropane-d6	6.072	67	94315	5.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.00%
41) Toluene-d8	7.320	98	266565	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
43) trans-1,3-Dichloroprop...	7.629	79	33917	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.092	63	202652	59.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.44%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	79979	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.60%
66) 1,2-Dichlorobenzene-d4	11.625	152	116701	5.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.00%
Target Compounds						
42) Toluene	7.404	91	5291	0.08	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021402.D
Acq On : 25 May 2021 20:49
Operator : SY/MD
Sample : M2496-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB438

Quant Time: May 26 07:54:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 26 07:52:48 2021
Response via : Initial Calibration

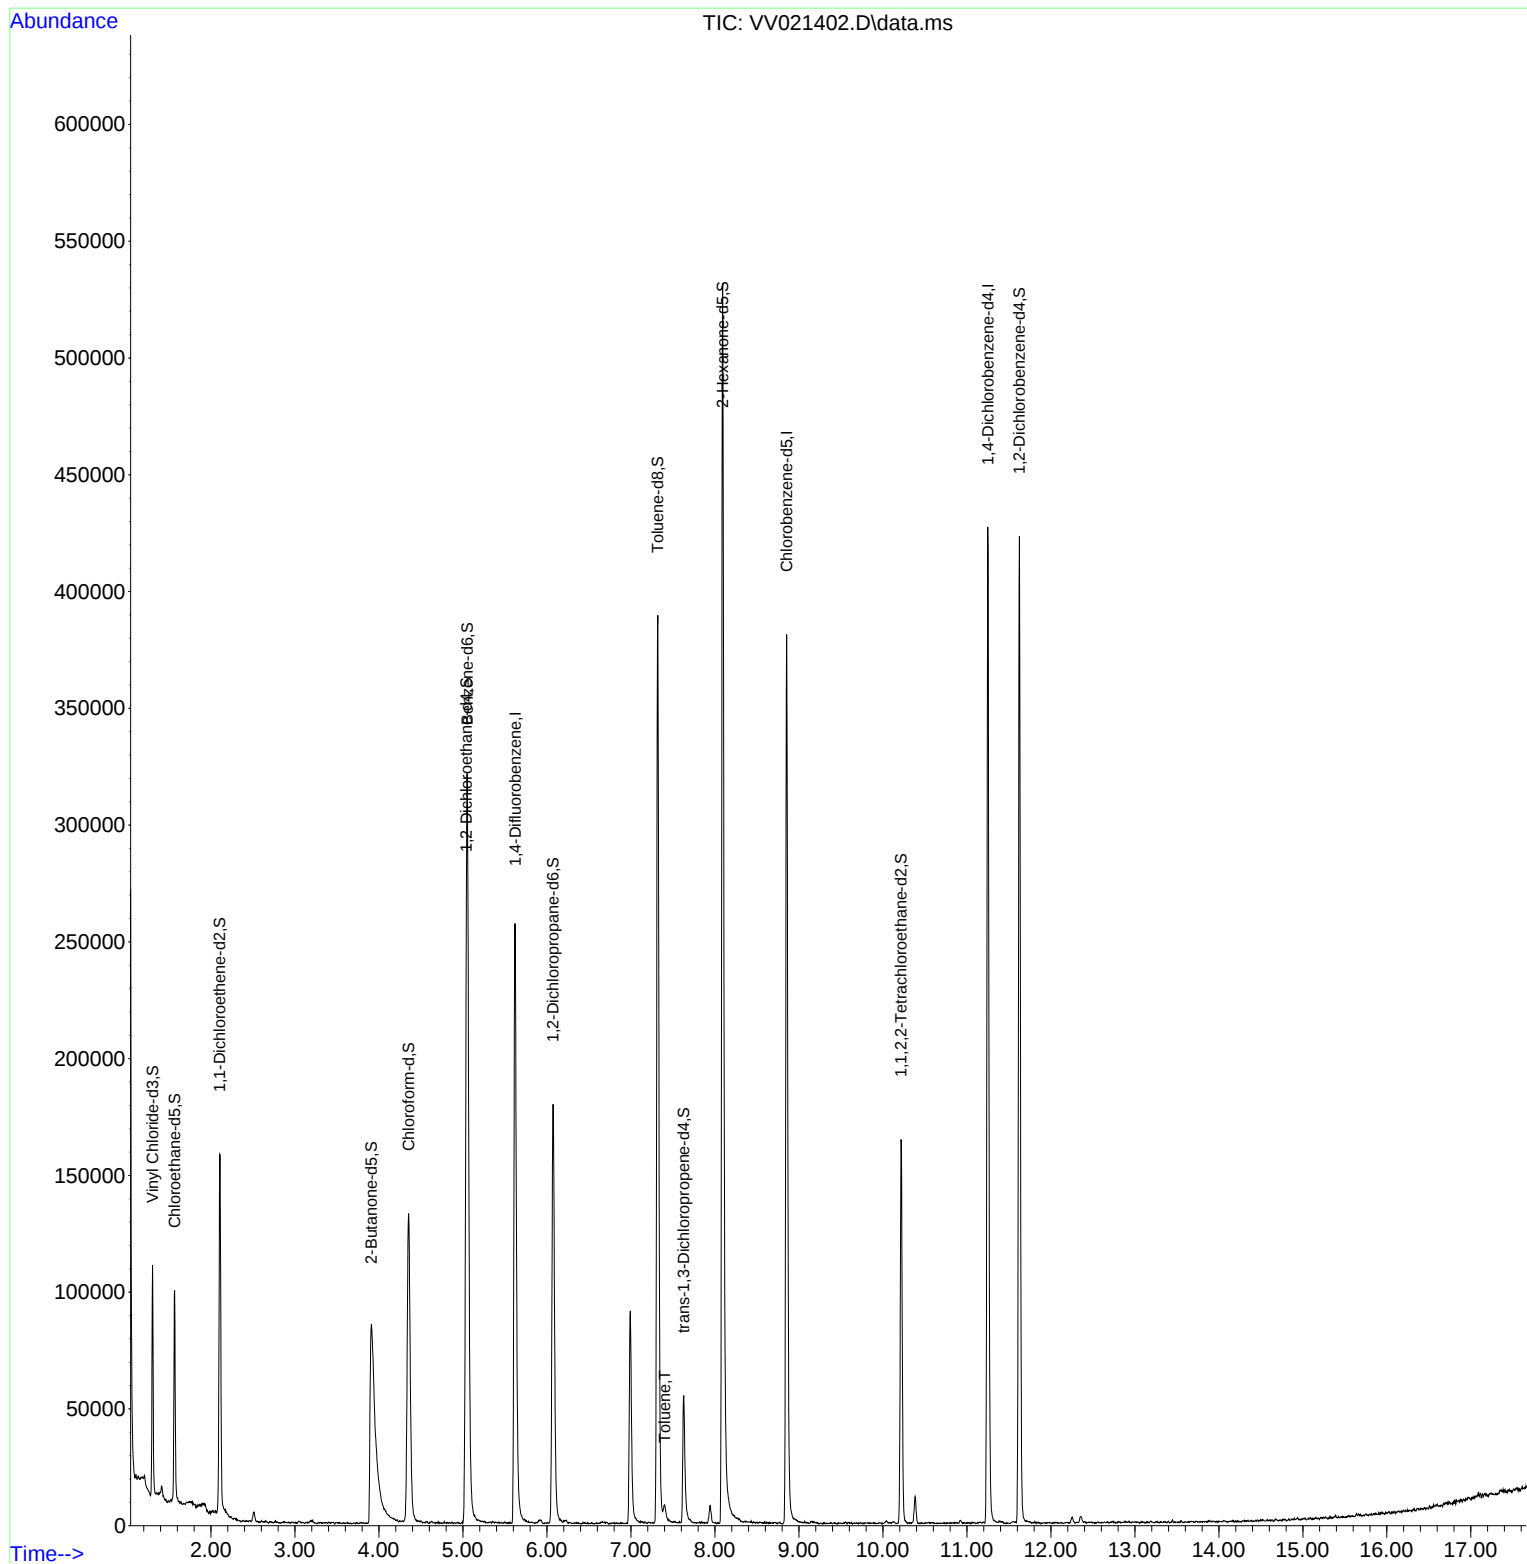

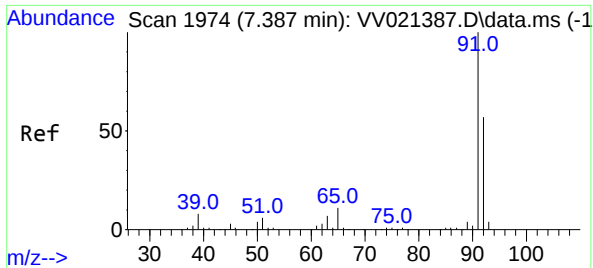

#42
Toluene
Concen: 0.08 ug/L
RT: 7.404 min Scan# 1979
Delta R.T. 0.016 min
Lab File: VV021402.D
Acq: 25 May 2021 20:49

Instrument :
MSVOA_V
ClientSampled :
GB438

Tgt Ion: 91 Resp: 5291
Ion Ratio Lower Upper
91 100
92 45.1 40.9 76.0

