

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021396.D
 Acq On : 25 May 2021 18:25
 Operator : SY/MD
 Sample : M2496-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB459

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV021396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	72	79	93	rVB2	136081	218904	25.39%	2.963%
2	1.568	157	164	185	rVB	93792	111856	12.97%	1.514%
3	2.108	323	332	346	rBV	165507	237578	27.56%	3.216%
4	2.195	352	359	380	rVB2	9352	28804	3.34%	0.390%
5	2.510	447	457	469	rVB2	7124	12908	1.50%	0.175%
6	3.690	806	824	846	rBV2	18152	51784	6.01%	0.701%
7	3.902	879	890	939	rBV2	90964	350169	40.62%	4.740%
8	4.355	1014	1031	1059	rBV2	142460	403023	46.75%	5.455%
9	5.050	1232	1247	1288	rBV3	323838	806943	93.60%	10.922%
10	5.619	1412	1424	1457	rBV	264822	543443	63.04%	7.356%
11	6.072	1550	1565	1591	rBV	181562	385121	44.67%	5.213%
12	6.583	1716	1724	1738	rVB3	18860	36393	4.22%	0.493%
13	6.992	1840	1851	1870	rBV	92471	170837	19.82%	2.312%
14	7.320	1934	1953	1970	rBV	399414	694491	80.56%	9.400%
15	7.397	1970	1977	1991	rVB	15020	29574	3.43%	0.400%
16	7.628	2039	2049	2072	rBV	53718	99222	11.51%	1.343%
17	7.943	2132	2147	2161	rVB2	13734	27346	3.17%	0.370%
18	8.091	2182	2193	2231	rBV	477187	862116	100.00%	11.669%
19	8.853	2419	2430	2460	rBV	385735	643673	74.66%	8.712%
20	10.217	2843	2854	2869	rBV	149430	238767	27.70%	3.232%
21	10.384	2893	2906	2918	rBV2	27100	46783	5.43%	0.633%
22	11.249	3164	3175	3197	rBV	440075	683786	79.31%	9.255%
23	11.532	3255	3263	3279	rBV4	9592	20158	2.34%	0.273%
24	11.625	3280	3292	3309	rVV	410767	647366	75.09%	8.762%
25	12.252	3478	3487	3501	rVB2	9474	16045	1.86%	0.217%
26	12.352	3506	3518	3530	rVV7	6217	11625	1.35%	0.157%
27	13.754	3945	3954	3964	rVB5	6227	9232	1.07%	0.125%




Sum of corrected areas: 7387947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021396.D
Acq On : 25 May 2021 18:25
Operator : SY/MD
Sample : M2496-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

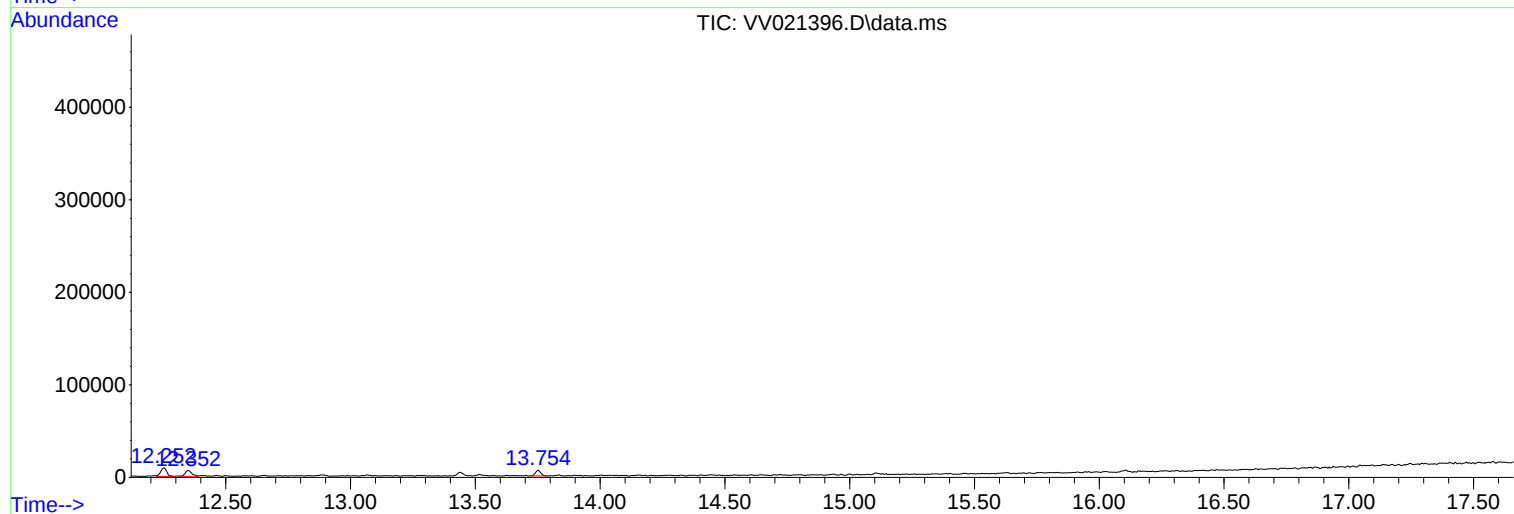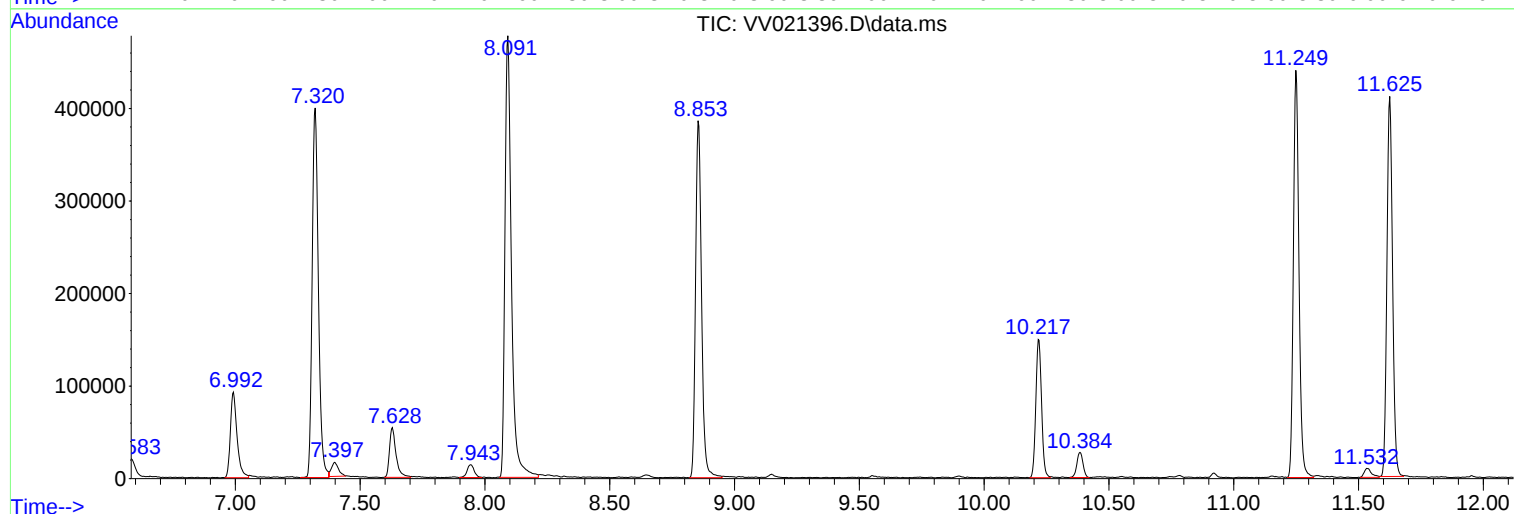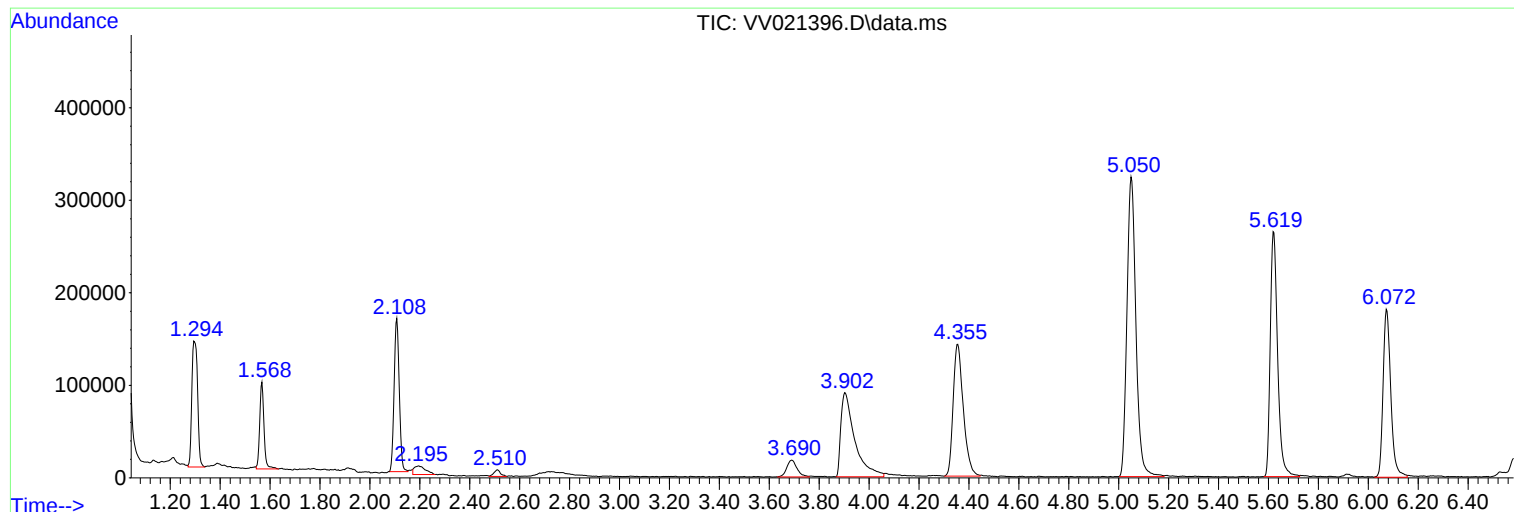

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021396.D
Acq On : 25 May 2021 18:25
Operator : SY/MD
Sample : M2496-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021396.D
Acq On : 25 May 2021 18:25
Operator : SY/MD
Sample : M2496-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB459

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
