

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021401.D
 Acq On : 25 May 2021 20:25
 Operator : SY/MD
 Sample : M2496-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB436

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	100982	101501	10.39%	1.418%
2	1.568	156	164	176	rBV	90598	104596	10.71%	1.462%
3	2.108	321	332	347	rBV2	163039	243206	24.90%	3.398%
4	3.908	880	892	949	rBV	89709	393538	40.29%	5.499%
5	4.352	1014	1030	1053	rBV2	134268	337298	34.53%	4.713%
6	5.050	1231	1247	1277	rBV2	322337	803938	82.31%	11.234%
7	5.619	1412	1424	1455	rBV	261370	531937	54.46%	7.433%
8	6.072	1552	1565	1591	rBV	186123	386524	39.57%	5.401%
9	6.992	1841	1851	1874	rBV	92572	174339	17.85%	2.436%
10	7.320	1941	1953	1971	rBV	393332	694045	71.05%	9.698%
11	7.397	1975	1977	1991	rVB4	6830	10706	1.10%	0.150%
12	7.628	2037	2049	2072	rBV	56432	105888	10.84%	1.480%
13	7.947	2137	2148	2153	rBV2	7606	12819	1.31%	0.179%
14	7.985	2153	2160	2172	rVB6	5935	10530	1.08%	0.147%
15	8.091	2183	2193	2226	rBV	537240	976775	100.00%	13.649%
16	8.854	2417	2430	2456	rBV	382563	644192	65.95%	9.002%
17	10.220	2839	2855	2877	rBV	166889	266903	27.32%	3.730%
18	10.384	2895	2906	2917	rBV3	10516	17711	1.81%	0.247%
19	11.249	3163	3175	3193	rBV	427883	675809	69.19%	9.444%
20	11.625	3280	3292	3310	rBV	418946	664038	67.98%	9.279%




Sum of corrected areas: 7156293

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021401.D
Acq On : 25 May 2021 20:25
Operator : SY/MD
Sample : M2496-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB436

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

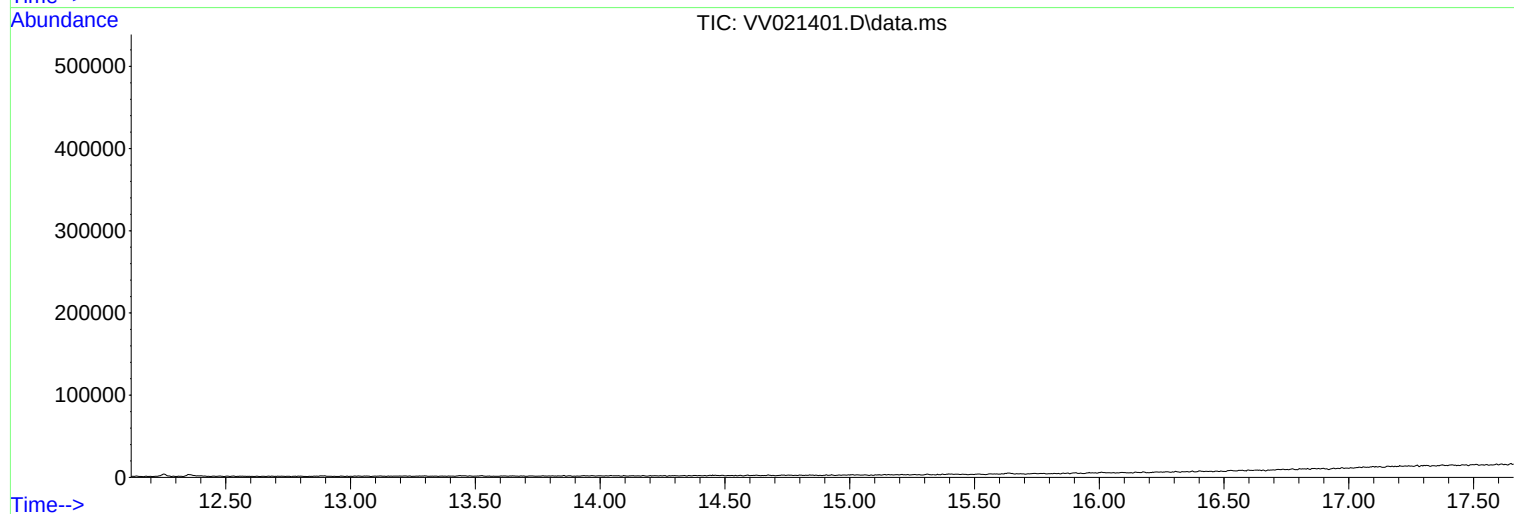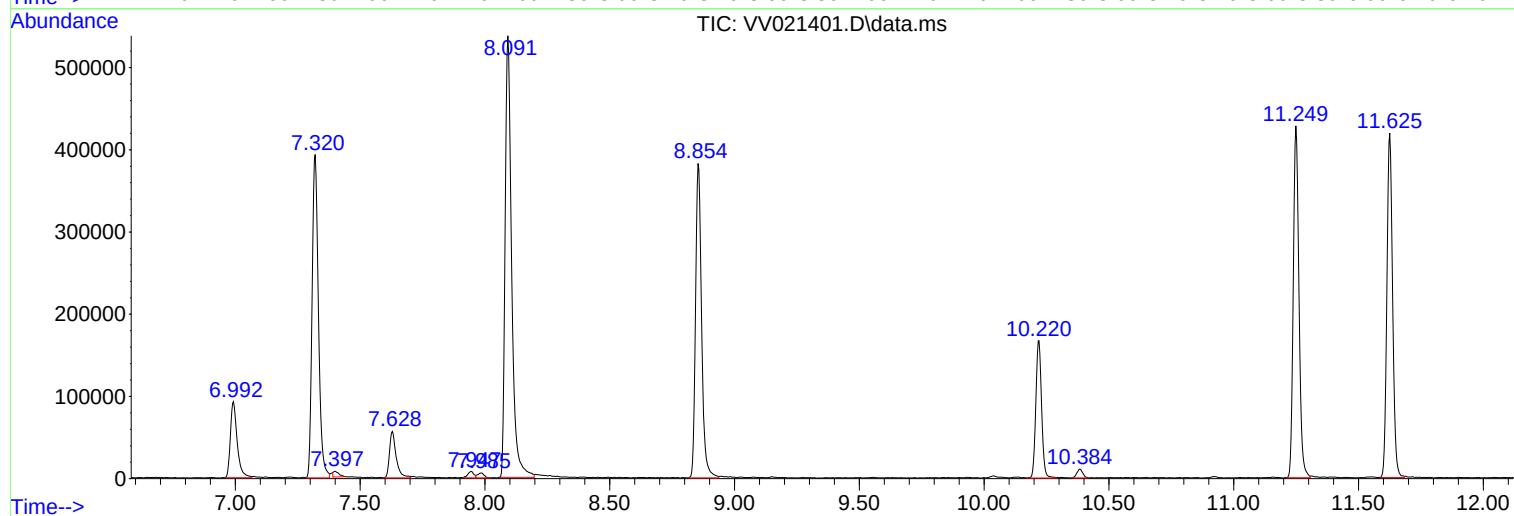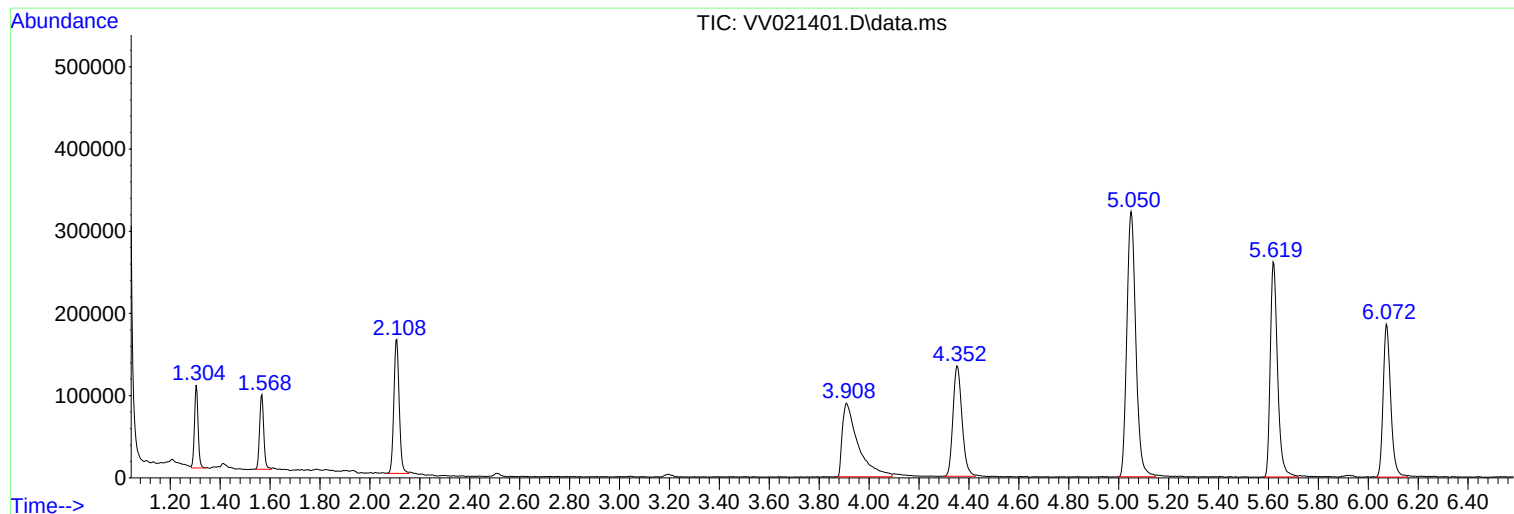

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021401.D
Acq On : 25 May 2021 20:25
Operator : SY/MD
Sample : M2496-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB436

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021401.D
Acq On : 25 May 2021 20:25
Operator : SY/MD
Sample : M2496-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB436

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
