

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021403.D
 Acq On : 25 May 2021 21:13
 Operator : SY/MD
 Sample : M2496-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB439

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV021403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	97812	95116	9.51%	1.272%
2	1.564	156	163	175	rVB	88293	97430	9.74%	1.303%
3	2.108	320	332	347	rBV2	200778	336588	33.65%	4.500%
4	3.198	658	671	686	rBV	11033	23397	2.34%	0.313%
5	3.915	877	894	955	rBV2	78243	407134	40.70%	5.444%
6	4.352	1013	1030	1055	rBV2	135040	339250	33.91%	4.536%
7	4.613	1098	1111	1127	rVB2	11115	26903	2.69%	0.360%
8	5.050	1231	1247	1279	rBV2	322346	806181	80.59%	10.779%
9	5.619	1410	1424	1458	rBV	262596	541828	54.16%	7.244%
10	6.072	1552	1565	1588	rBV	182540	382542	38.24%	5.115%
11	6.992	1840	1851	1877	rBV	91783	174026	17.40%	2.327%
12	7.320	1939	1953	1971	rBV	390043	685500	68.53%	9.165%
13	7.397	1972	1977	1994	rVB3	7953	16408	1.64%	0.219%
14	7.628	2039	2049	2075	rBV	55131	103744	10.37%	1.387%
15	7.979	2139	2158	2172	rBV2	103289	183718	18.37%	2.456%
16	8.091	2183	2193	2227	rBV	532044	1000354	100.00%	13.375%
17	8.854	2418	2430	2453	rBV	387882	638655	63.84%	8.539%
18	10.217	2843	2854	2872	rBV	167891	266486	26.64%	3.563%
19	10.384	2897	2906	2917	rVB2	9528	15244	1.52%	0.204%
20	11.249	3164	3175	3198	rBV	435200	680697	68.05%	9.101%
21	11.625	3277	3292	3314	rBV	418849	657967	65.77%	8.797%




Sum of corrected areas: 7479168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021403.D
Acq On : 25 May 2021 21:13
Operator : SY/MD
Sample : M2496-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB439

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

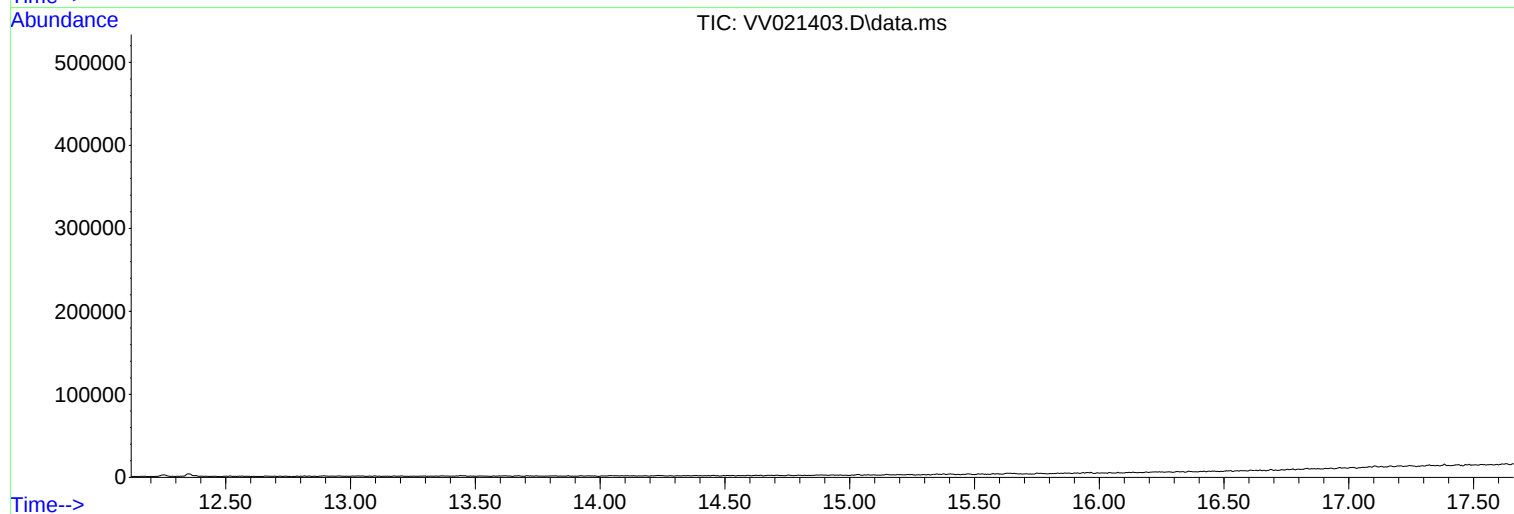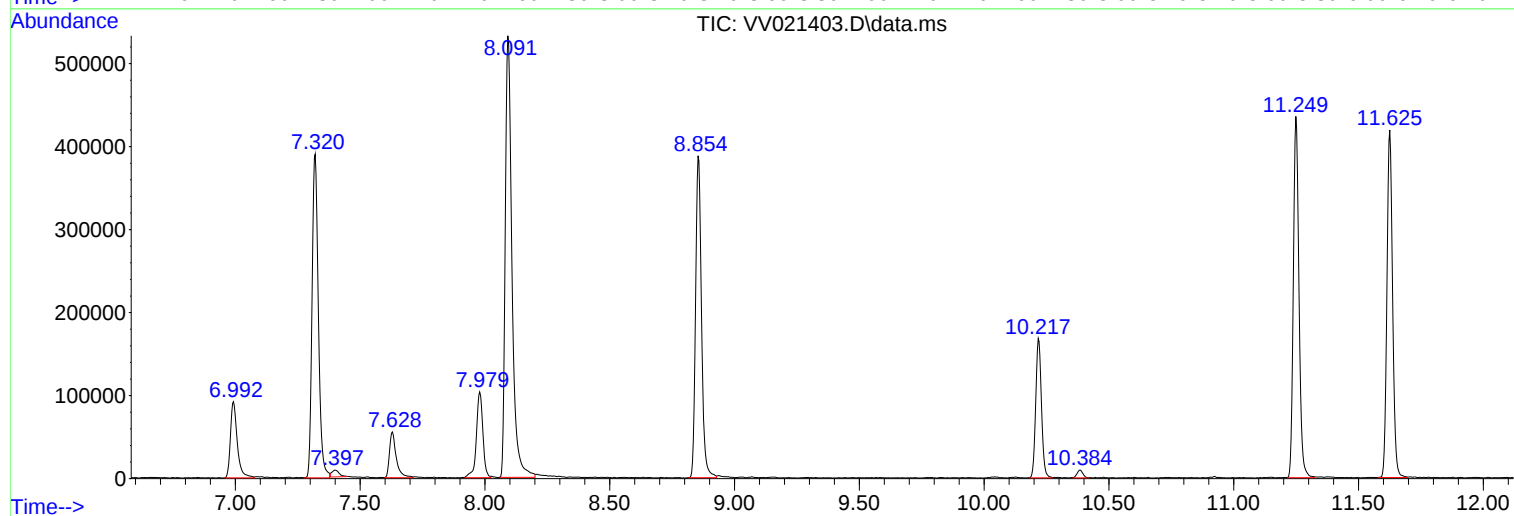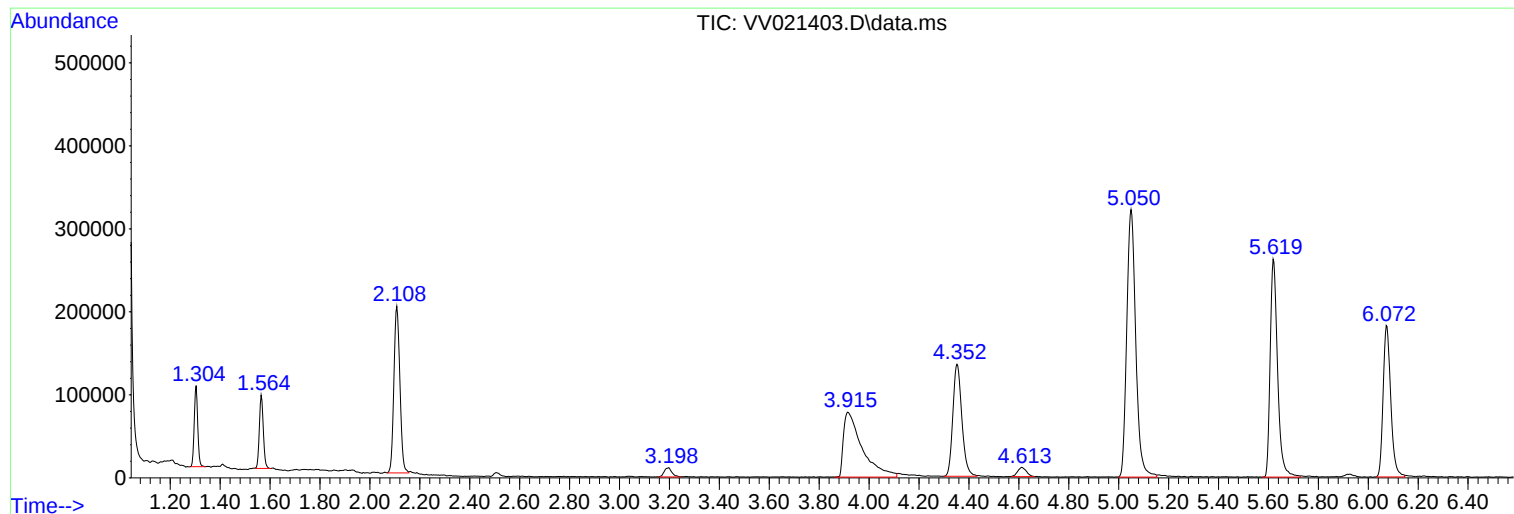

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021403.D
Acq On : 25 May 2021 21:13
Operator : SY/MD
Sample : M2496-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB439

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
Data File : VV021403.D
Acq On : 25 May 2021 21:13
Operator : SY/MD
Sample : M2496-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB439

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
