
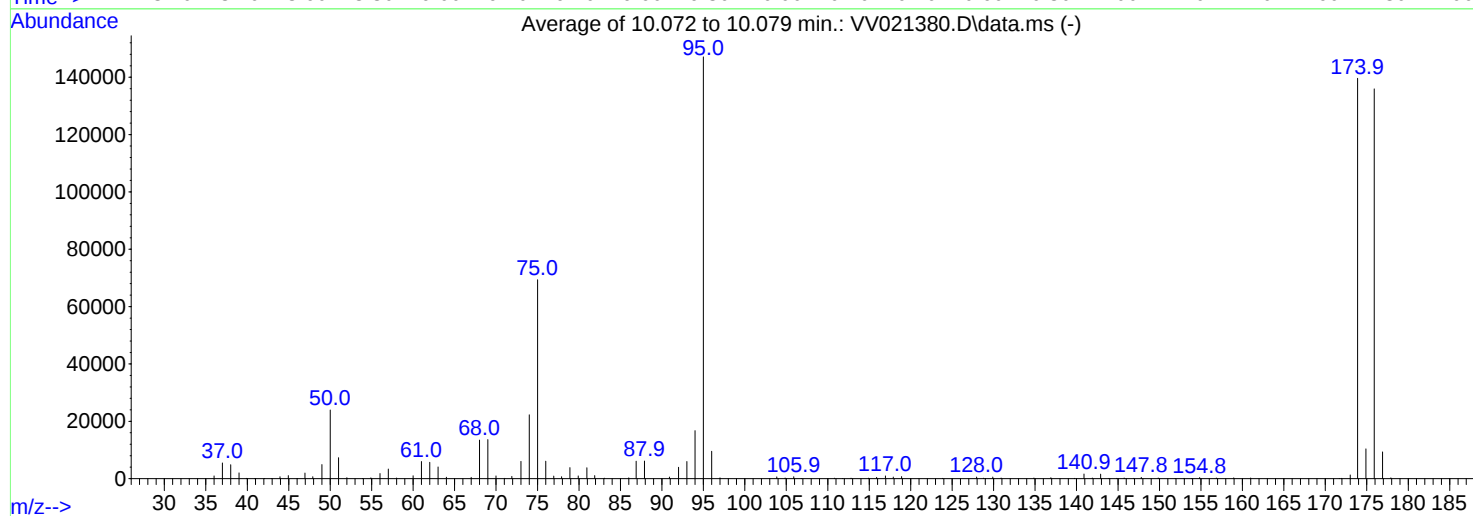


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052521\
 Data File : VV021380.D
 Acq On : 25 May 2021 09:35
 Operator : SY/MD
 Sample : BFB61
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB161

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 26 07:52:48 2021

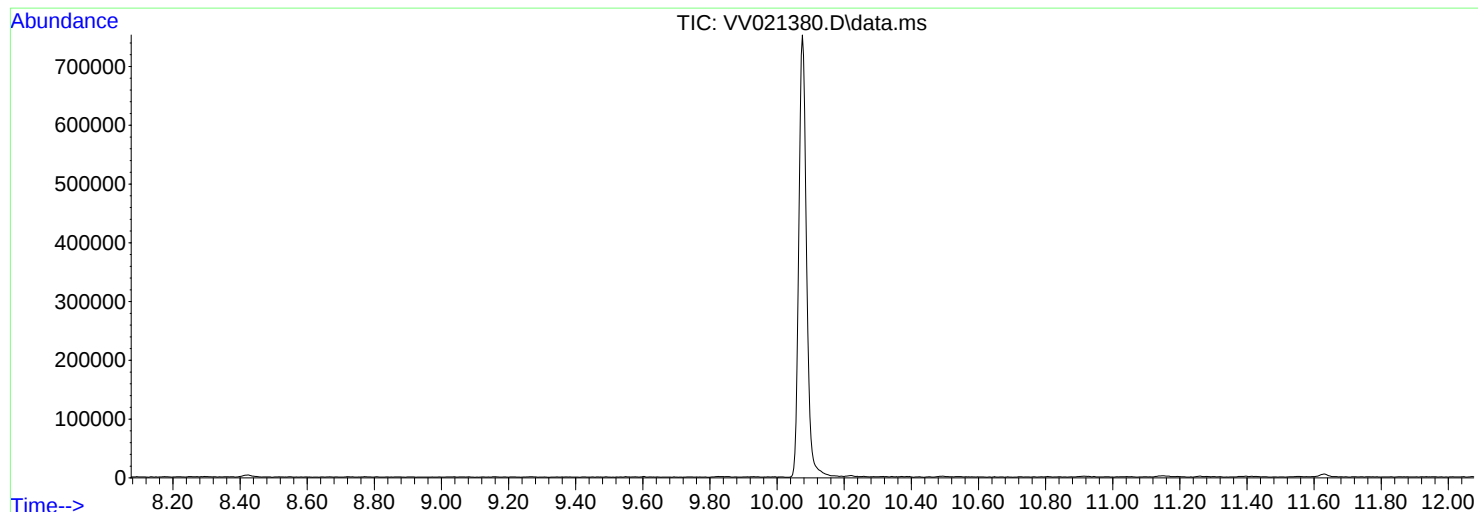

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	23941	PASS
75	95	30	80	47.2	69371	PASS
95	95	100	100	100.0	147115	PASS
96	95	5	9	6.5	9526	PASS
173	174	0.00	2	0.9	1276	PASS
174	95	50	120	94.9	139605	PASS
175	174	5	9	7.4	10368	PASS
176	174	95	105	97.4	135936	PASS
177	176	5	10	6.8	9298	PASS

m/z	Abundance
36.00	1030.0
37.00	5441.0
38.00	5047.0
39.00	2130.0
39.90	302.0
41.00	141.0
42.10	133.0
42.90	210.0
44.00	1224.0
45.00	1061.0
47.00	2138.0
47.90	622.0
49.00	4967.0
50.00	23944.0
51.00	7478.0
52.00	359.0
54.90	418.0
56.00	1834.0
57.00	3326.0
58.00	208.0
60.00	983.0
61.00	6190.0
62.00	5654.0
63.00	4121.0
64.00	505.0
67.00	497.0
68.00	13458.0
69.00	13629.0
70.00	945.0
71.10	131.0
71.90	825.0
73.00	6248.0
74.00	22256.0
75.00	69304.0
76.00	6143.0
77.00	925.0
77.90	659.0
78.90	3968.0
79.90	1009.0
80.90	3839.0
81.90	1014.0
83.00	201.0
86.00	200.0
86.90	6073.0
87.90	6058.0
90.90	567.0
92.00	3934.0
93.00	5893.0
94.00	16504.0
95.00	145792.0
96.00	9424.0
97.00	235.0
103.90	667.0
104.90	254.0
105.90	645.0
106.80	135.0
110.80	111.0
112.80	177.0
114.90	244.0
115.90	425.0
116.90	906.0
117.90	619.0
118.90	806.0
127.90	540.0
128.80	278.0
129.90	559.0
130.90	254.0
134.80	230.0
136.90	345.0
139.70	115.0
140.90	1548.0
141.90	214.0
142.90	1496.0
144.00	167.0
144.80	128.0
145.80	258.0
146.90	143.0
147.80	446.0
149.80	197.0
151.90	132.0
152.90	143.0
153.90	128.0
154.90	430.0
156.90	225.0
158.90	287.0
161.00	247.0
171.90	201.0
173.00	1204.0
173.90	134400.0
174.90	10058.0
175.90	131072.0
176.90	9068.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

177.90

275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
36.00	963.0
37.00	5679.0
38.00	5077.0
39.00	2101.0
39.90	299.0
40.90	132.0
42.10	106.0
42.90	207.0
44.00	1267.0
45.00	1115.0
47.00	2023.0
47.90	672.0
49.00	5048.0
50.00	24656.0
51.00	7466.0
52.00	374.0
55.00	415.0
56.00	1869.0
57.00	3451.0
58.00	234.0
60.00	1012.0
61.00	6136.0
62.00	5826.0
63.00	4175.0
64.00	493.0
67.00	441.0
68.00	14003.0
69.00	14084.0
70.00	974.0
71.10	147.0
71.90	826.0
73.00	6174.0
74.00	22904.0
75.00	71672.0
76.00	6300.0
77.00	936.0
77.90	685.0
78.90	4045.0
79.90	1008.0
80.90	3911.0
81.90	1123.0
83.00	169.0
86.00	278.0
86.90	6288.0
87.90	6304.0
90.90	565.0
92.00	4076.0
93.00	6150.0
94.00	17280.0
95.00	151744.0
96.00	9829.0
97.00	295.0
103.80	618.0
104.80	252.0
105.90	695.0
106.80	109.0
110.80	152.0
112.80	182.0
114.90	180.0
115.90	458.0
116.90	989.0
117.90	587.0
118.90	742.0
123.90	124.0
128.00	580.0
129.00	226.0
129.90	553.0
130.90	256.0
134.90	240.0
136.90	378.0
139.80	122.0
140.90	1651.0
141.90	232.0
142.90	1650.0
143.90	140.0
144.80	152.0
145.70	242.0
146.90	120.0
147.80	519.0
149.80	226.0
151.90	120.0
153.00	135.0
154.90	412.0
156.80	245.0
158.90	277.0
161.00	249.0
172.00	221.0
173.00	1319.0
173.90	144128.0
174.90	10714.0
175.90	140288.0
176.90	9647.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

177.90

303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
36.00	953.0
37.00	5319.0
38.00	4484.0
39.00	1887.0
39.90	298.0
40.90	138.0
42.90	180.0
44.00	1219.0
44.90	1059.0
46.00	102.0
46.90	1649.0
47.90	713.0
49.00	4753.0
50.00	23224.0
51.00	6921.0
52.00	325.0
53.90	104.0
55.00	418.0
56.00	1711.0
57.00	3221.0
58.00	230.0
60.00	973.0
61.00	5619.0
62.00	5669.0
63.00	3987.0
64.00	462.0
67.00	379.0
68.00	12923.0
69.00	13109.0
70.00	943.0
71.00	137.0
71.90	783.0
73.00	5618.0
74.00	21640.0
75.00	67136.0
76.00	5885.0
76.90	834.0
77.90	632.0
78.90	3619.0
79.90	928.0
81.00	3668.0
81.90	994.0
83.10	139.0
86.00	343.0
86.90	5868.0
87.90	6042.0
90.90	531.0
92.00	3863.0
93.00	5924.0
94.00	16472.0
95.00	143808.0
96.00	9324.0
97.00	319.0
103.90	577.0
104.80	231.0
105.90	676.0
110.80	176.0
111.80	123.0
112.80	140.0
114.80	133.0
115.90	450.0
117.00	1021.0
117.90	485.0
118.90	656.0
123.80	142.0
128.00	577.0
128.80	221.0
129.90	497.0
130.90	235.0
134.90	214.0
136.90	358.0
139.80	104.0
140.90	1620.0
141.90	232.0
142.90	1588.0
143.80	110.0
144.90	148.0
145.70	222.0
147.80	465.0
149.90	223.0
153.00	133.0
154.80	389.0
156.80	259.0
159.00	213.0
161.00	247.0
171.70	201.0
173.00	1305.0
173.90	140288.0
174.90	10333.0
175.90	136448.0
176.90	9178.0
177.90	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
39.90	206.0
40.90	132.0
43.10	144.0
43.90	561.0
54.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161